

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011819\
 Data File : FB019456.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jan 2019 8:53
 Operator : MJ/SJ
 Sample : BSF0118S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 18 21:47:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.040	177505	19.976 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.896	556933	27.963 ng/ml
2) t	2,2,4-Trimethylpentane	7.655	558978	29.343 ng/ml
3) t	n-Heptane	7.996	171316	9.819 ng/ml
4) t	Benzene	8.132	200420	10.207 ng/ml
6) t	Toluene	10.888	562136	31.076 ng/ml
7) t	Ethylbenzene	13.340	225996	10.200 ng/ml
8) t	m-Xylene	13.473	468054	20.396 ng/ml
9) t	O-Xylene	14.205	459060	20.460 ng/ml
10) t	1,2,4-Trimethylbenzene	16.491	463842	20.342 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011819\
Data File : FB019456.D
Signal(s) : FID2B.CH
Acq On : 18 Jan 2019 8:53
Operator : MJ/SJ
Sample : BSF0118S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 18 21:47:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

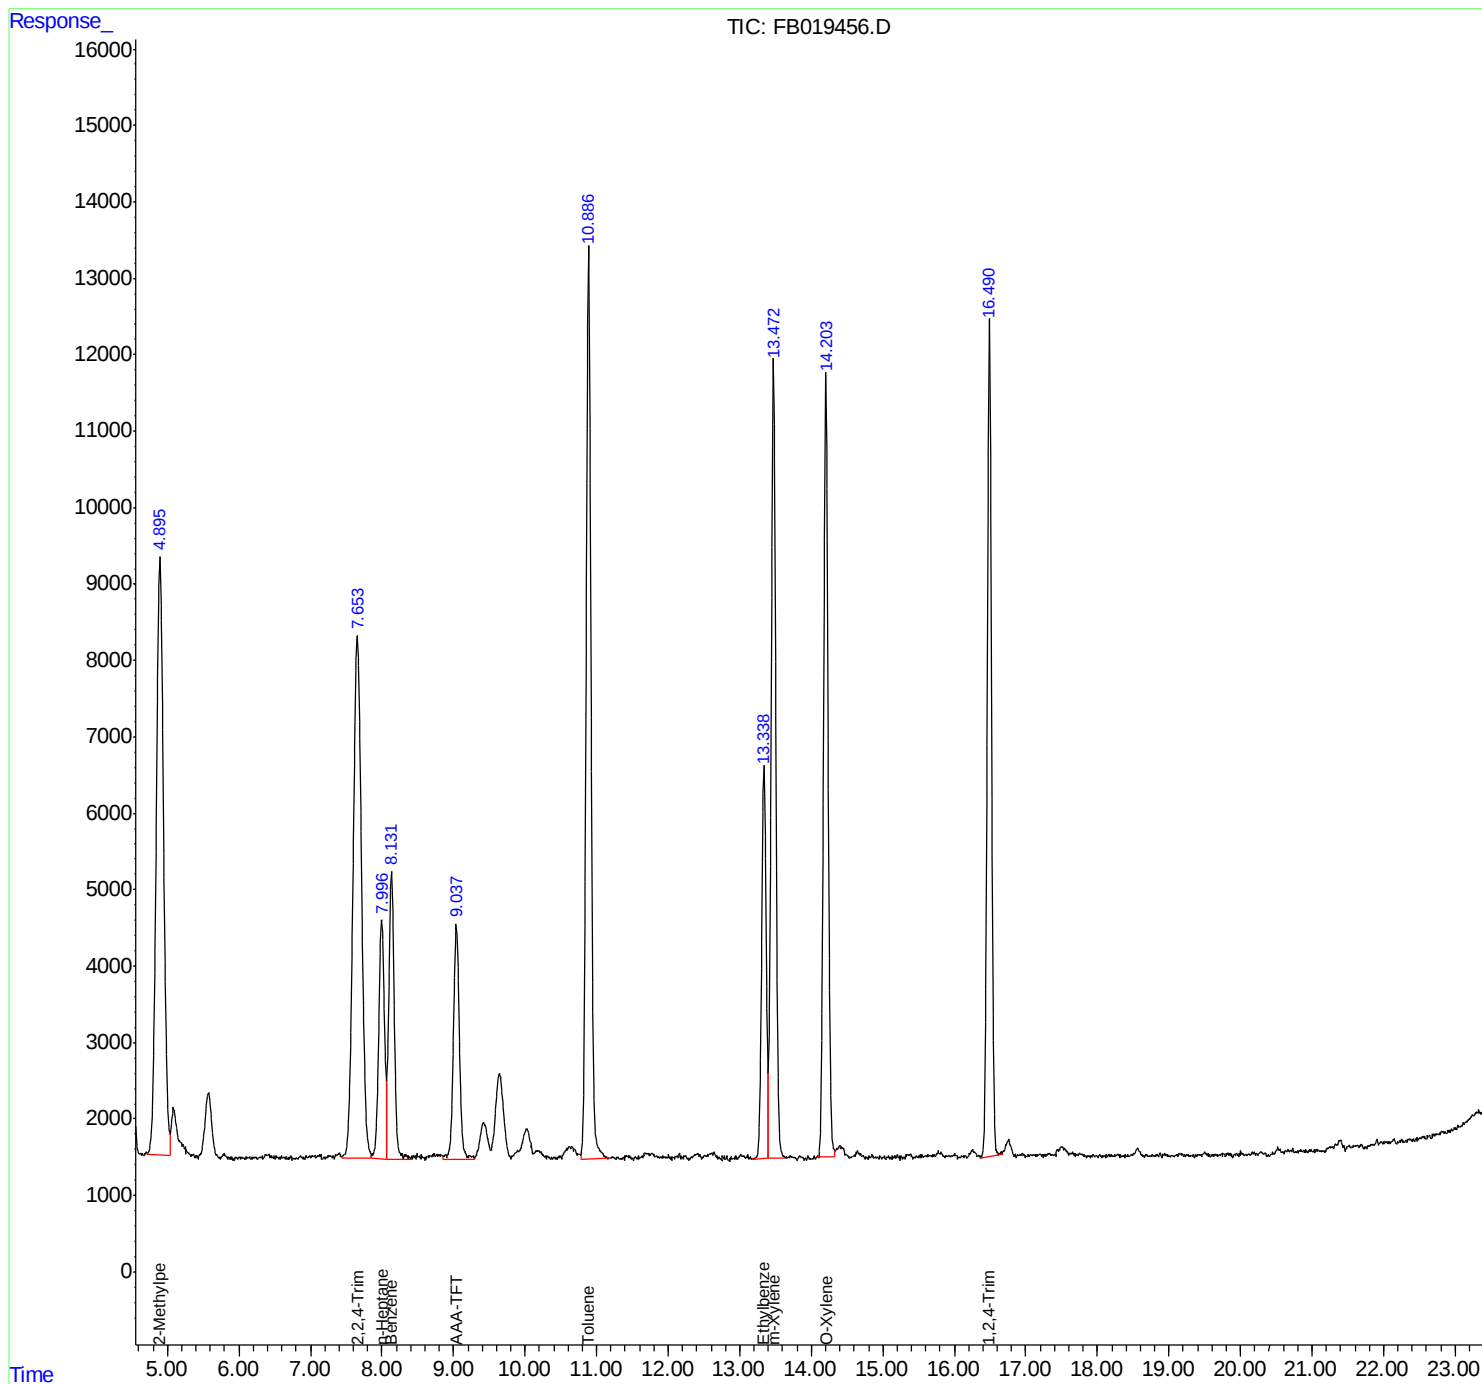

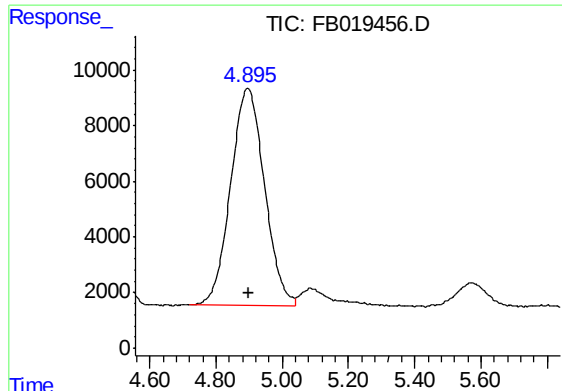


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 556933
Conc: 27.96 ng/ml

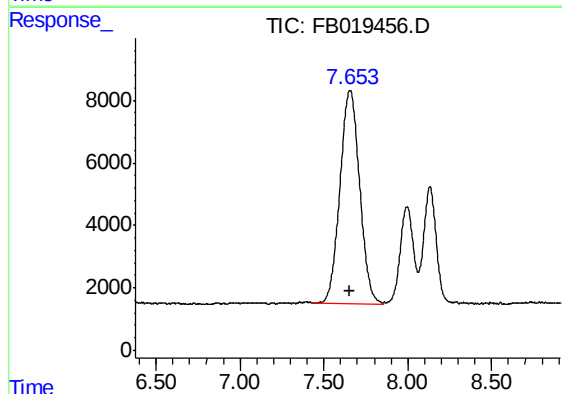


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.003 min
Response: 558978
Conc: 29.34 ng/ml

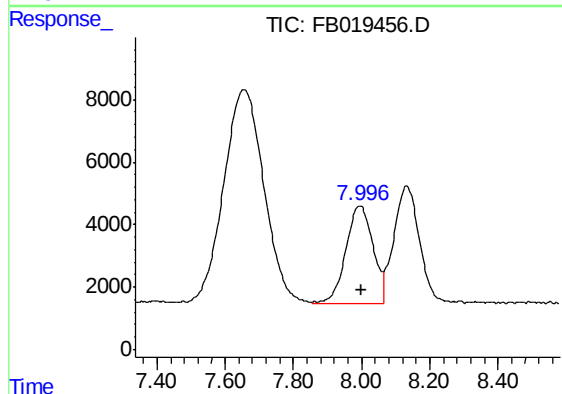


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.002 min
Response: 171316
Conc: 9.82 ng/ml

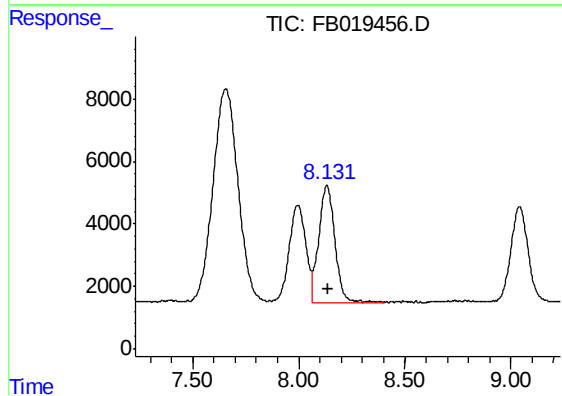


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.003 min
Response: 200420
Conc: 10.21 ng/ml

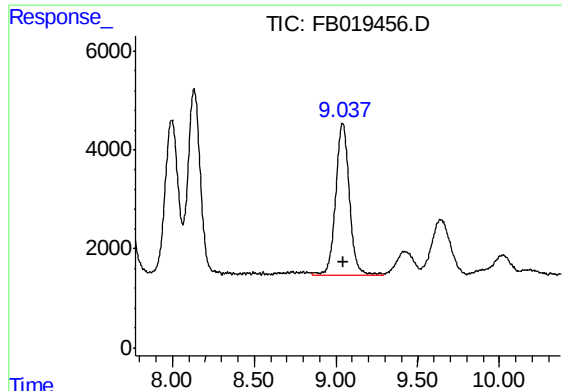


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.003 min
Response: 177505
Conc: 19.98 ng/ml

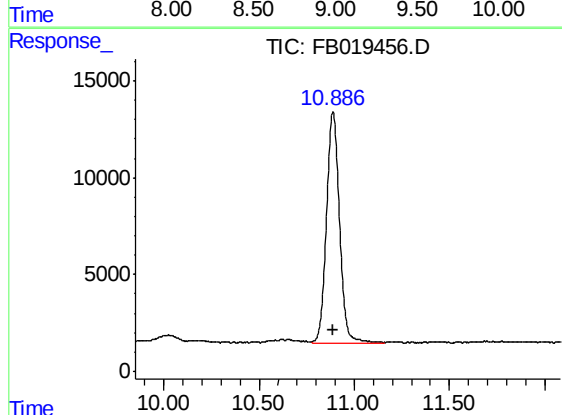


#6 Toluene

R.T.: 10.888 min
Delta R.T.: -0.003 min
Response: 562136
Conc: 31.08 ng/ml

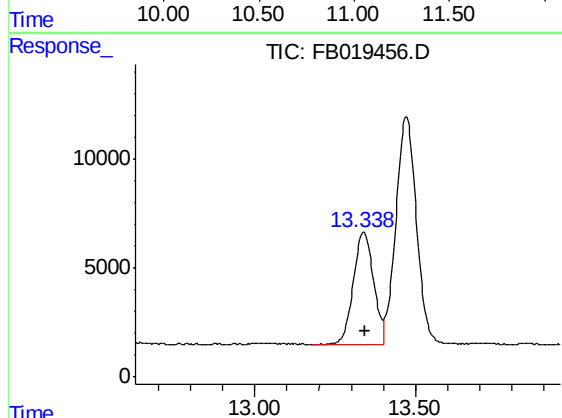


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.002 min
Response: 225996
Conc: 10.20 ng/ml

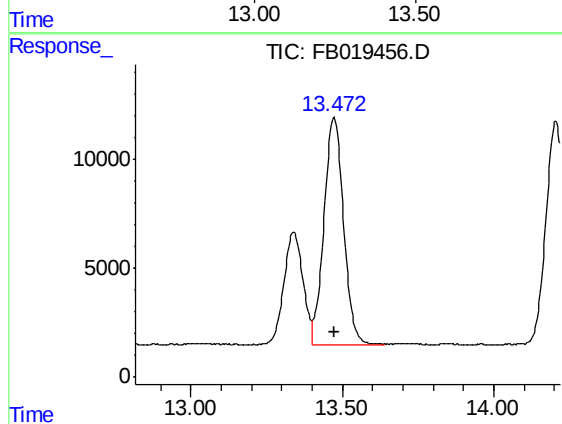


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.003 min
Response: 468054
Conc: 20.40 ng/ml

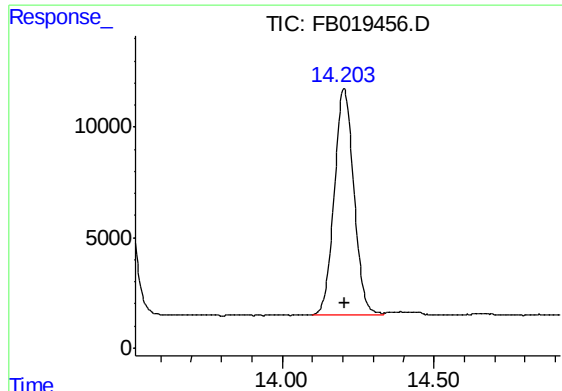

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: -0.003 min
Response: 459060
Conc: 20.46 ng/ml

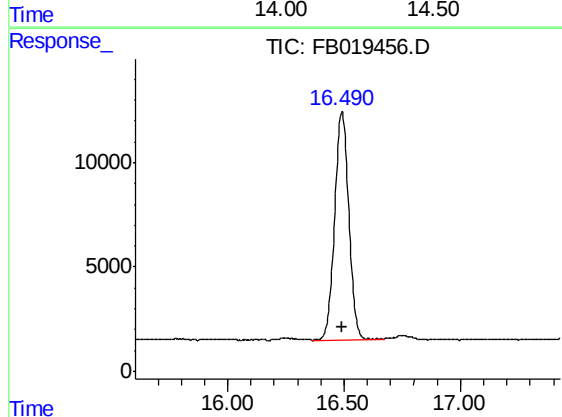

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: -0.003 min
Response: 463842
Conc: 20.34 ng/ml