

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011823\
 Data File : FB029124.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jan 2023 10:46
 Operator : AJ/MA
 Sample : BSF0118S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 18 23:23:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	281269	23.018 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	488221	33.347 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	561937	35.417 ng/ml
3) t n-Heptane	7.749	179973	10.771 ng/ml
4) t Benzene	7.886	215261	10.125 ng/ml
6) t Toluene	10.619	625050	31.011 ng/ml
7) t Ethylbenzene	13.055	198895	10.370 ng/ml
8) t m-Xylene	13.188	395574	21.143 ng/ml
9) t O-Xylene	13.915	386782	21.494 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	394086	22.105 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011823\
Data File : FB029124.D
Signal(s) : FID2B.CH
Acq On : 18 Jan 2023 10:46
Operator : AJ/MA
Sample : BSF0118S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 18 23:23:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

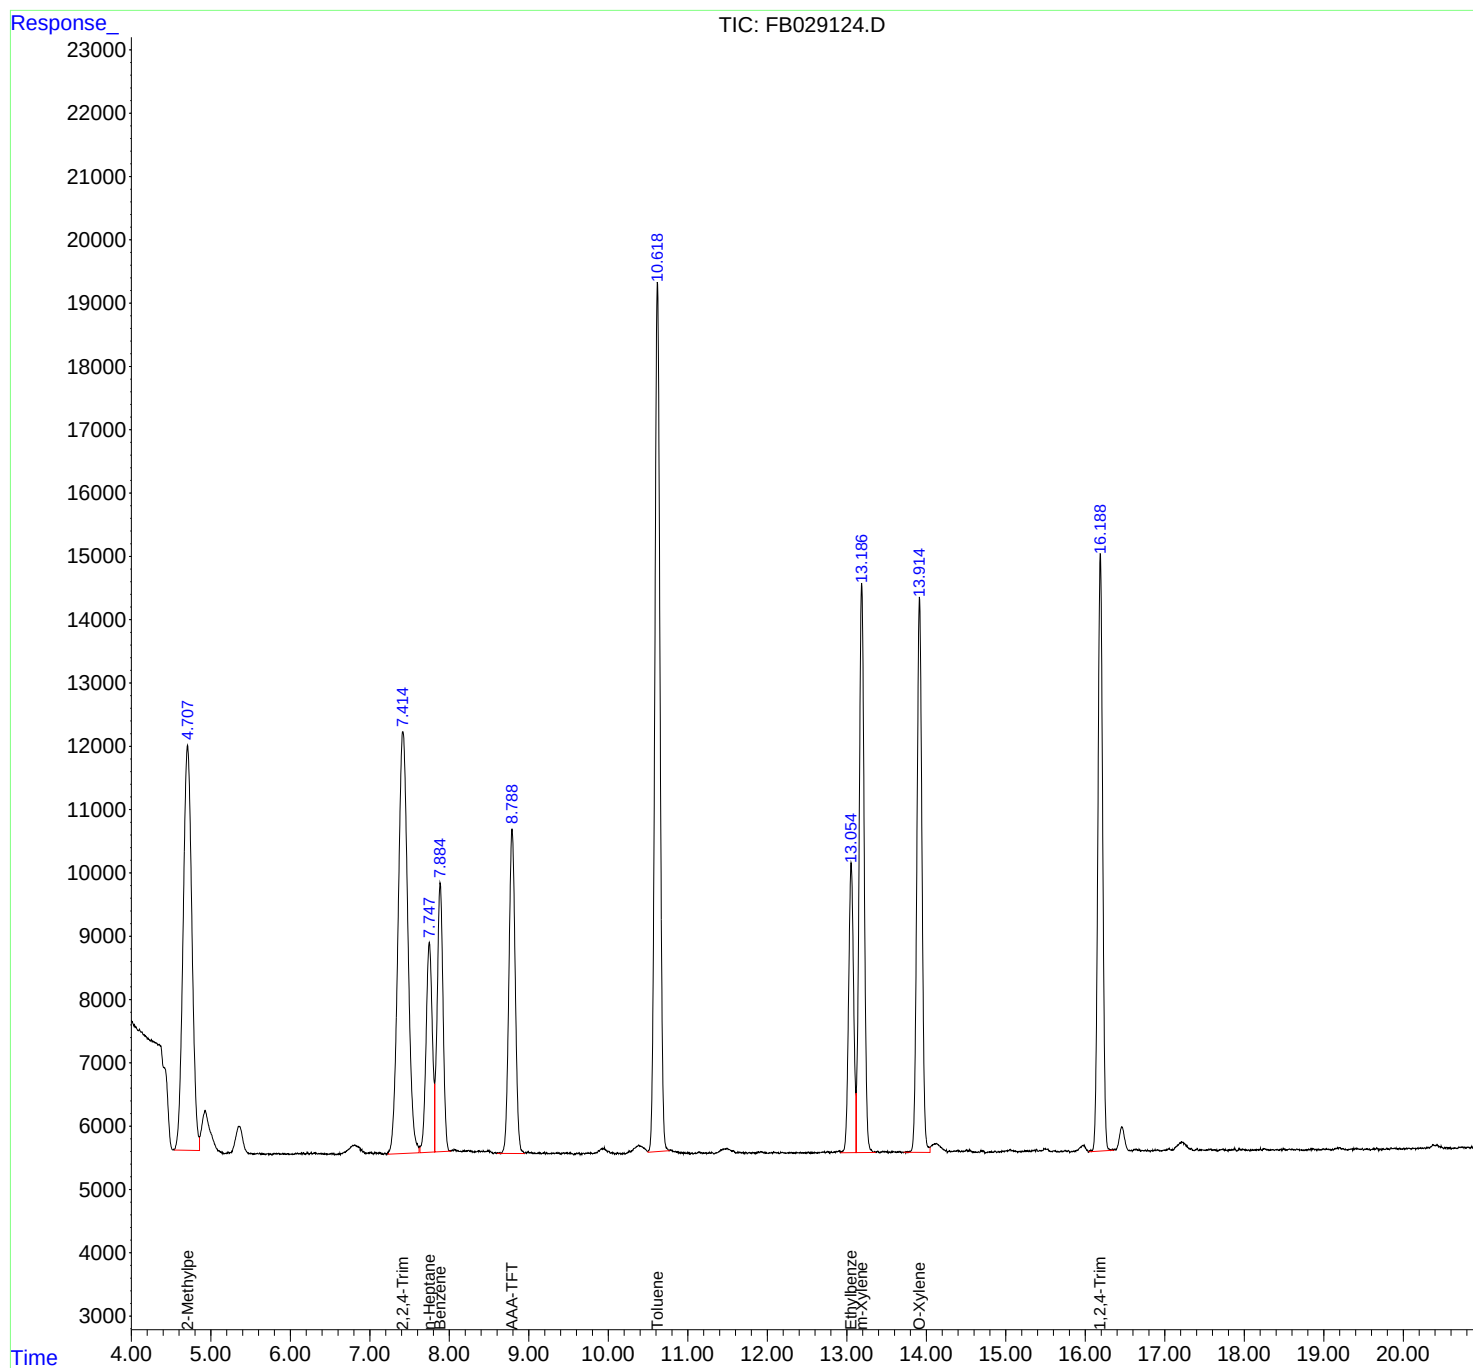

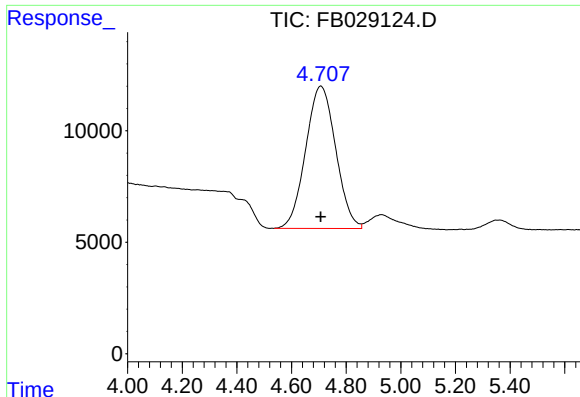


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.001 min
Response: 488221
Conc: 33.35 ng/ml

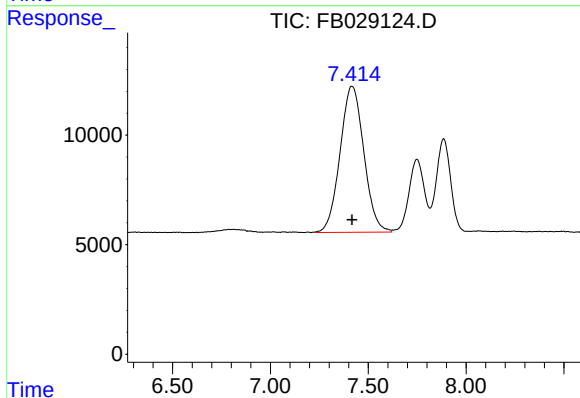


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 561937
Conc: 35.42 ng/ml

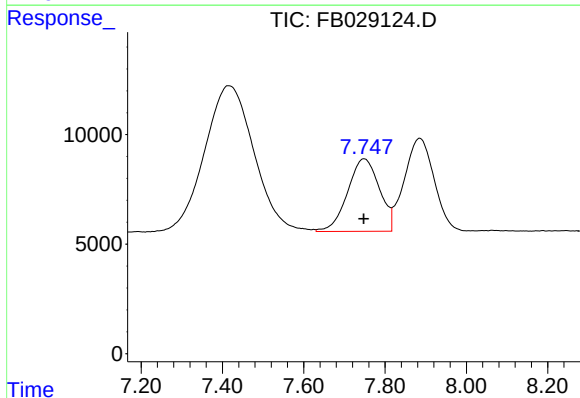


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.001 min
Response: 179973
Conc: 10.77 ng/ml

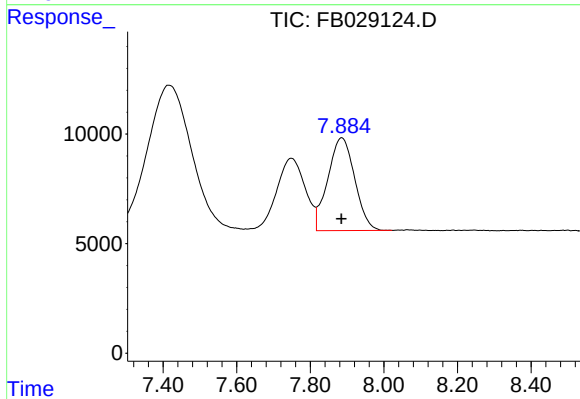


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 215261
Conc: 10.12 ng/ml

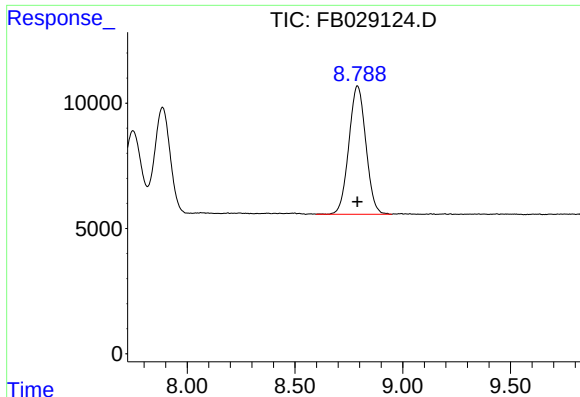


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 281269
Conc: 23.02 ng/ml

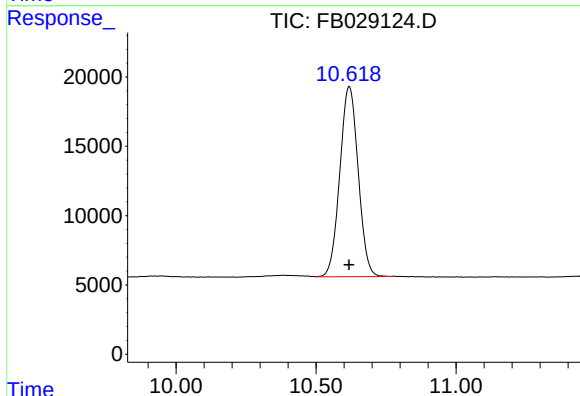


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.001 min
Response: 625050
Conc: 31.01 ng/ml

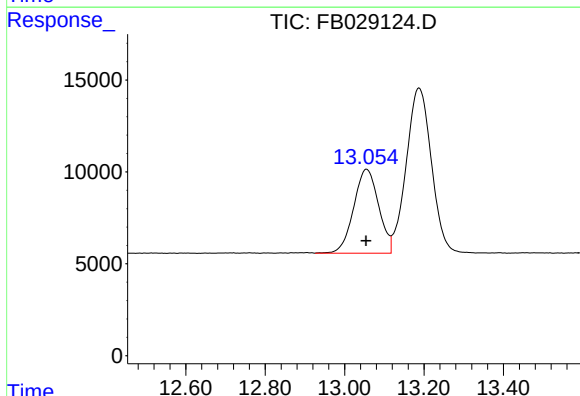


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.001 min
Response: 198895
Conc: 10.37 ng/ml

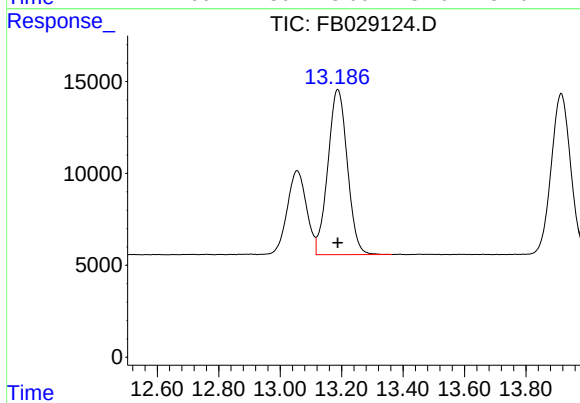

#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 395574
Conc: 21.14 ng/ml

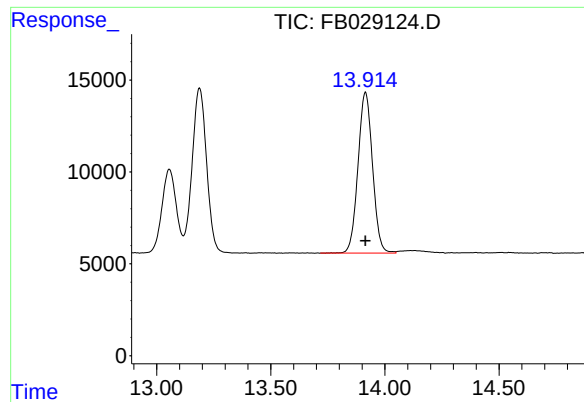


#9 O-Xylene

R.T.: 13.915 min

Delta R.T.: 0.000 min

Response: 386782

Conc: 21.49 ng/ml

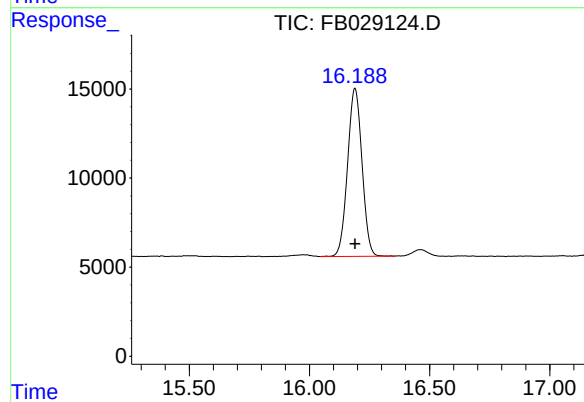

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min

Delta R.T.: 0.000 min

Response: 394086

Conc: 22.11 ng/ml