

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011922\
Data File : FB026599.D
Signal(s) : FID2B.CH
Acq On : 19 Jan 2022 14:05
Operator : AJ/MA
Sample : N1176-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 20 00:07:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
Quant Title :
QLast Update : Mon Jan 10 13:16:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	167885	16.255 ng/ml
Target Compounds			
6) t Toluene	10.623	8570	0.436 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011922\
Data File : FB026599.D
Signal(s) : FID2B.CH
Acq On : 19 Jan 2022 14:05
Operator : AJ/MA
Sample : N1176-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 20 00:07:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
Quant Title :
QLast Update : Mon Jan 10 13:16:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

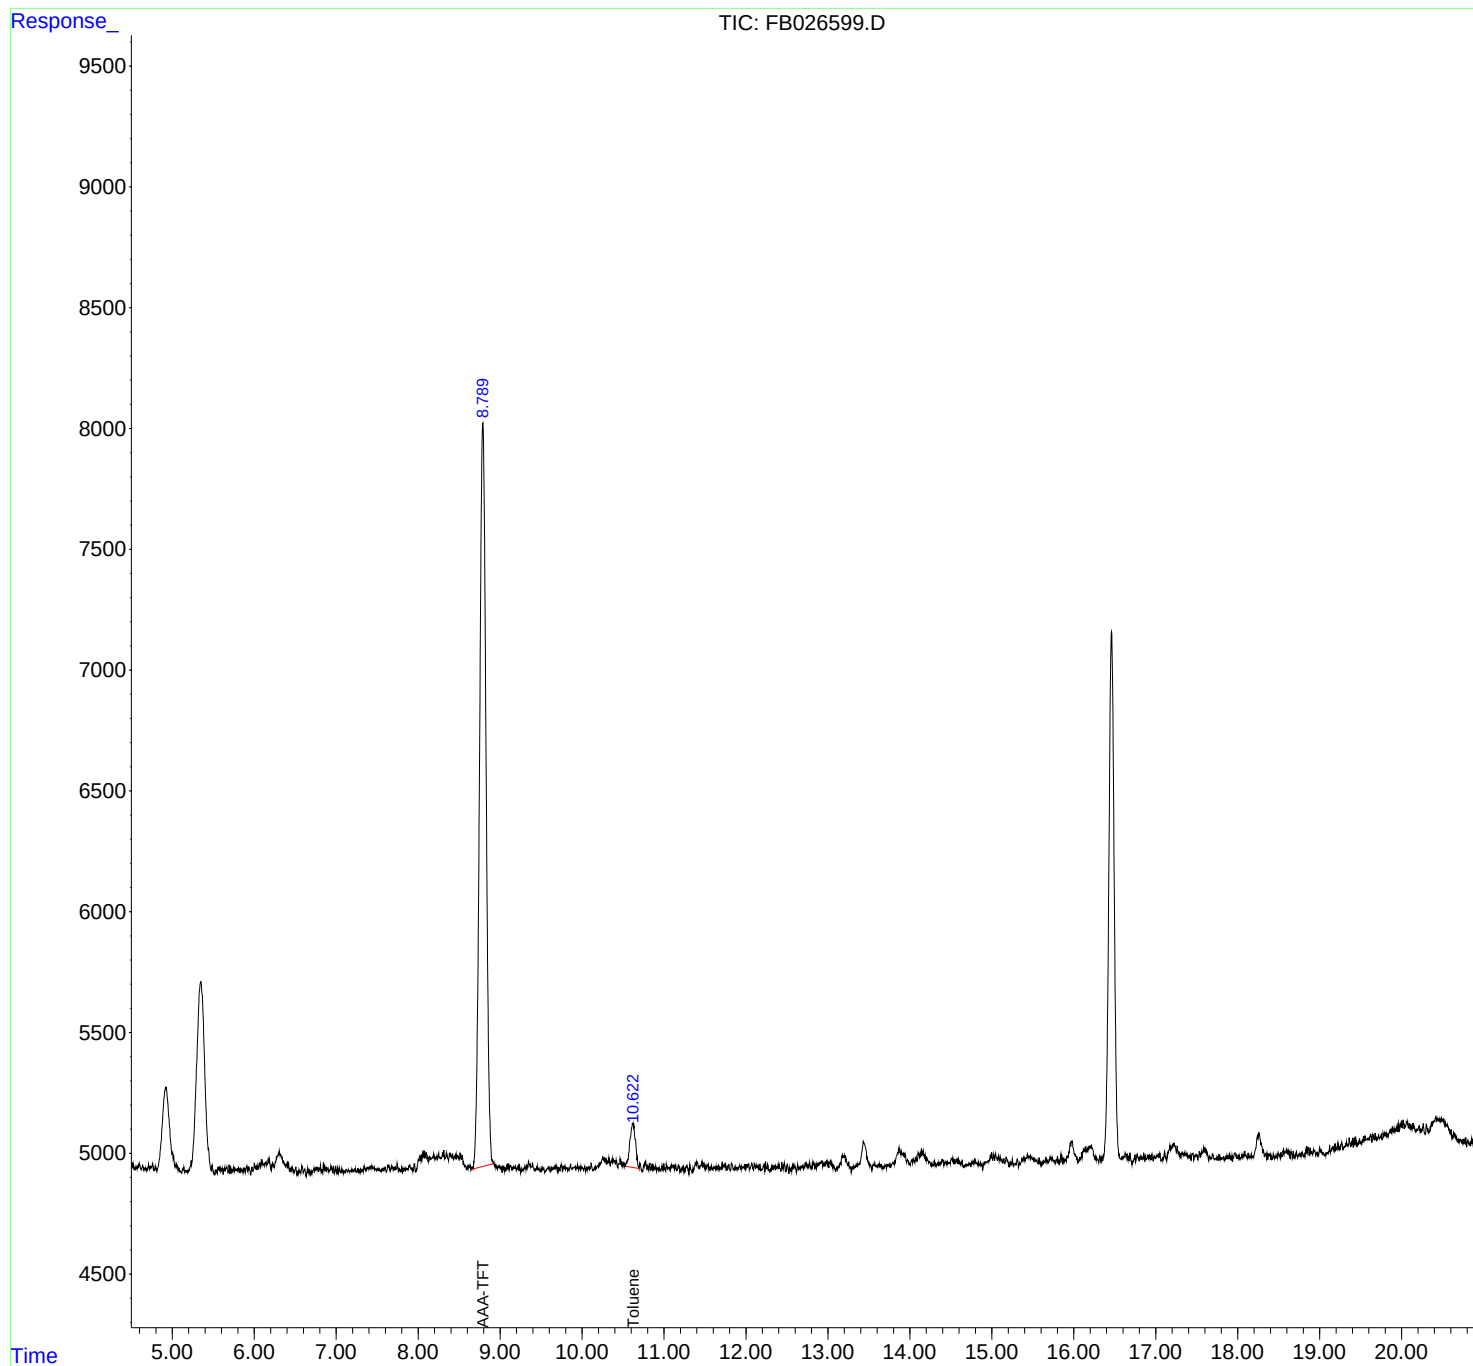


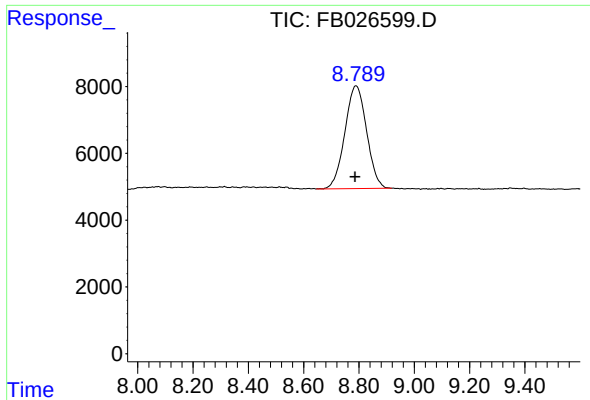

#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.004 min
Response: 167885
Conc: 16.26 ng/ml

Instrument :
FID_B
ClientSampleId :

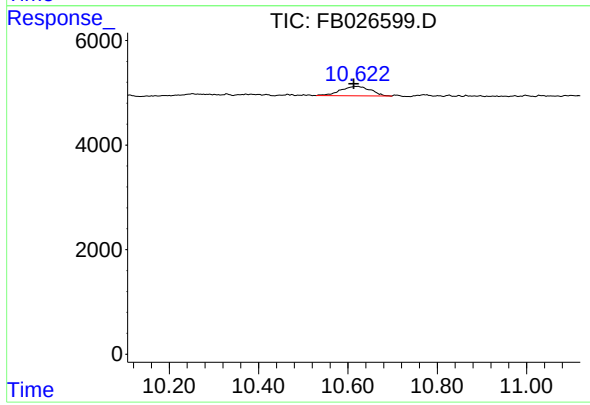

#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.010 min
Response: 8570
Conc: 0.44 ng/ml