

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011922\
 Data File : FB026600.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jan 2022 15:17
 Operator : AJ/MA
 Sample : N1176-01MS
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 20 00:07:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
 Quant Title :
 QLast Update : Mon Jan 10 13:16:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	199855	19.350 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	385217	24.735 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	457595	25.133 ng/ml
3) t n-Heptane	7.747	147033	8.299 ng/ml
4) t Benzene	7.885	179212	8.777 ng/ml
6) t Toluene	10.617	520092	26.484 ng/ml
7) t Ethylbenzene	13.054	160310	8.680 ng/ml
8) t m-Xylene	13.186	320534	17.392 ng/ml
9) t O-Xylene	13.914	311485	17.321 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	319654	17.311 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011922\
Data File : FB026600.D
Signal(s) : FID2B.CH
Acq On : 19 Jan 2022 15:17
Operator : AJ/MA
Sample : N1176-01MS
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 20 00:07:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
Quant Title :
QLast Update : Mon Jan 10 13:16:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

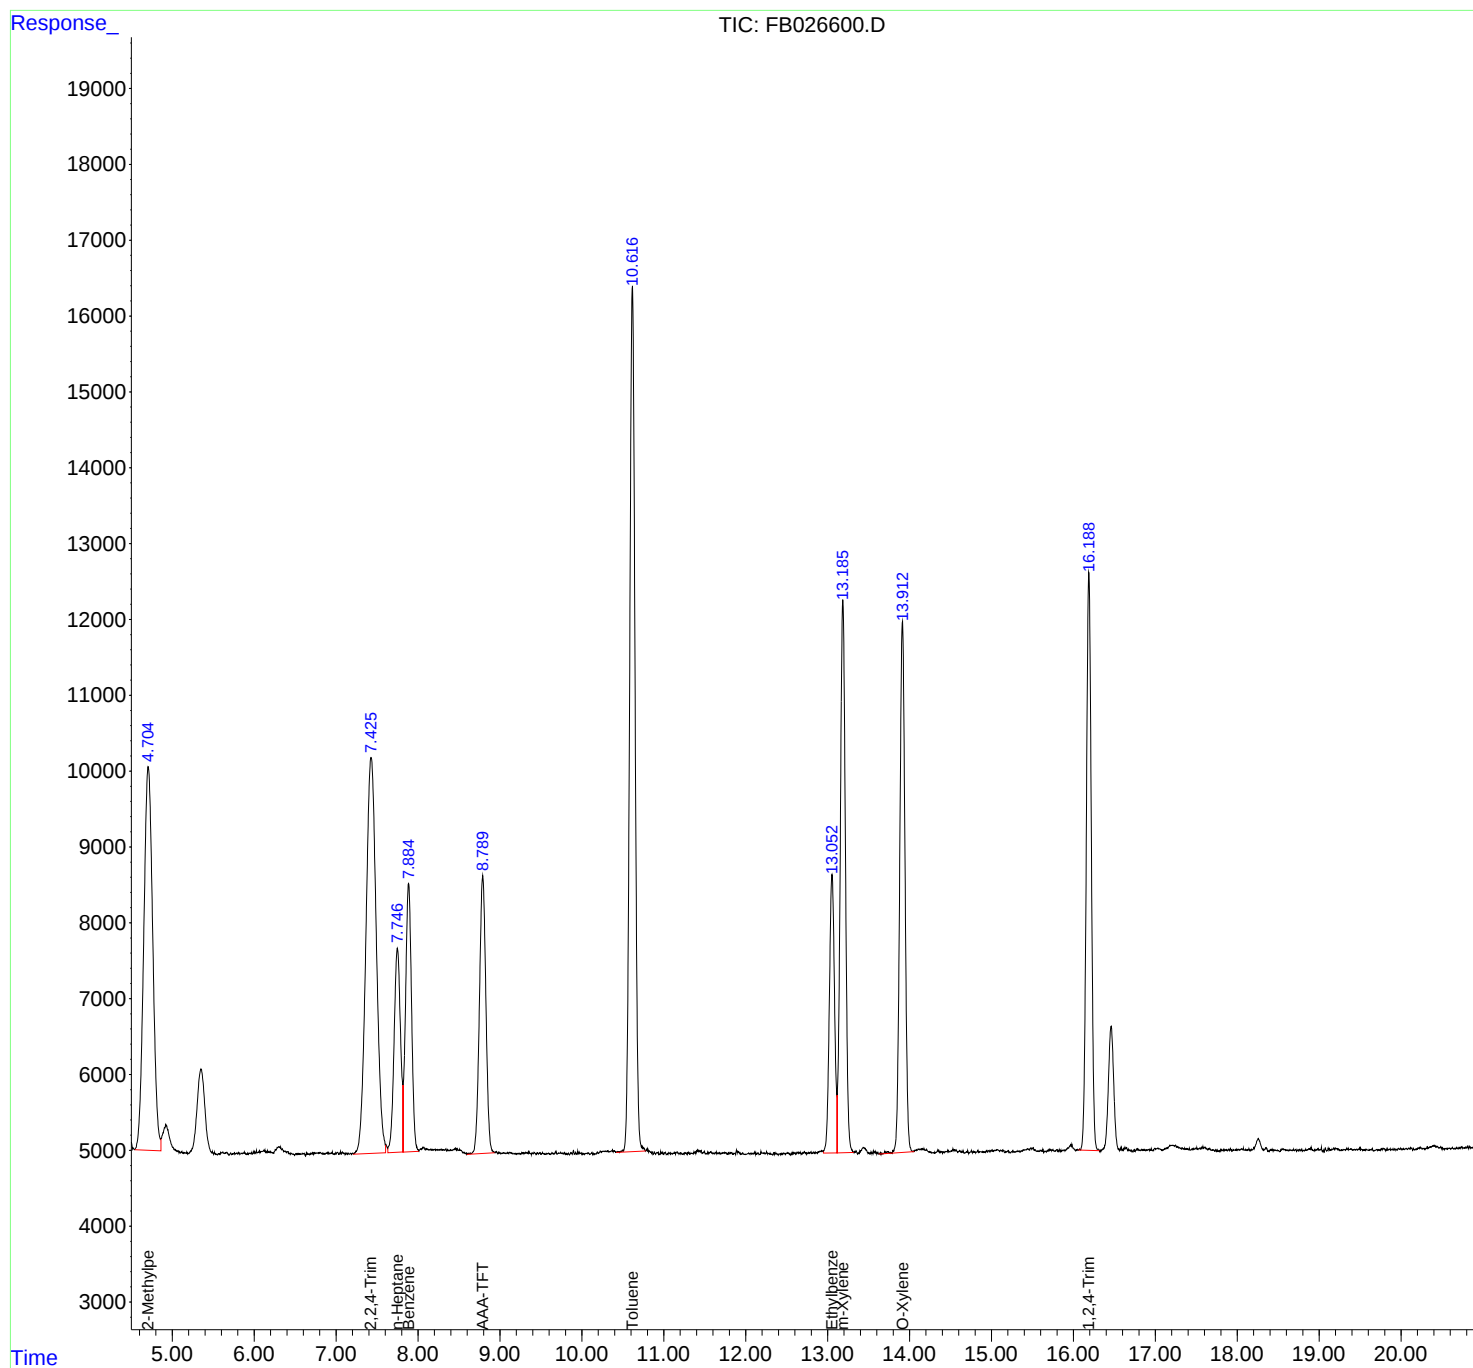


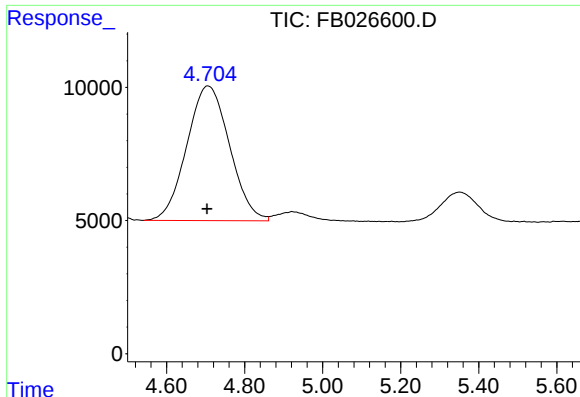

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.002 min
Response: 385217
Conc: 24.74 ng/ml

Instrument :
FID_B
ClientSampleId :

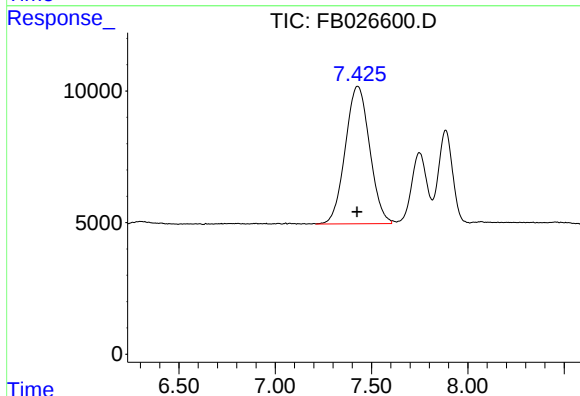


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.001 min
Response: 457595
Conc: 25.13 ng/ml

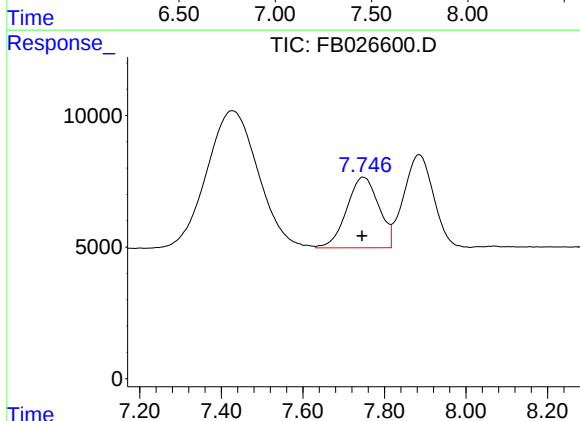


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.002 min
Response: 147033
Conc: 8.30 ng/ml

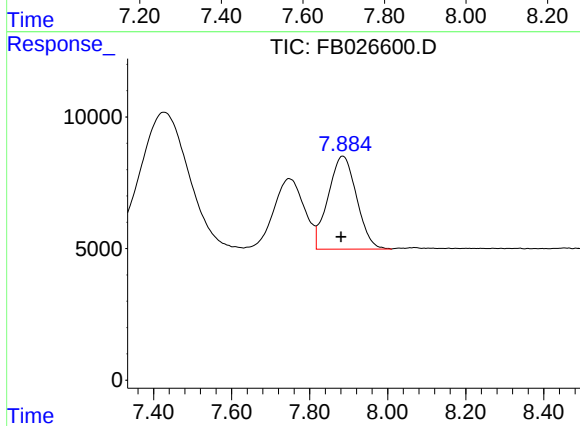

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.005 min
Response: 179212
Conc: 8.78 ng/ml

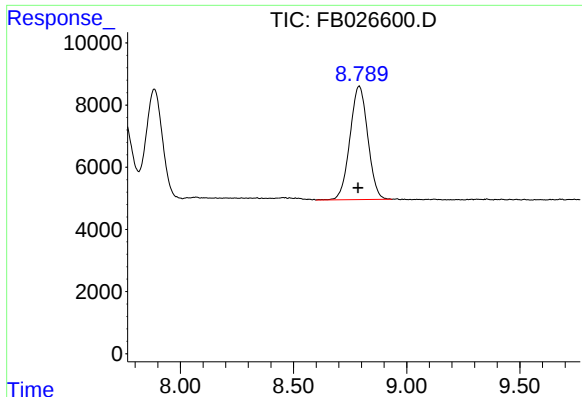

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.005 min
Response: 199855
Conc: 19.35 ng/ml

Instrument :
FID_B
ClientSampleId :

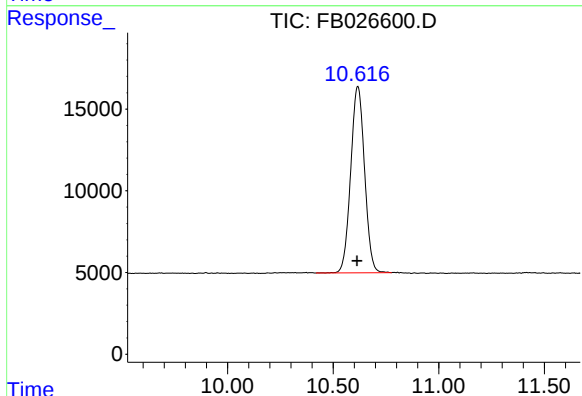


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.004 min
Response: 520092
Conc: 26.48 ng/ml

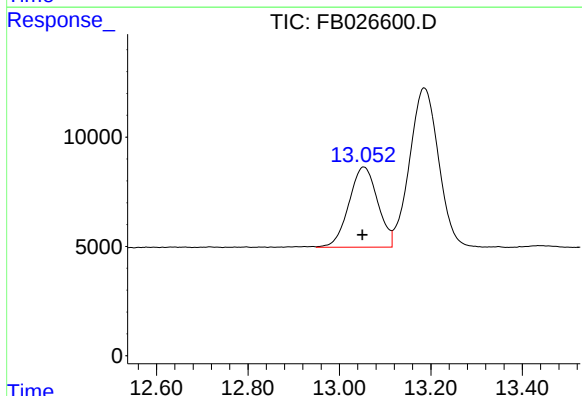


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.004 min
Response: 160310
Conc: 8.68 ng/ml

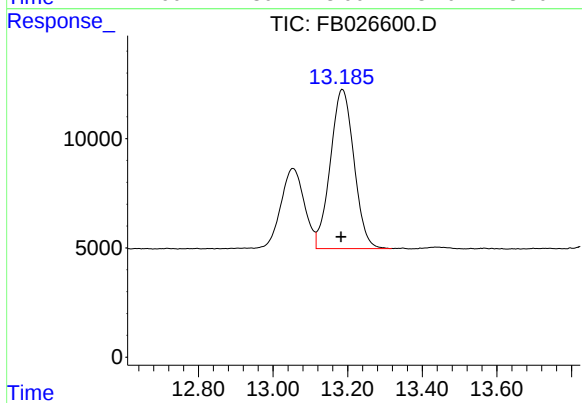

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.004 min
Response: 320534
Conc: 17.39 ng/ml

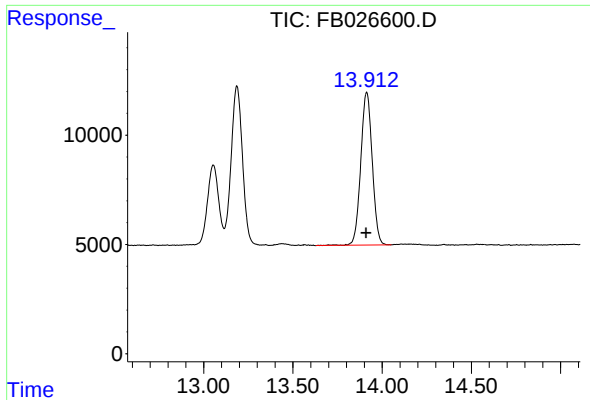

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.004 min
Response: 311485
Conc: 17.32 ng/ml

Instrument :
FID_B
ClientSampleId :

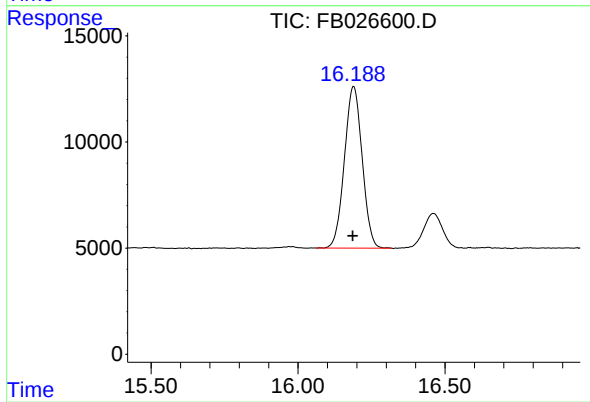

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.004 min
Response: 319654
Conc: 17.31 ng/ml