

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011922\
 Data File : FB026597.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jan 2022 12:37
 Operator : AJ/MA
 Sample : BSF0119S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0119S1

Integration File: SAMPLE.e
 Quant Time: Jan 20 00:06:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
 Quant Title :
 QLast Update : Mon Jan 10 13:16:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	198595	19.228 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	453248	29.104 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	526408	28.913 ng/ml
3) t n-Heptane	7.746	172791	9.752 ng/ml
4) t Benzene	7.882	200244	9.807 ng/ml
6) t Toluene	10.615	606065	30.862 ng/ml
7) t Ethylbenzene	13.053	183036	9.910 ng/ml
8) t m-Xylene	13.185	362556	19.672 ng/ml
9) t O-Xylene	13.912	348334	19.370 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	355618	19.259 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011922\
Data File : FB026597.D
Signal(s) : FID2B.CH
Acq On : 19 Jan 2022 12:37
Operator : AJ/MA
Sample : BSF0119S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0119S1

Integration File: SAMPLE.e
Quant Time: Jan 20 00:06:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
Quant Title :
QLast Update : Mon Jan 10 13:16:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

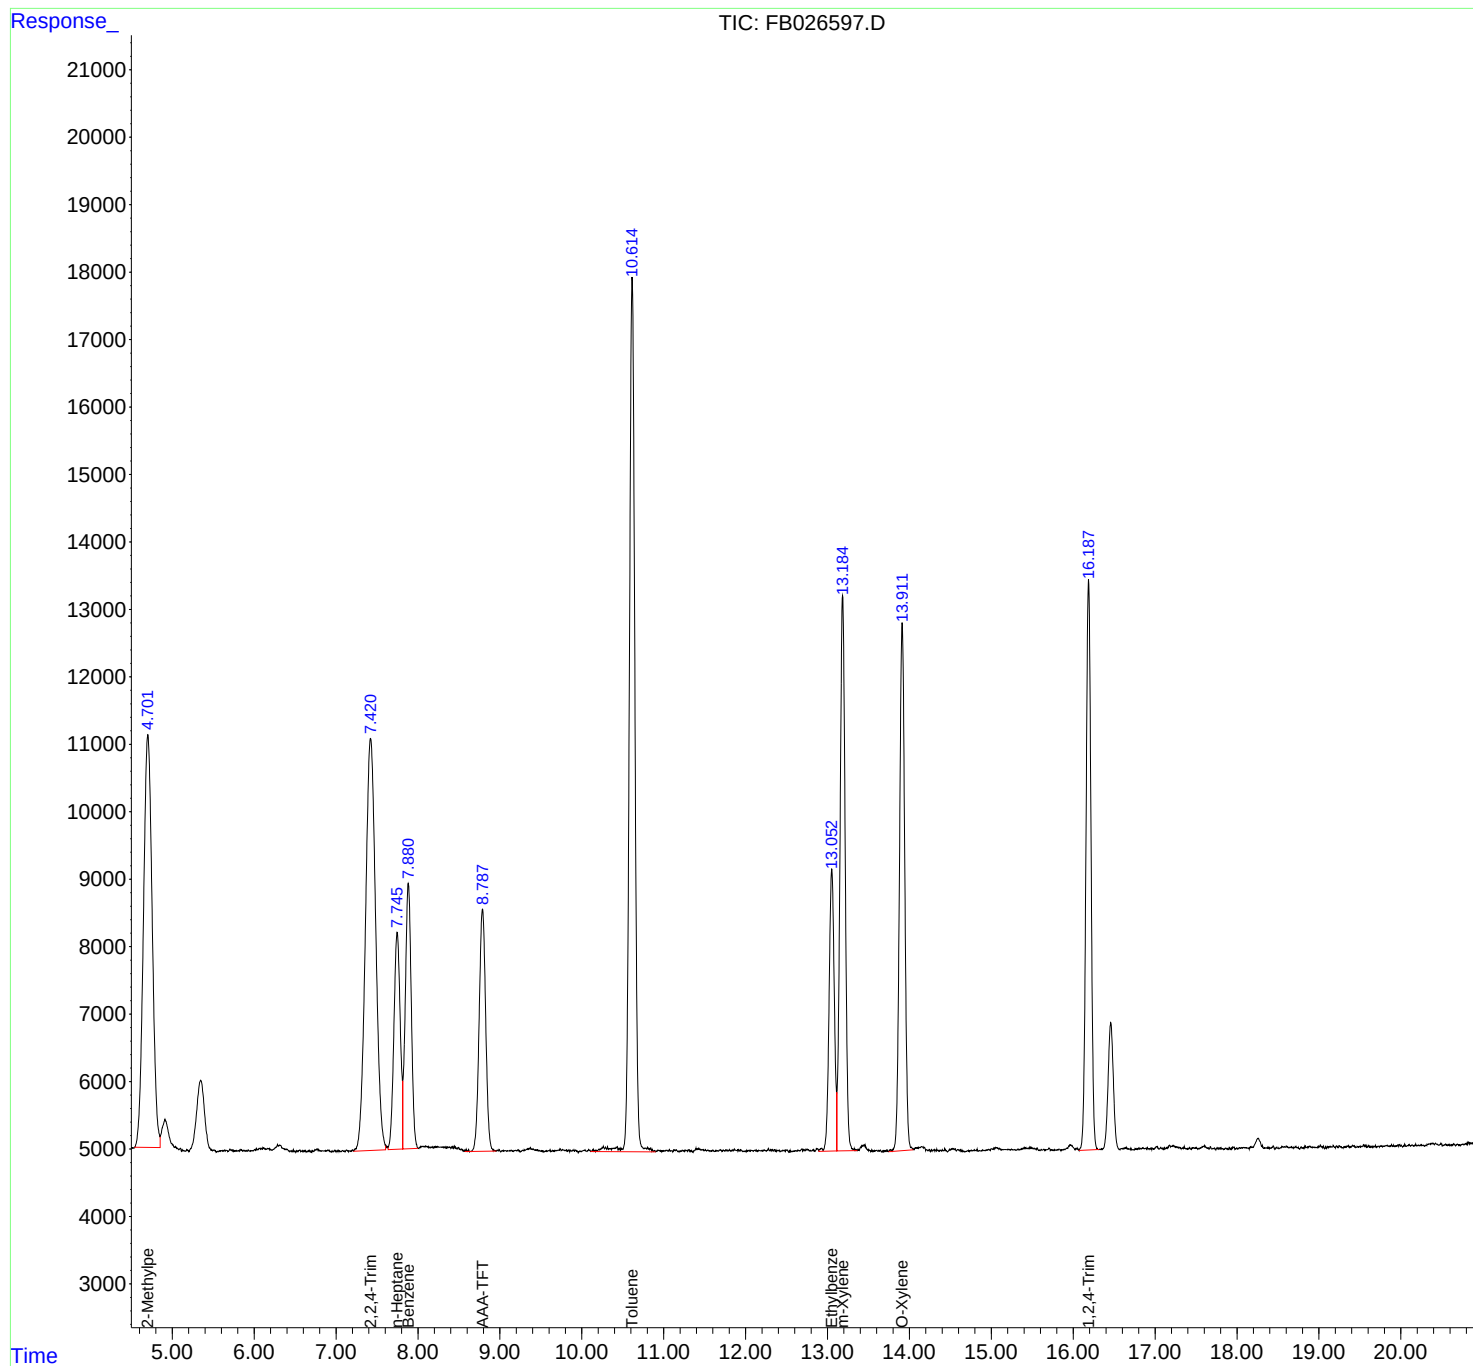


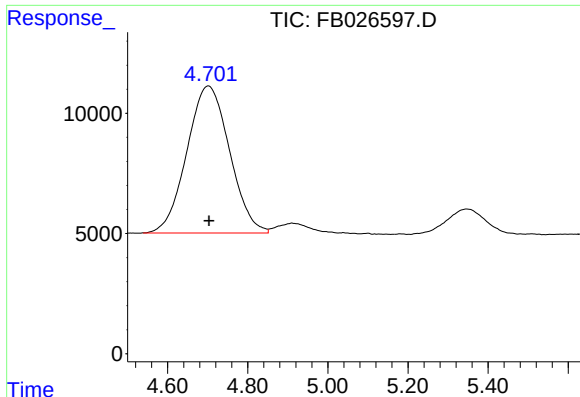

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.001 min
Response: 453248
Conc: 29.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0119S1

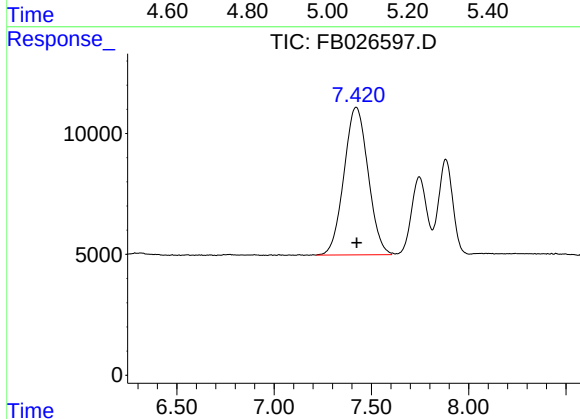


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.004 min
Response: 526408
Conc: 28.91 ng/ml

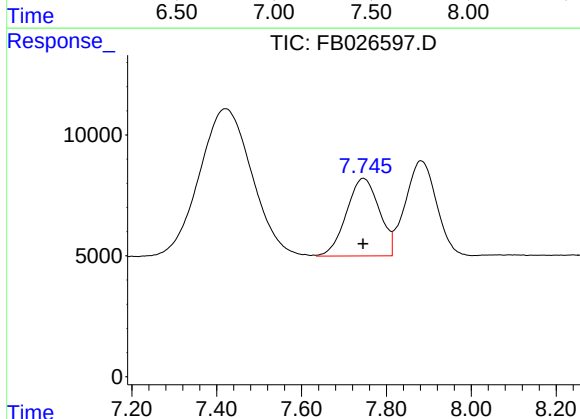


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 172791
Conc: 9.75 ng/ml

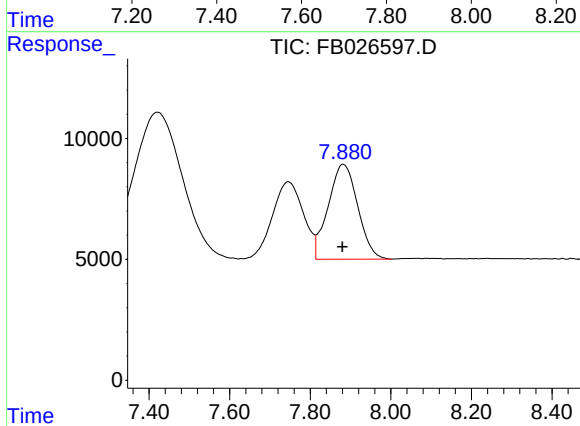

#4 Benzene


R.T.: 7.882 min
Delta R.T.: 0.002 min
Response: 200244
Conc: 9.81 ng/ml

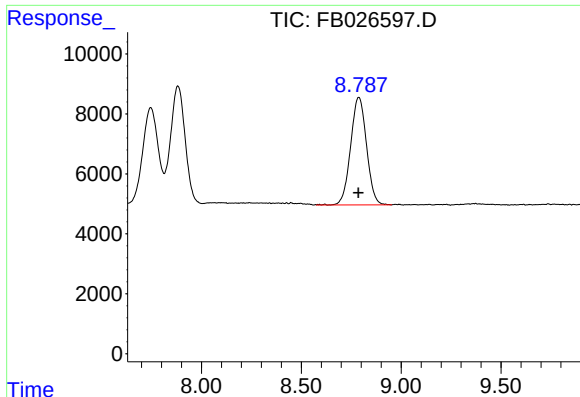

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.002 min
Response: 198595
Conc: 19.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0119S1

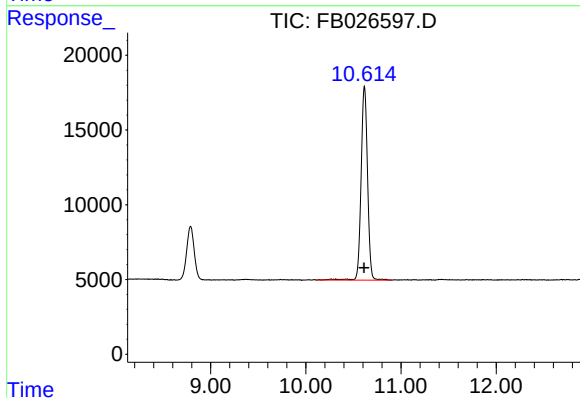


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.002 min
Response: 606065
Conc: 30.86 ng/ml

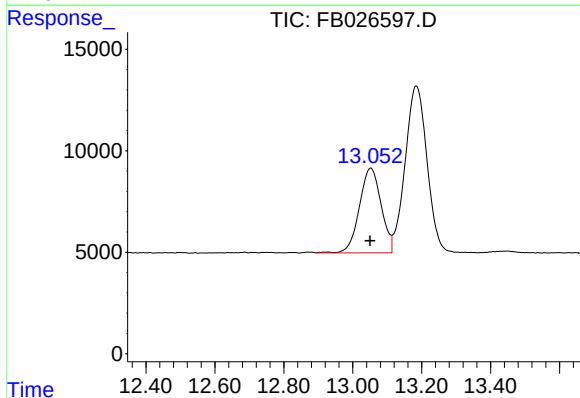


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.002 min
Response: 183036
Conc: 9.91 ng/ml

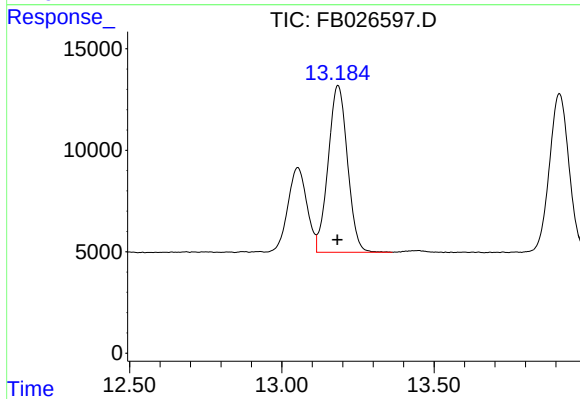

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.003 min
Response: 362556
Conc: 19.67 ng/ml

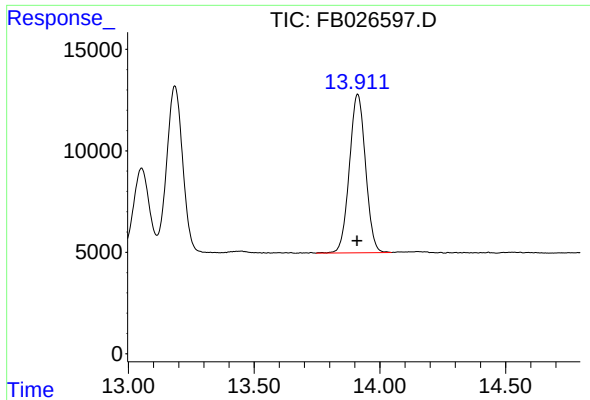

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.002 min
Response: 348334
Conc: 19.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0119S1

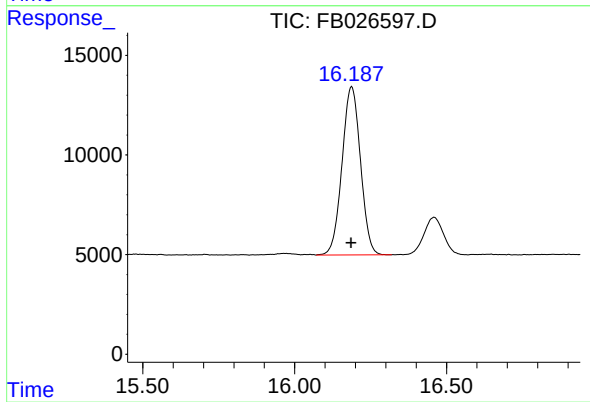

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.002 min
Response: 355618
Conc: 19.26 ng/ml