

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011923\
 Data File : FB029134.D
 Signal(s) : FID2B.CH
 Acq On : 19 Jan 2023 11:32
 Operator : AJ/MA
 Sample : BSF0119S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 20 00:03:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	245475	20.089 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	448807	30.655 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	522353	32.922 ng/ml
3) t n-Heptane	7.751	165931	9.931 ng/ml
4) t Benzene	7.888	211878	9.966 ng/ml
6) t Toluene	10.621	608951	30.213 ng/ml
7) t Ethylbenzene	13.058	191343	9.976 ng/ml
8) t m-Xylene	13.190	380608	20.343 ng/ml
9) t O-Xylene	13.916	374155	20.792 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	376947	21.144 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011923\
Data File : FB029134.D
Signal(s) : FID2B.CH
Acq On : 19 Jan 2023 11:32
Operator : AJ/MA
Sample : BSF0119S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 20 00:03:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

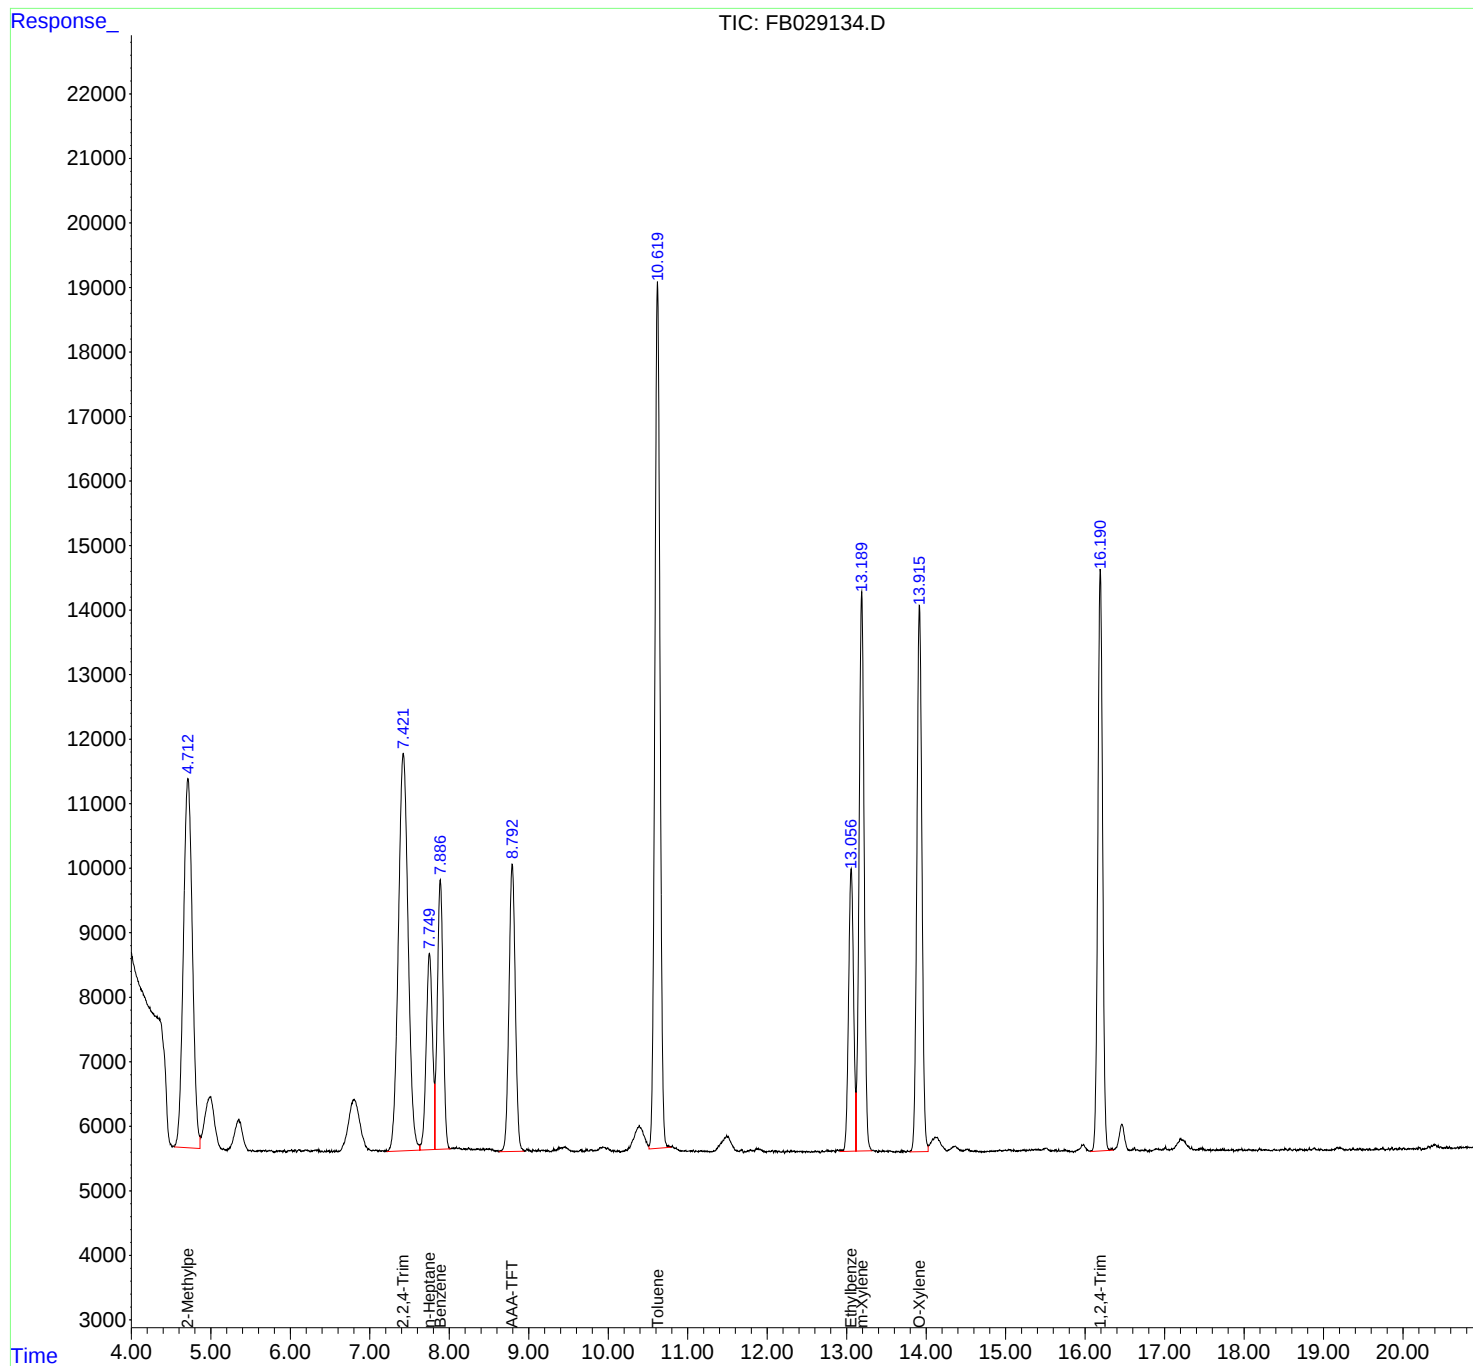

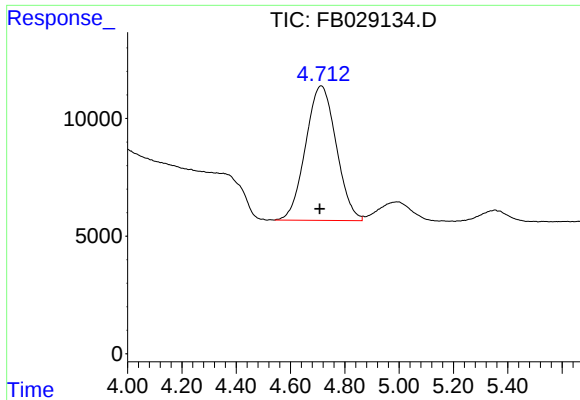


#1 2-Methylpentane

R.T.: 4.713 min
Delta R.T.: 0.006 min
Response: 448807
Conc: 30.65 ng/ml

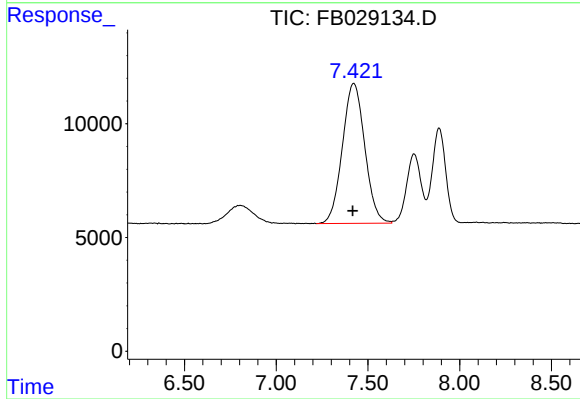


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.005 min
Response: 522353
Conc: 32.92 ng/ml

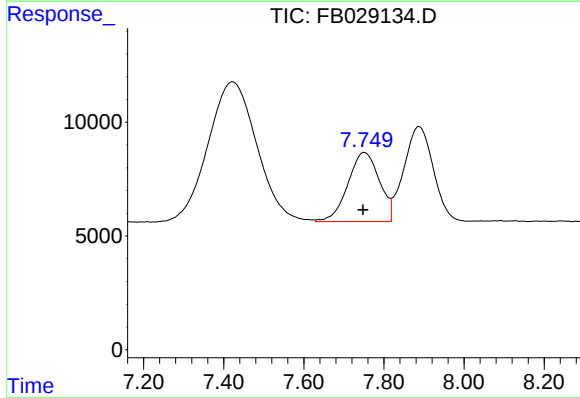


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.003 min
Response: 165931
Conc: 9.93 ng/ml

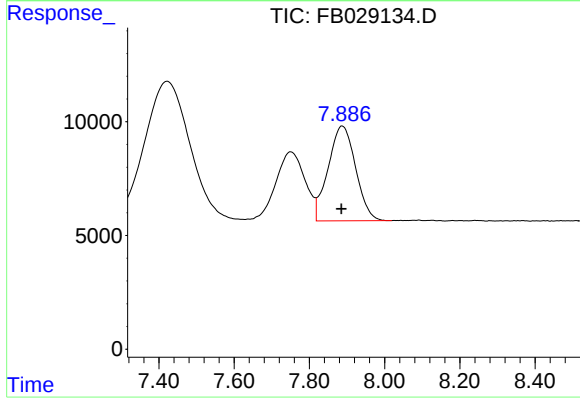


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.003 min
Response: 211878
Conc: 9.97 ng/ml

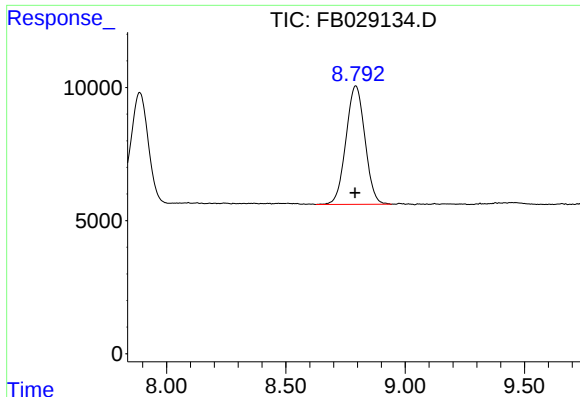


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 245475
Conc: 20.09 ng/ml

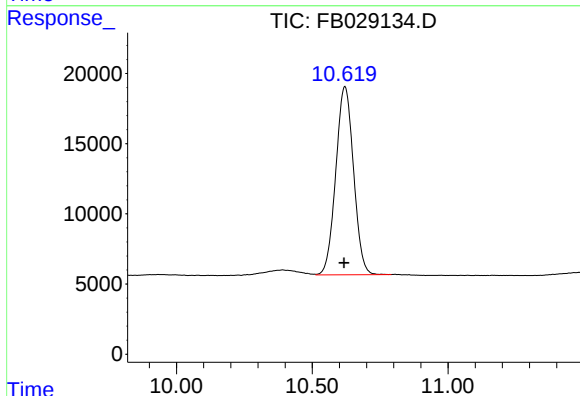


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.003 min
Response: 608951
Conc: 30.21 ng/ml

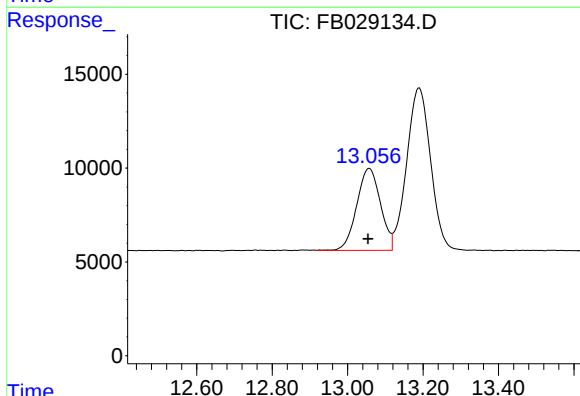


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 191343
Conc: 9.98 ng/ml

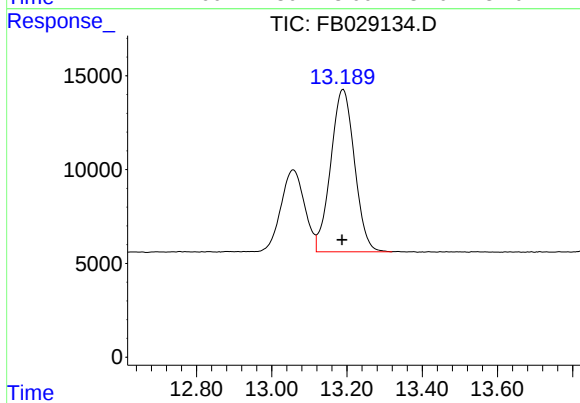

#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.003 min
Response: 380608
Conc: 20.34 ng/ml

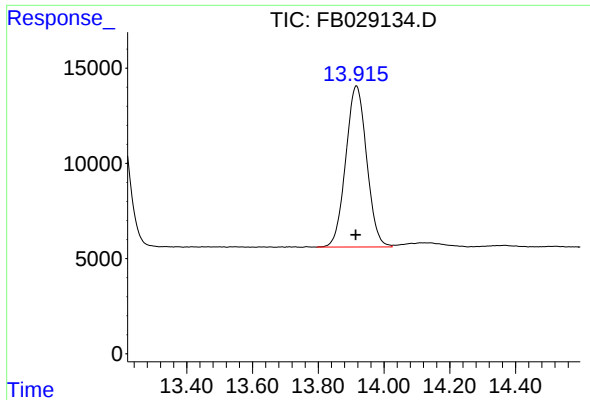


#9 O-Xylene

R.T.: 13.916 min

Delta R.T.: 0.002 min

Response: 374155

Conc: 20.79 ng/ml

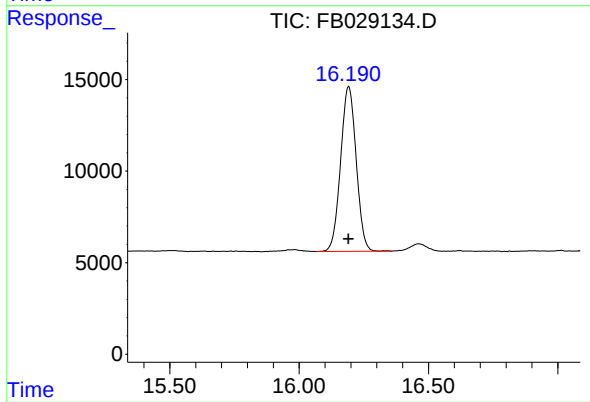

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min

Delta R.T.: 0.002 min

Response: 376947

Conc: 21.14 ng/ml