

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012020\
 Data File : FB023456.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jan 2020 9:42
 Operator : DD/AJ
 Sample : BSF0120S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 21 00:32:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	471975	19.870 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.685	977017	30.917 ng/ml
2) t	2,2,4-Trimethylpentane	7.413	1083523	31.912 ng/ml
3) t	n-Heptane	7.753	357225	10.668 ng/ml
4) t	Benzene	7.887	421966	10.333 ng/ml
6) t	Toluene	10.625	1211946	30.668 ng/ml
7) t	Ethylbenzene	13.065	371025	9.934 ng/ml
8) t	m-Xylene	13.199	707758	19.903 ng/ml
9) t	O-Xylene	13.926	685274	19.832 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	595698	20.372 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012020\
Data File : FB023456.D
Signal(s) : FID2B.CH
Acq On : 20 Jan 2020 9:42
Operator : DD/AJ
Sample : BSF0120S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 21 00:32:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

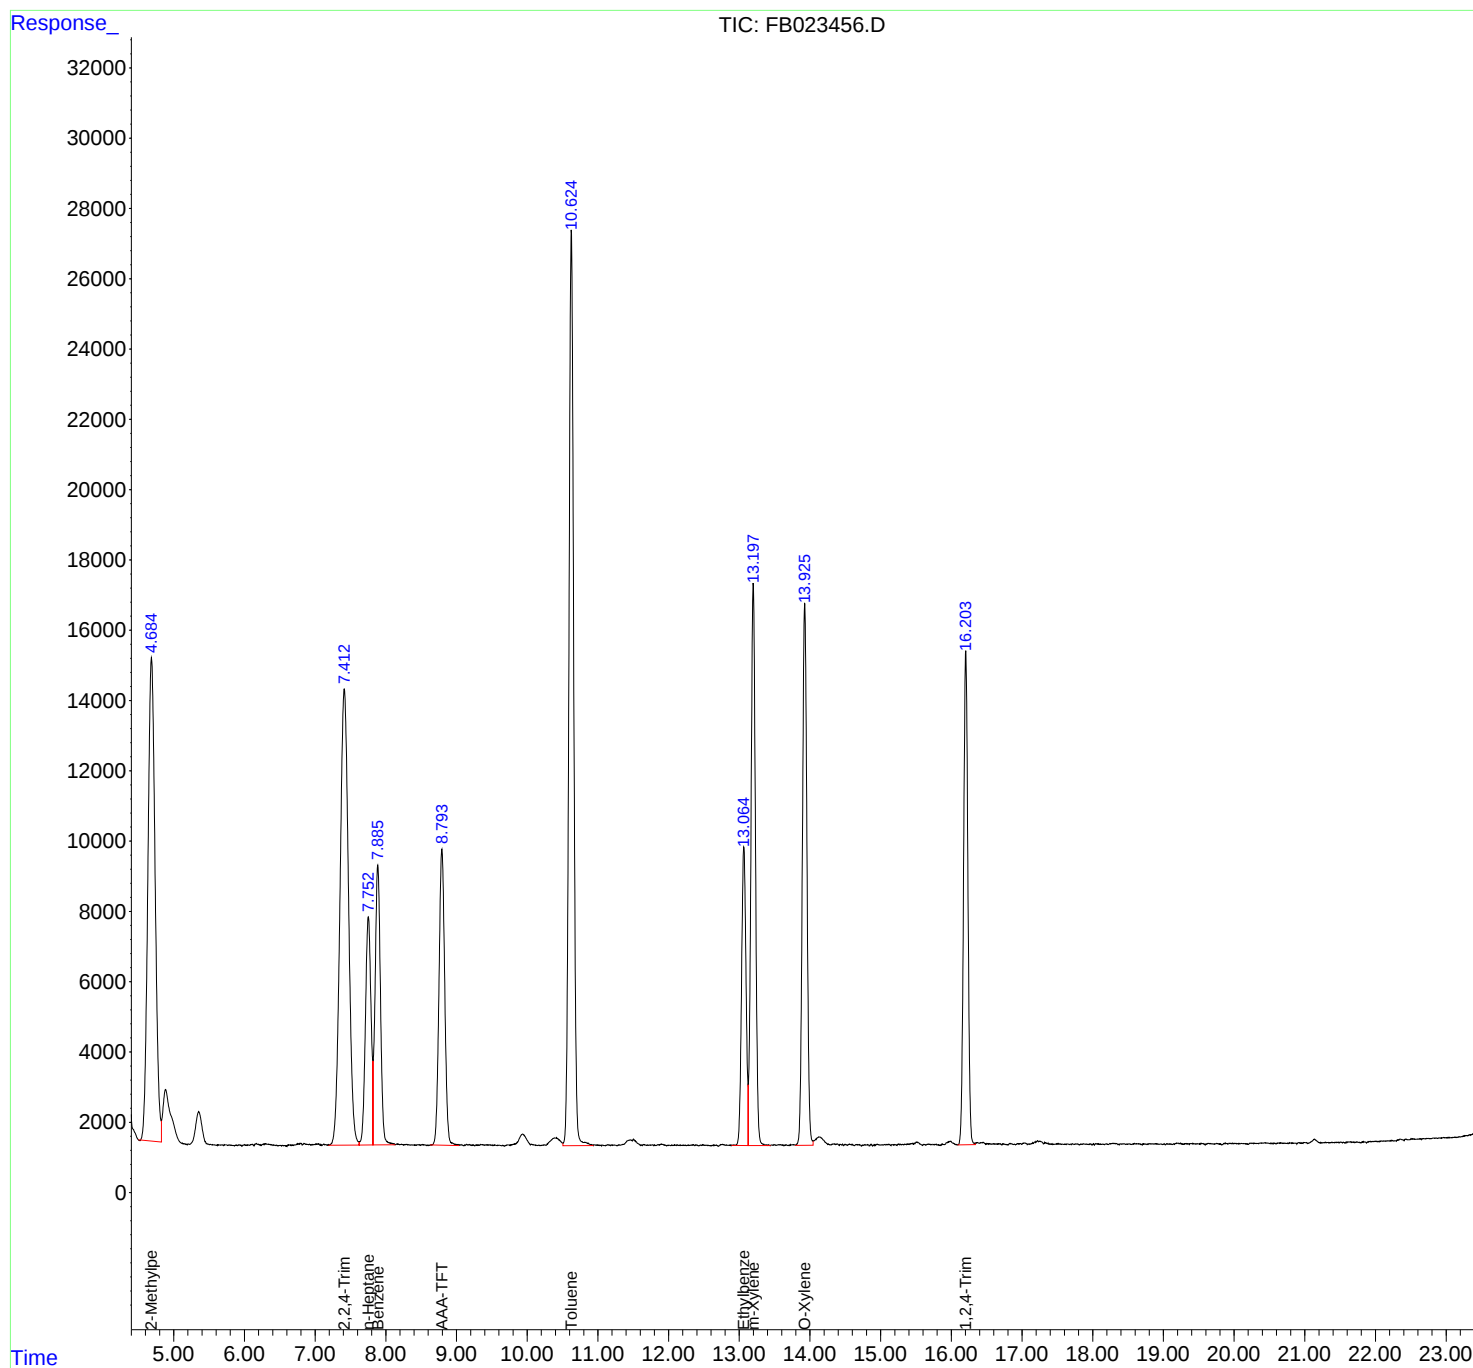

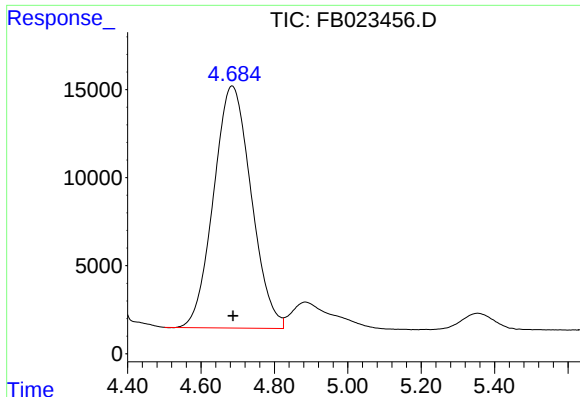


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.002 min
Response: 977017
Conc: 30.92 ng/ml

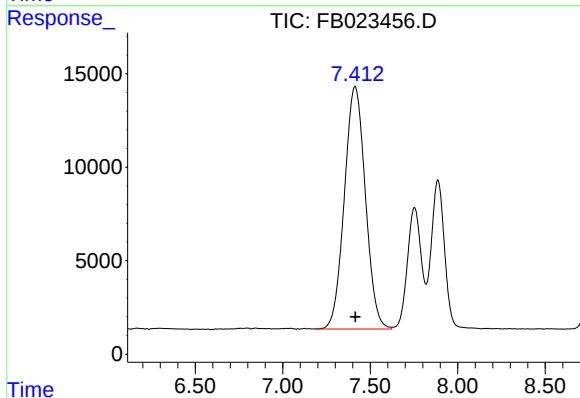


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.002 min
Response: 1083523
Conc: 31.91 ng/ml

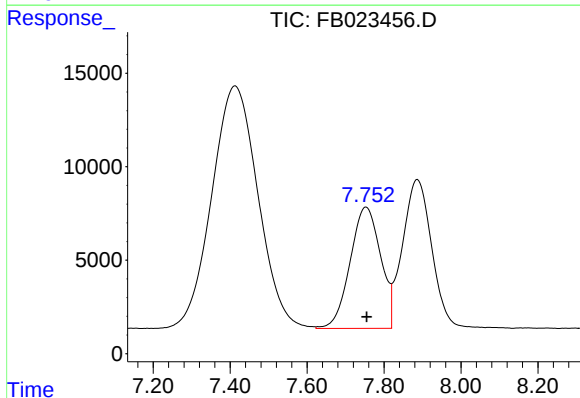


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 357225
Conc: 10.67 ng/ml

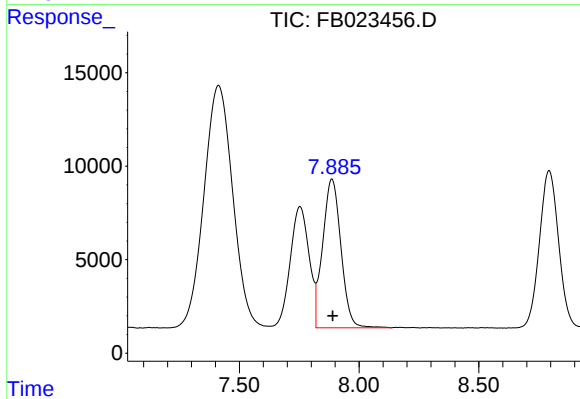


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 421966
Conc: 10.33 ng/ml

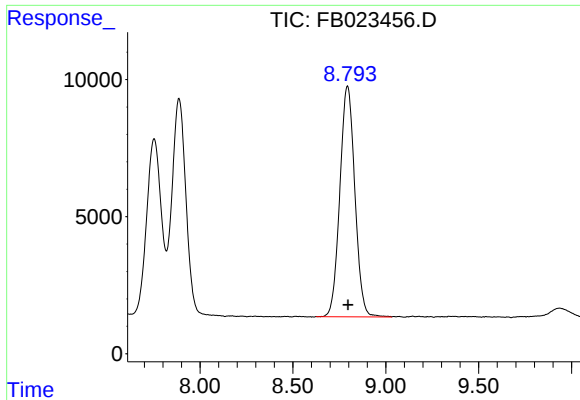


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 471975
Conc: 19.87 ng/ml

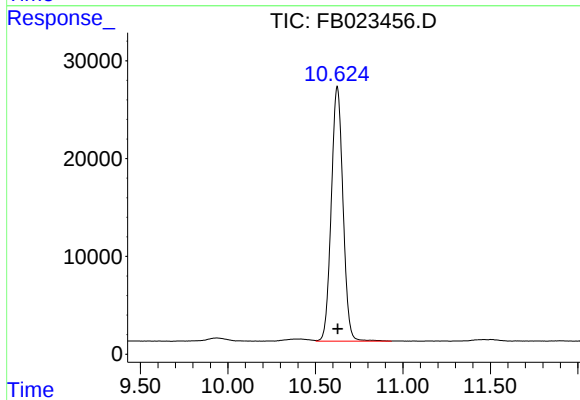


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 1211946
Conc: 30.67 ng/ml

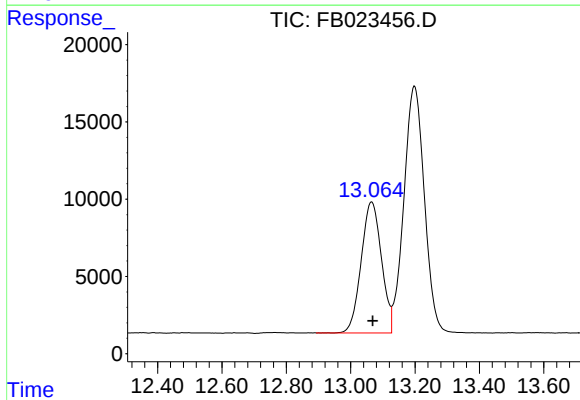


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 371025
Conc: 9.93 ng/ml

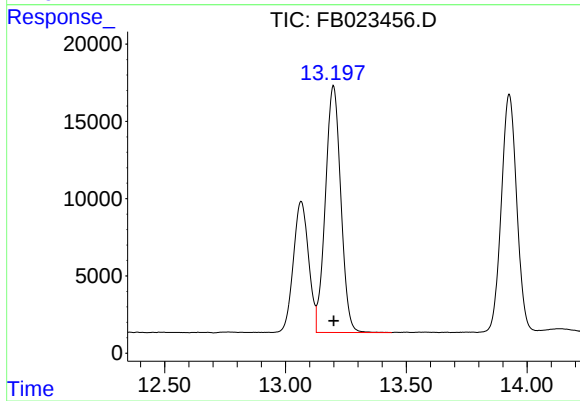


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 707758
Conc: 19.90 ng/ml

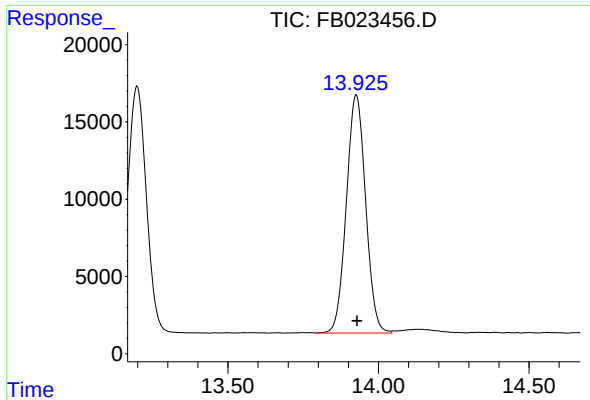

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.002 min
Response: 685274
Conc: 19.83 ng/ml

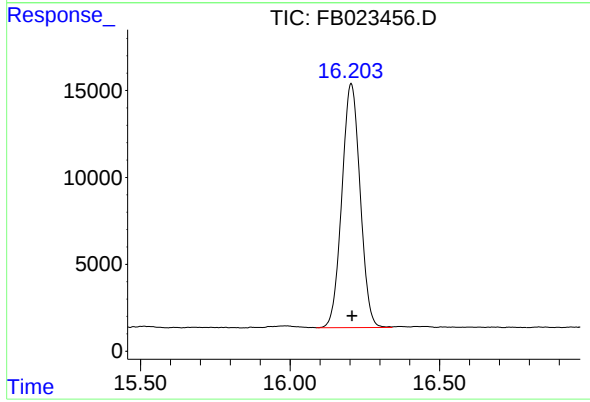

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 595698
Conc: 20.37 ng/ml