

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012023\
 Data File : FB029151.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jan 2023 16:16
 Operator : AJ/MA
 Sample : 01232-03MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 21 02:06:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	229747	18.802 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	337452	23.049 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	400819	25.262 ng/ml
3) t n-Heptane	7.756	134499	8.049 ng/ml
4) t Benzene	7.892	189364	8.907 ng/ml
6) t Toluene	10.623	548640	27.220 ng/ml
7) t Ethylbenzene	13.060	171777	8.956 ng/ml
8) t m-Xylene	13.192	335598	17.937 ng/ml
9) t O-Xylene	13.919	328192	18.238 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	297507	16.688 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012023\
Data File : FB029151.D
Signal(s) : FID2B.CH
Acq On : 20 Jan 2023 16:16
Operator : AJ/MA
Sample : 01232-03MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 21 02:06:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

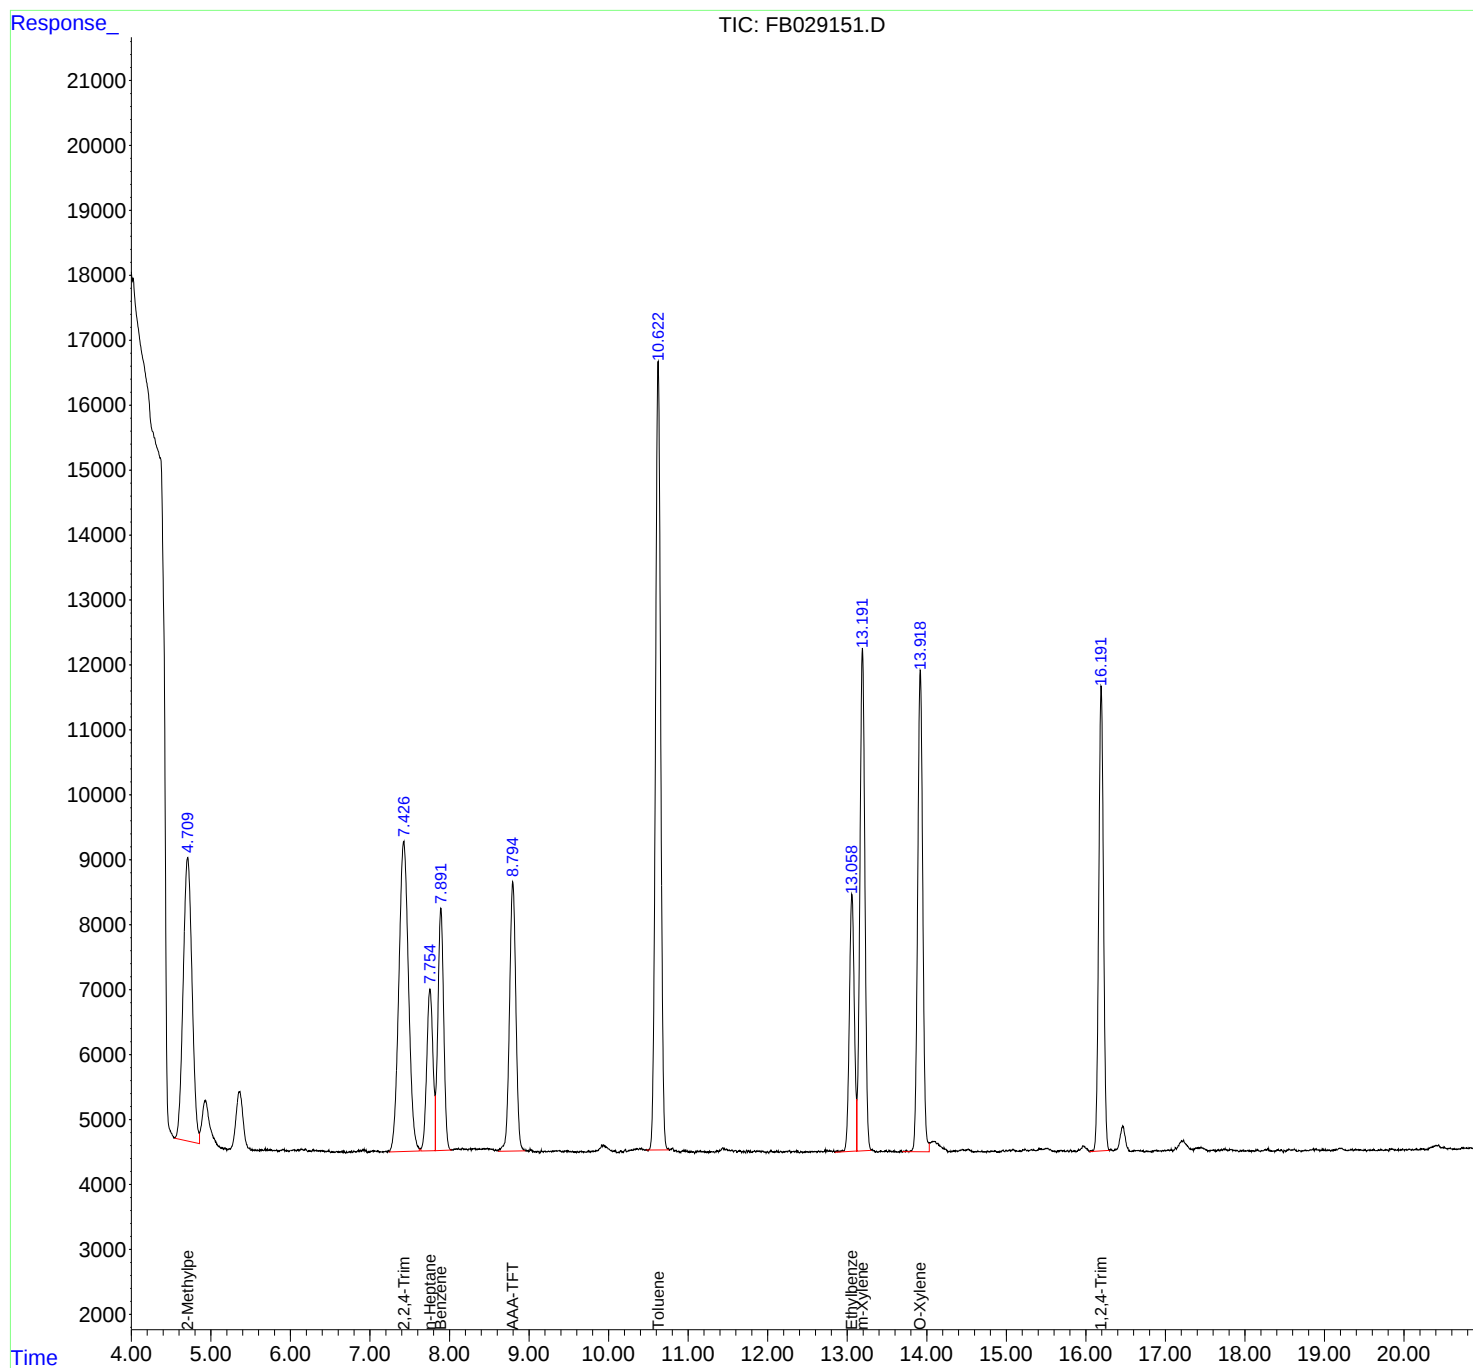

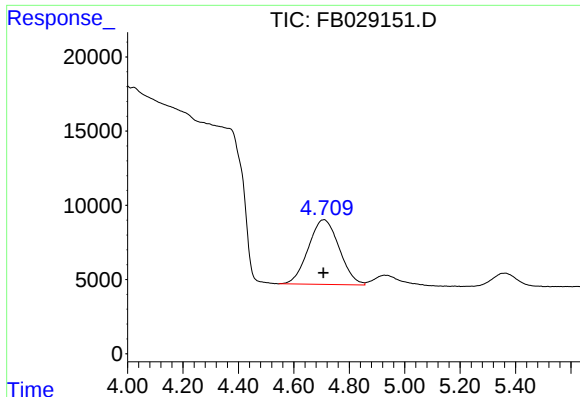


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 337452
Conc: 23.05 ng/ml

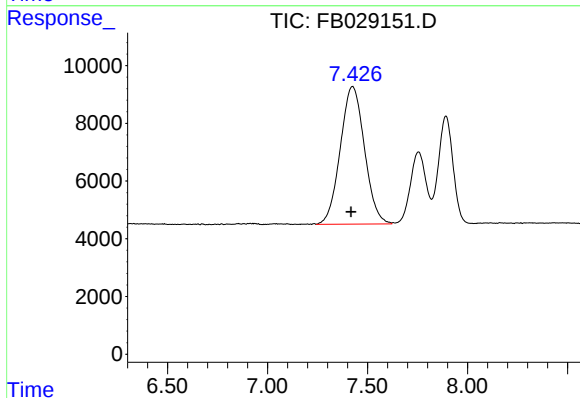


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.009 min
Response: 400819
Conc: 25.26 ng/ml

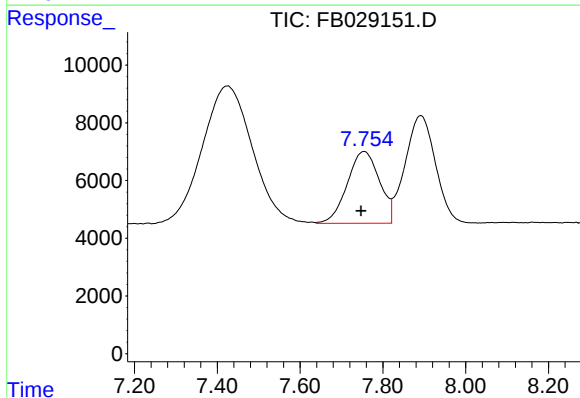


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.008 min
Response: 134499
Conc: 8.05 ng/ml

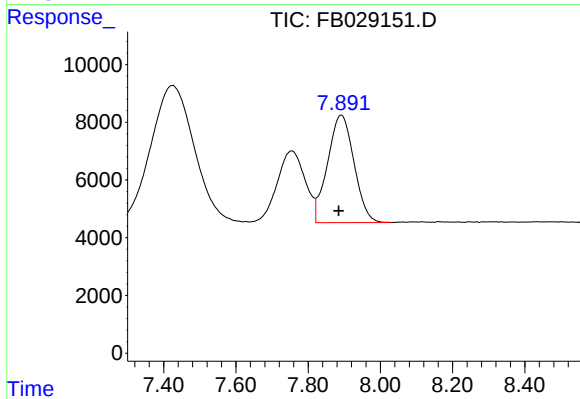


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.007 min
Response: 189364
Conc: 8.91 ng/ml

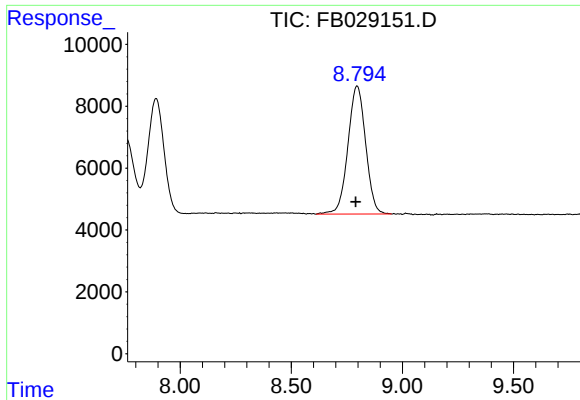


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.007 min
Response: 229747
Conc: 18.80 ng/ml

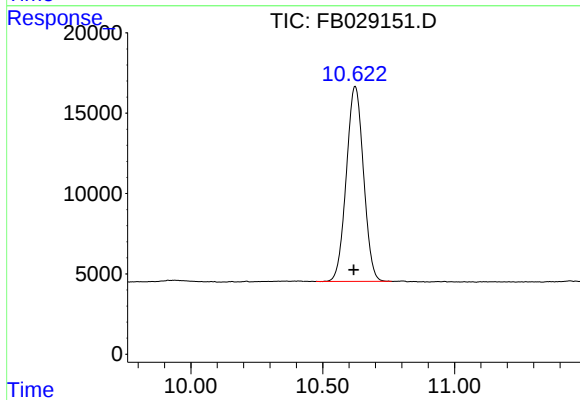


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.006 min
Response: 548640
Conc: 27.22 ng/ml

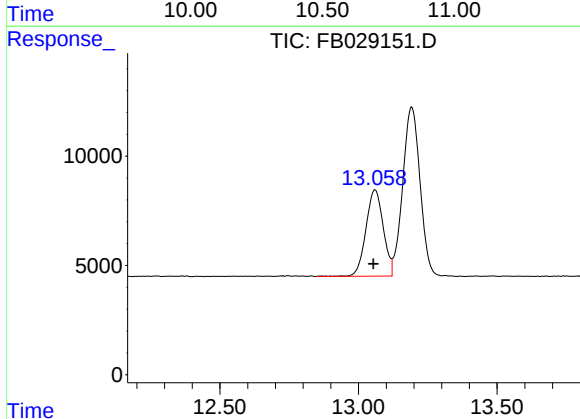


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 171777
Conc: 8.96 ng/ml

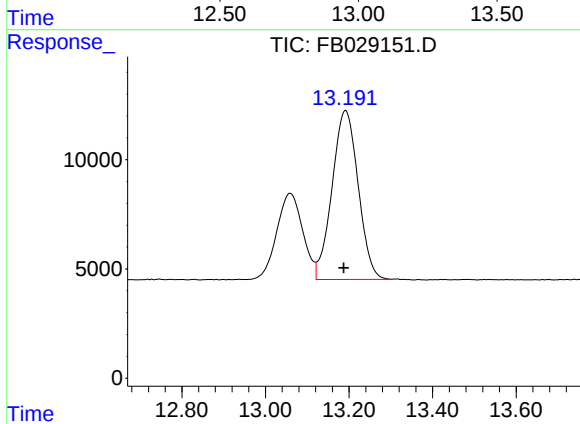


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: 0.005 min
Response: 335598
Conc: 17.94 ng/ml

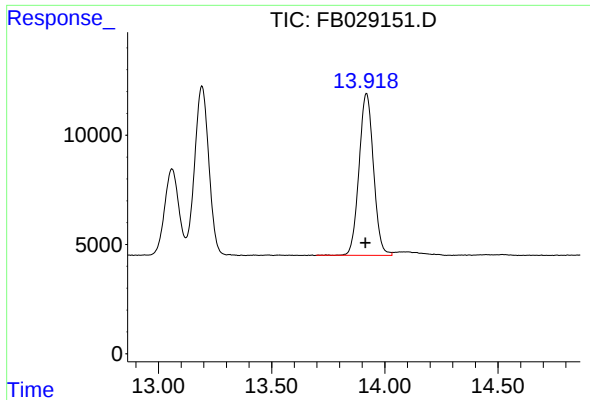

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.005 min
Response: 328192
Conc: 18.24 ng/ml

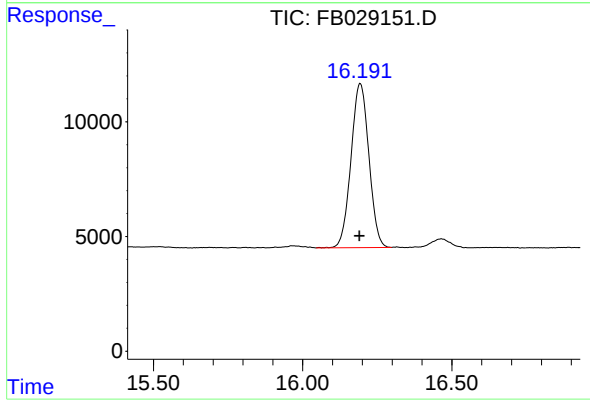

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.003 min
Response: 297507
Conc: 16.69 ng/ml