

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB012120\  
 Data File : FB023463.D  
 Signal(s) : FID2B.CH  
 Acq On : 21 Jan 2020 10:18  
 Operator : DD/AJ  
 Sample : VBF0121S1  
 Misc : 5.01g/5.00ml DI WATER  
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
 Quant Time: Jan 22 01:04:18 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011620.M  
 Quant Title :  
 QLast Update : Thu Jan 16 11:42:55 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    |                        | R.T.   | Response | Conc Units   |
|-----------------------------|------------------------|--------|----------|--------------|
| -----                       |                        |        |          |              |
| System Monitoring Compounds |                        |        |          |              |
| 5) s                        | AAA-TFT                | 8.792  | 483129   | 20.339 ng/ml |
| Target Compounds            |                        |        |          |              |
| 1) t                        | 2-Methylpentane        | 4.674  | 3463     | 0.110 ng/ml  |
| 2) t                        | 2,2,4-Trimethylpentane | 7.406  | 9901     | 0.292 ng/ml  |
| 6) t                        | Toluene                | 10.631 | 2161     | 0.055 ng/ml  |
| 8) t                        | m-Xylene               | 13.191 | 4314     | 0.121 ng/ml  |
| 9) t                        | O-Xylene               | 13.924 | 2074     | 0.060 ng/ml  |
| 10) t                       | 1,2,4-Trimethylbenzene | 16.200 | 2344     | 0.080 ng/ml  |
| -----                       |                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB012120\  
Data File : FB023463.D  
Signal(s) : FID2B.CH  
Acq On : 21 Jan 2020 10:18  
Operator : DD/AJ  
Sample : VBF0121S1  
Misc : 5.01g/5.00ml DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jan 22 01:04:18 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011620.M  
Quant Title :  
QLast Update : Thu Jan 16 11:42:55 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

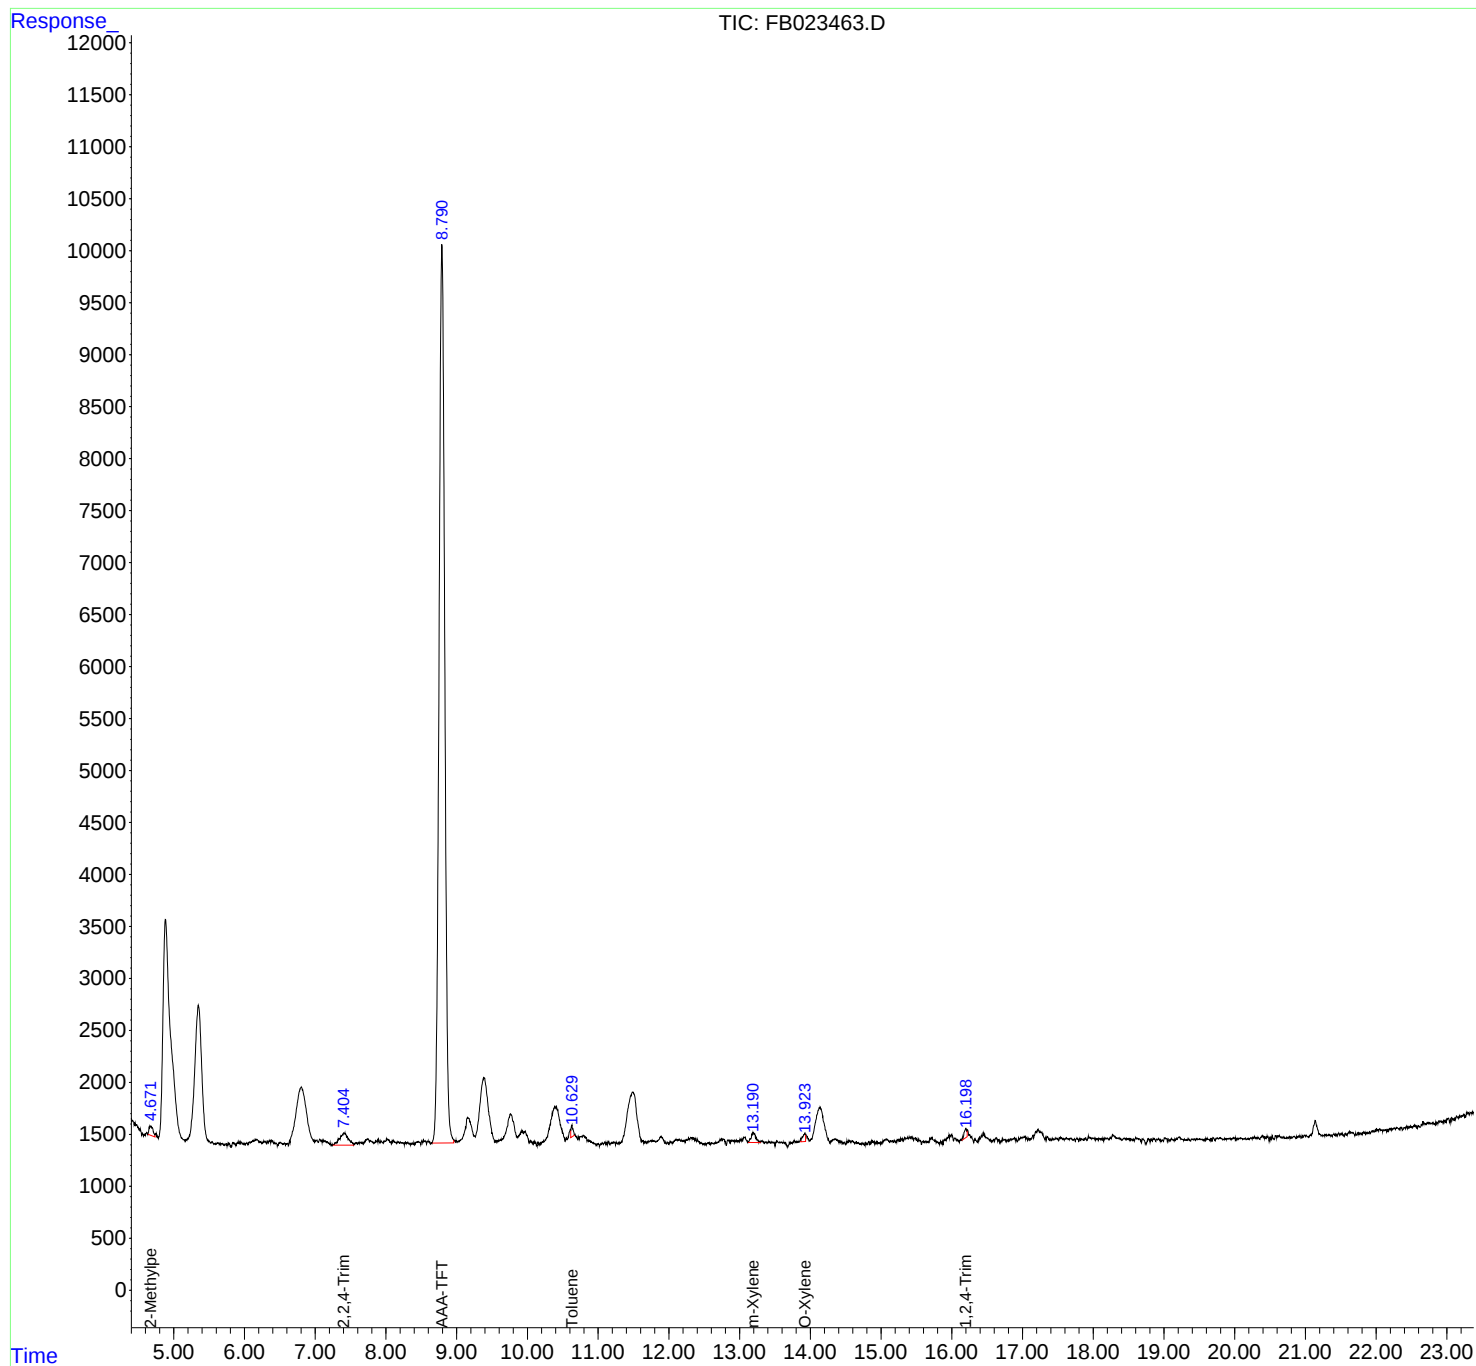

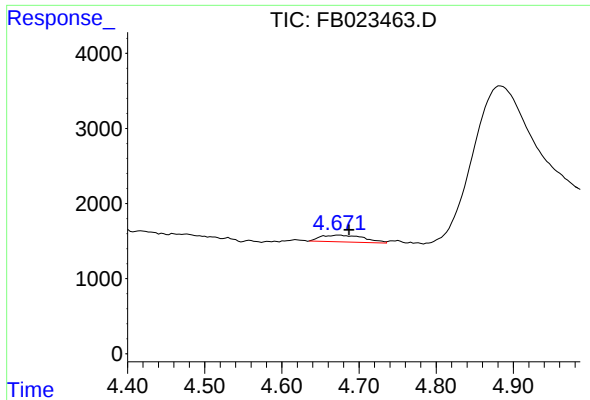


#1 2-Methylpentane

R.T.: 4.674 min  
Delta R.T.: -0.013 min  
Response: 3463  
Conc: 0.11 ng/ml

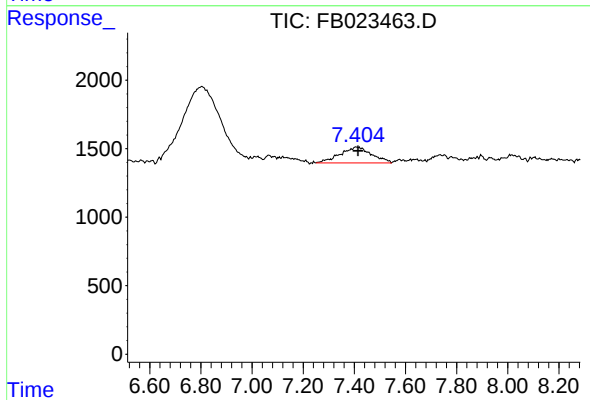


#2 2,2,4-Trimethylpentane

R.T.: 7.406 min  
Delta R.T.: -0.009 min  
Response: 9901  
Conc: 0.29 ng/ml

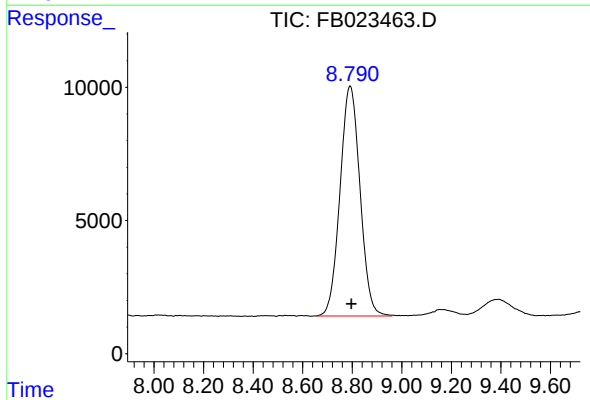


#5 AAA-TFT

R.T.: 8.792 min  
Delta R.T.: -0.005 min  
Response: 483129  
Conc: 20.34 ng/ml

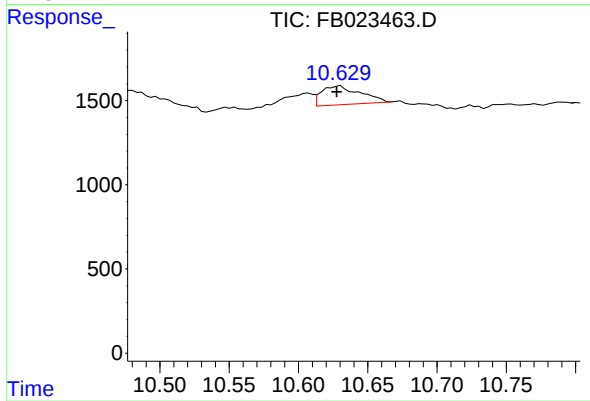


#6 Toluene

R.T.: 10.631 min  
Delta R.T.: 0.003 min  
Response: 2161  
Conc: 0.05 ng/ml

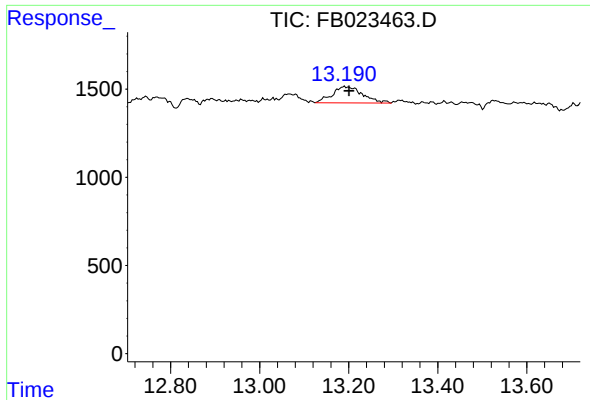


#8 m-Xylene

R.T.: 13.191 min  
Delta R.T.: -0.010 min  
Response: 4314  
Conc: 0.12 ng/ml

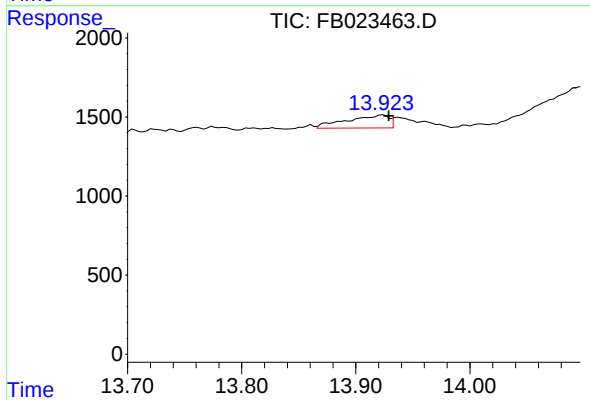

#9 o-Xylene

R.T.: 13.924 min  
Delta R.T.: -0.005 min  
Response: 2074  
Conc: 0.06 ng/ml

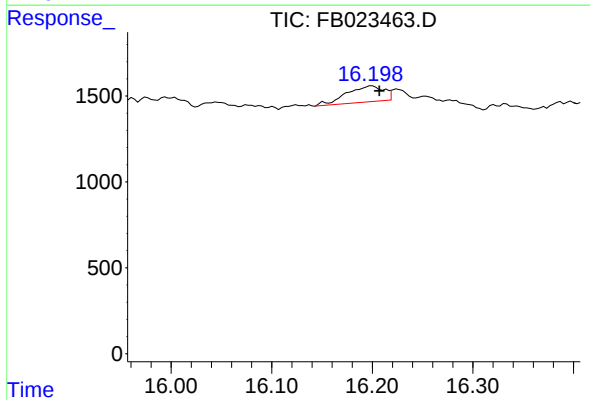

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min  
Delta R.T.: -0.007 min  
Response: 2344  
Conc: 0.08 ng/ml