

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012120\
Data File : FB023466.D
Signal(s) : FID2B.CH
Acq On : 21 Jan 2020 11:48
Operator : DD/AJ
Sample : L1210-06
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 22 01:04:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	498803	20.999 ng/ml
Target Compounds			
6) t Toluene	10.625	2593	0.066 ng/ml
8) t m-Xylene	13.201	1633	0.046 ng/ml
9) t O-Xylene	13.916	1735	0.050 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012120\
Data File : FB023466.D
Signal(s) : FID2B.CH
Acq On : 21 Jan 2020 11:48
Operator : DD/AJ
Sample : L1210-06
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 22 01:04:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

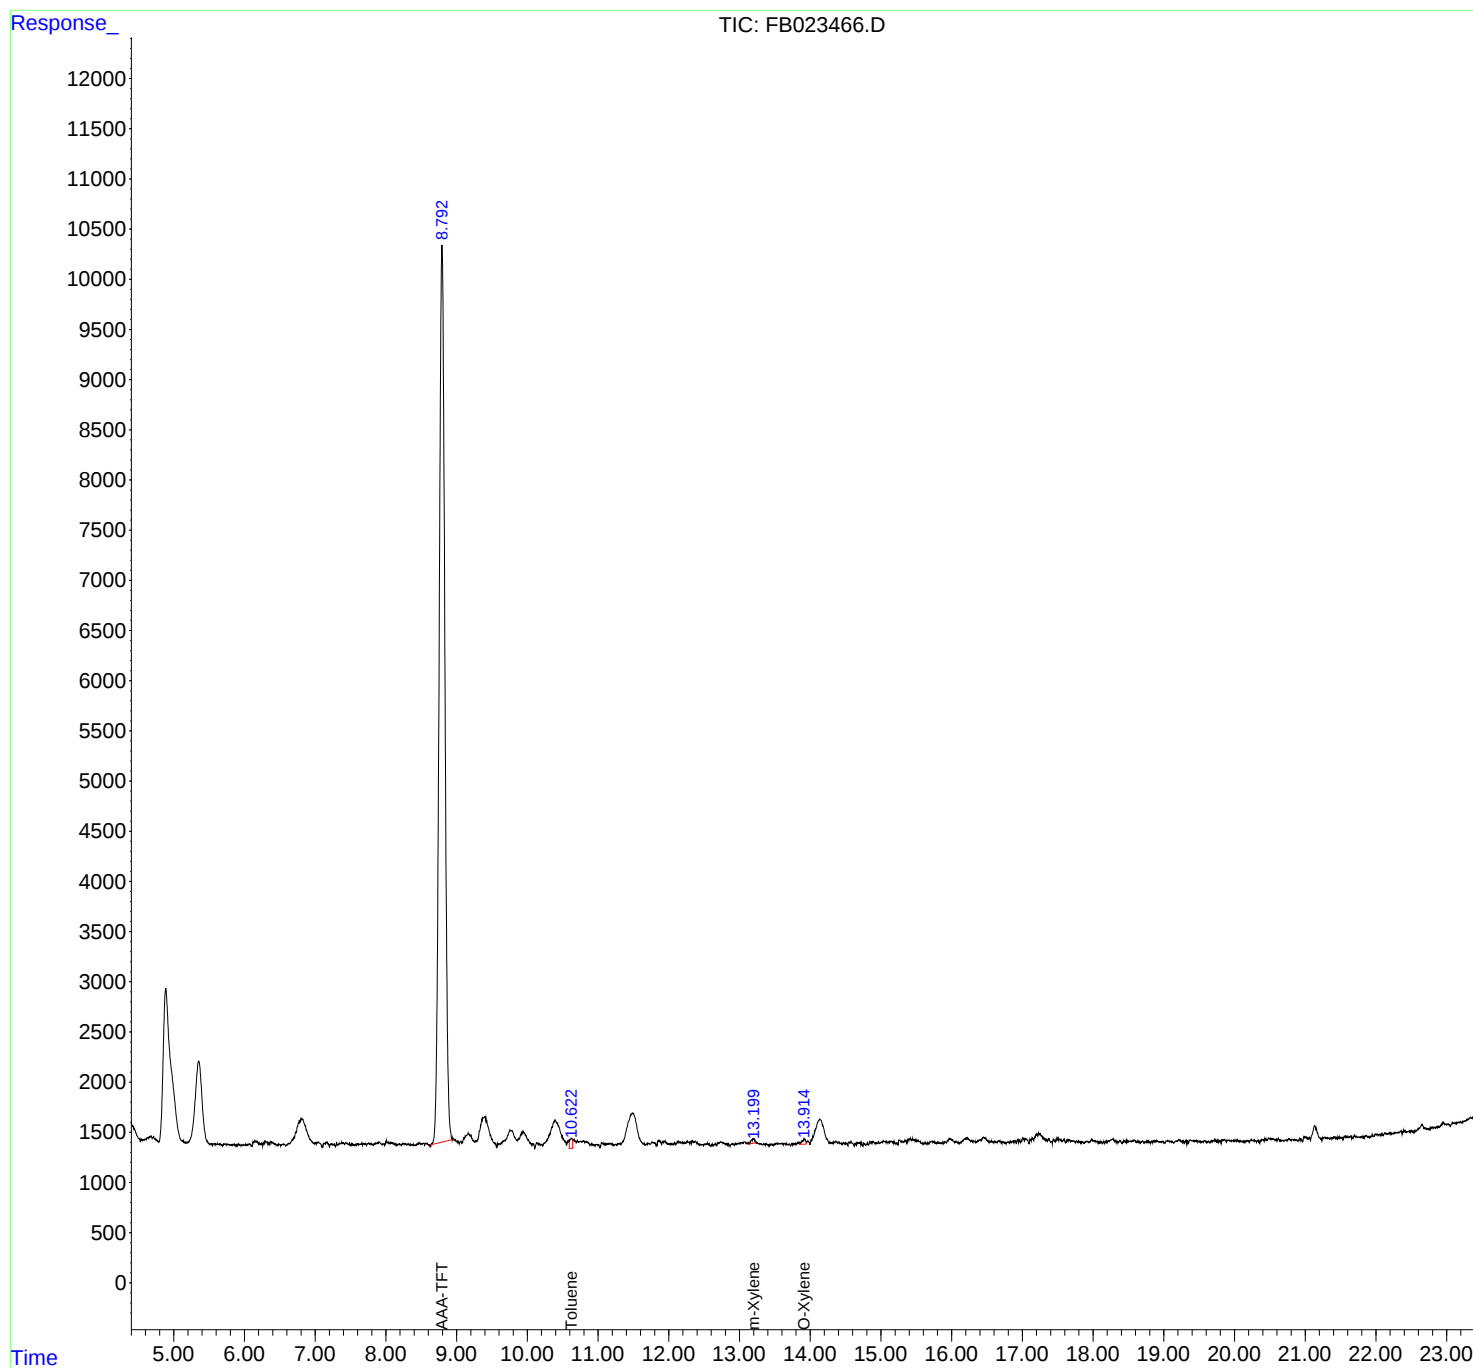

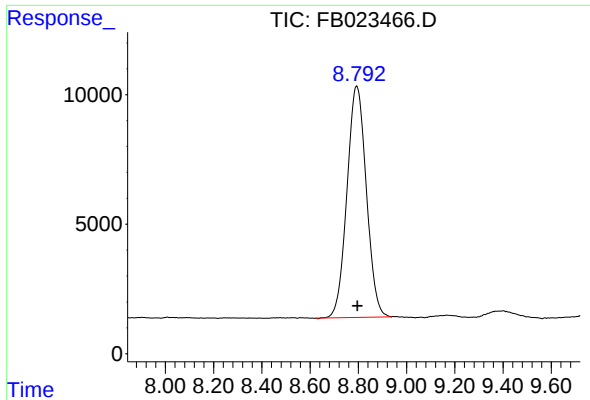


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 498803
Conc: 21.00 ng/ml

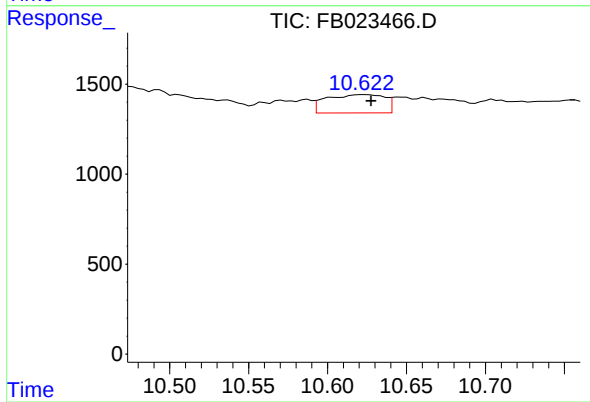


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 2593
Conc: 0.07 ng/ml

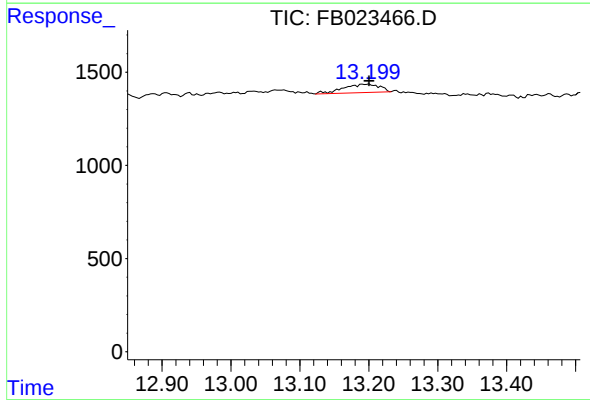

#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 1633
Conc: 0.05 ng/ml

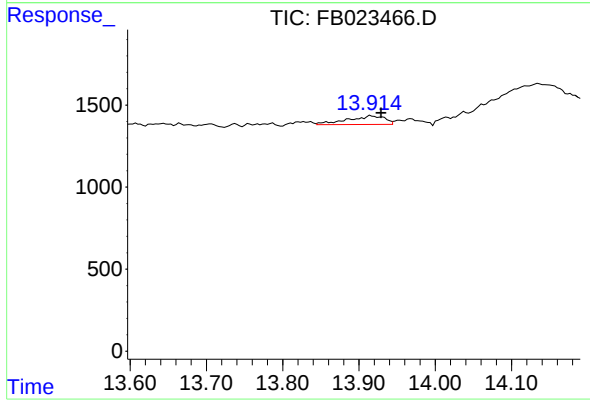

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.013 min
Response: 1735
Conc: 0.05 ng/ml