

Data Path : P:\HPCHEM1\FID B\Data\FB012218\
Data File : FB013186.D
Signal(s) : FID2B.CH
Acq On : 23 Jan 2018 6:19
Operator : MJ/SJ
Sample : J1218-01
Misc : 5.05g/5.00mL DI Water
ALS Vial : 35 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 23 09:09:18 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB012218.M
Quant Title :
QLast Update : Mon Jan 22 11:28:15 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.137	95744	12.551 ng/ml
Target Compounds			
7) t Ethylbenzene	13.430	15047	0.895 ng/ml
8) t m-Xylene	13.565	22985	1.267 ng/ml
9) t o-Xylene	14.301	30743	1.612 ng/ml
10) t 1,2,4-Trimethylbenzene	16.592	62047	3.147 ng/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.


Data Path : P:\HPCHEM1\FID B\Data\FB012218\
Data File : FB013186.D
Signal(s) : FID2B.CH
Acq On : 23 Jan 2018 6:19
Operator : MJ/SJ
Sample : J1218-01
Misc : 5.05g/5.00mL DI Water
ALS Vial : 35 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 23 09:09:18 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB012218.M
Quant Title :
QLast Update : Mon Jan 22 11:28:15 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60m x 0.53mm x 3.00um




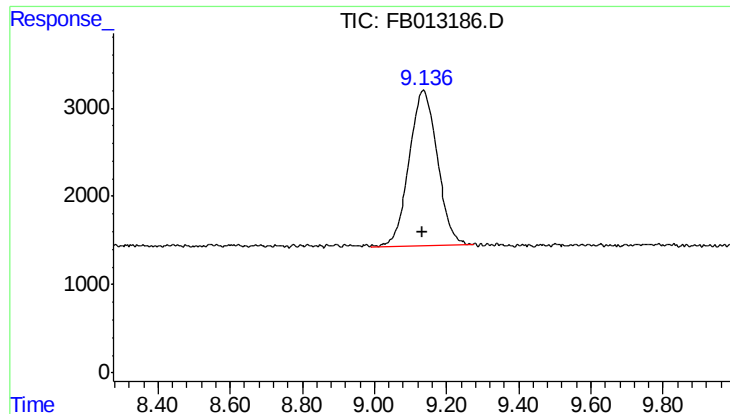

#5 AAA-TFT


R.T.: 9.137 min
Delta R.T.: 0.003 min
Response: 95744
Conc: 12.55 ng/ml

Instrument :
FID_B
ClientSampleId :

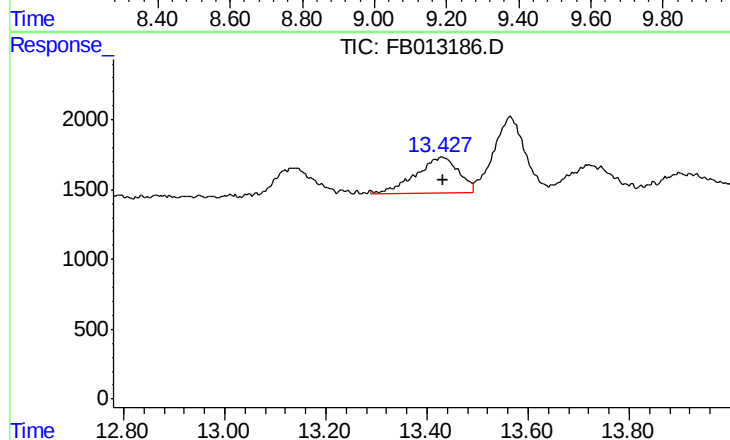


#7 Ethylbenzene

R.T.: 13.430 min
Delta R.T.: -0.001 min
Response: 15047
Conc: 0.89 ng/ml

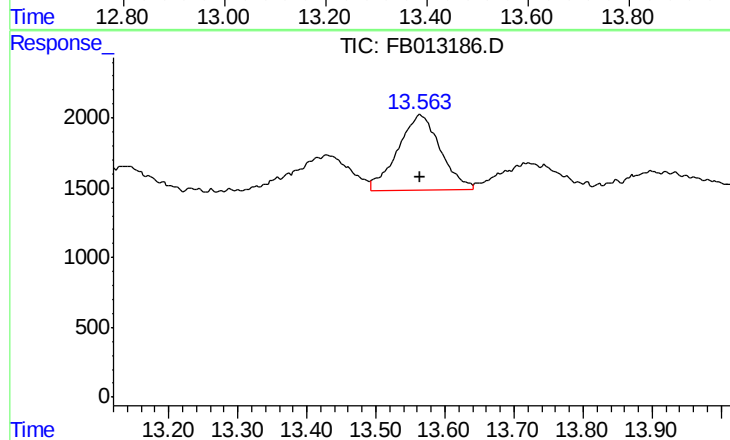


#8 m-Xylene

R.T.: 13.565 min
Delta R.T.: 0.001 min
Response: 22985
Conc: 1.27 ng/ml

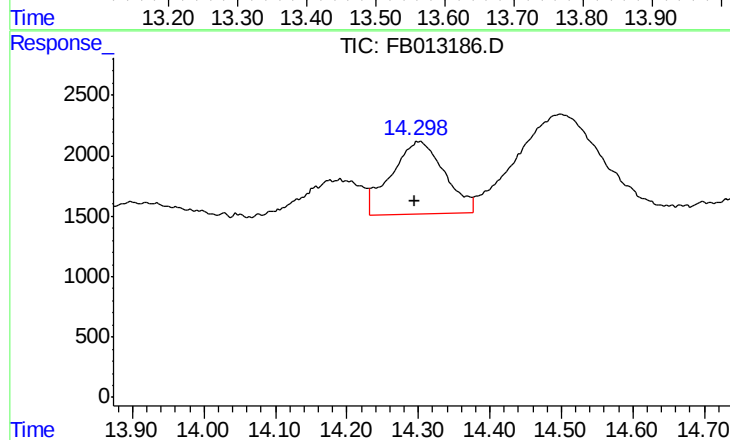

#9 O-Xylene

R.T.: 14.301 min
Delta R.T.: 0.006 min
Response: 30743
Conc: 1.61 ng/ml

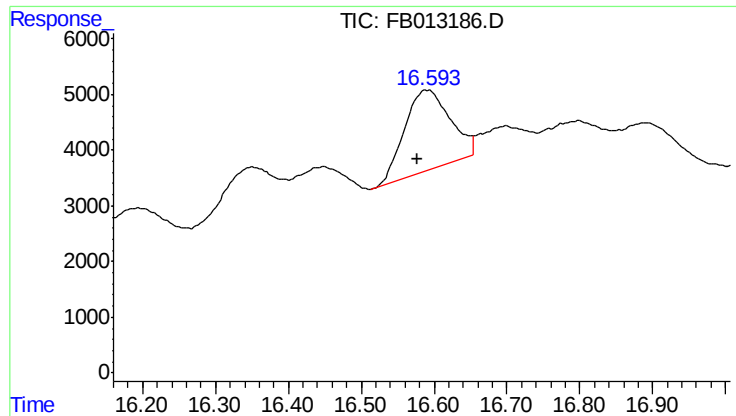

#10 1,2,4-Trimethylbenzene

R.T.: 16.592 min
Delta R.T.: 0.014 min
Response: 62047
Conc: 3.15 ng/ml

Instrument :
FID_B
ClientSampleId :