

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012220\
 Data File : FB023477.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jan 2020 12:07
 Operator : DD/AJ
 Sample : L1216-06MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 23 00:18:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	518372	21.823 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	905233	28.646 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	989469	29.142 ng/ml
3) t n-Heptane	7.752	319016	9.527 ng/ml
4) t Benzene	7.887	407087	9.968 ng/ml
6) t Toluene	10.624	1170114	29.609 ng/ml
7) t Ethylbenzene	13.064	361051	9.667 ng/ml
8) t m-Xylene	13.197	691286	19.440 ng/ml
9) t O-Xylene	13.925	673764	19.499 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	570208	19.500 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012220\
Data File : FB023477.D
Signal(s) : FID2B.CH
Acq On : 22 Jan 2020 12:07
Operator : DD/AJ
Sample : L1216-06MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 23 00:18:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

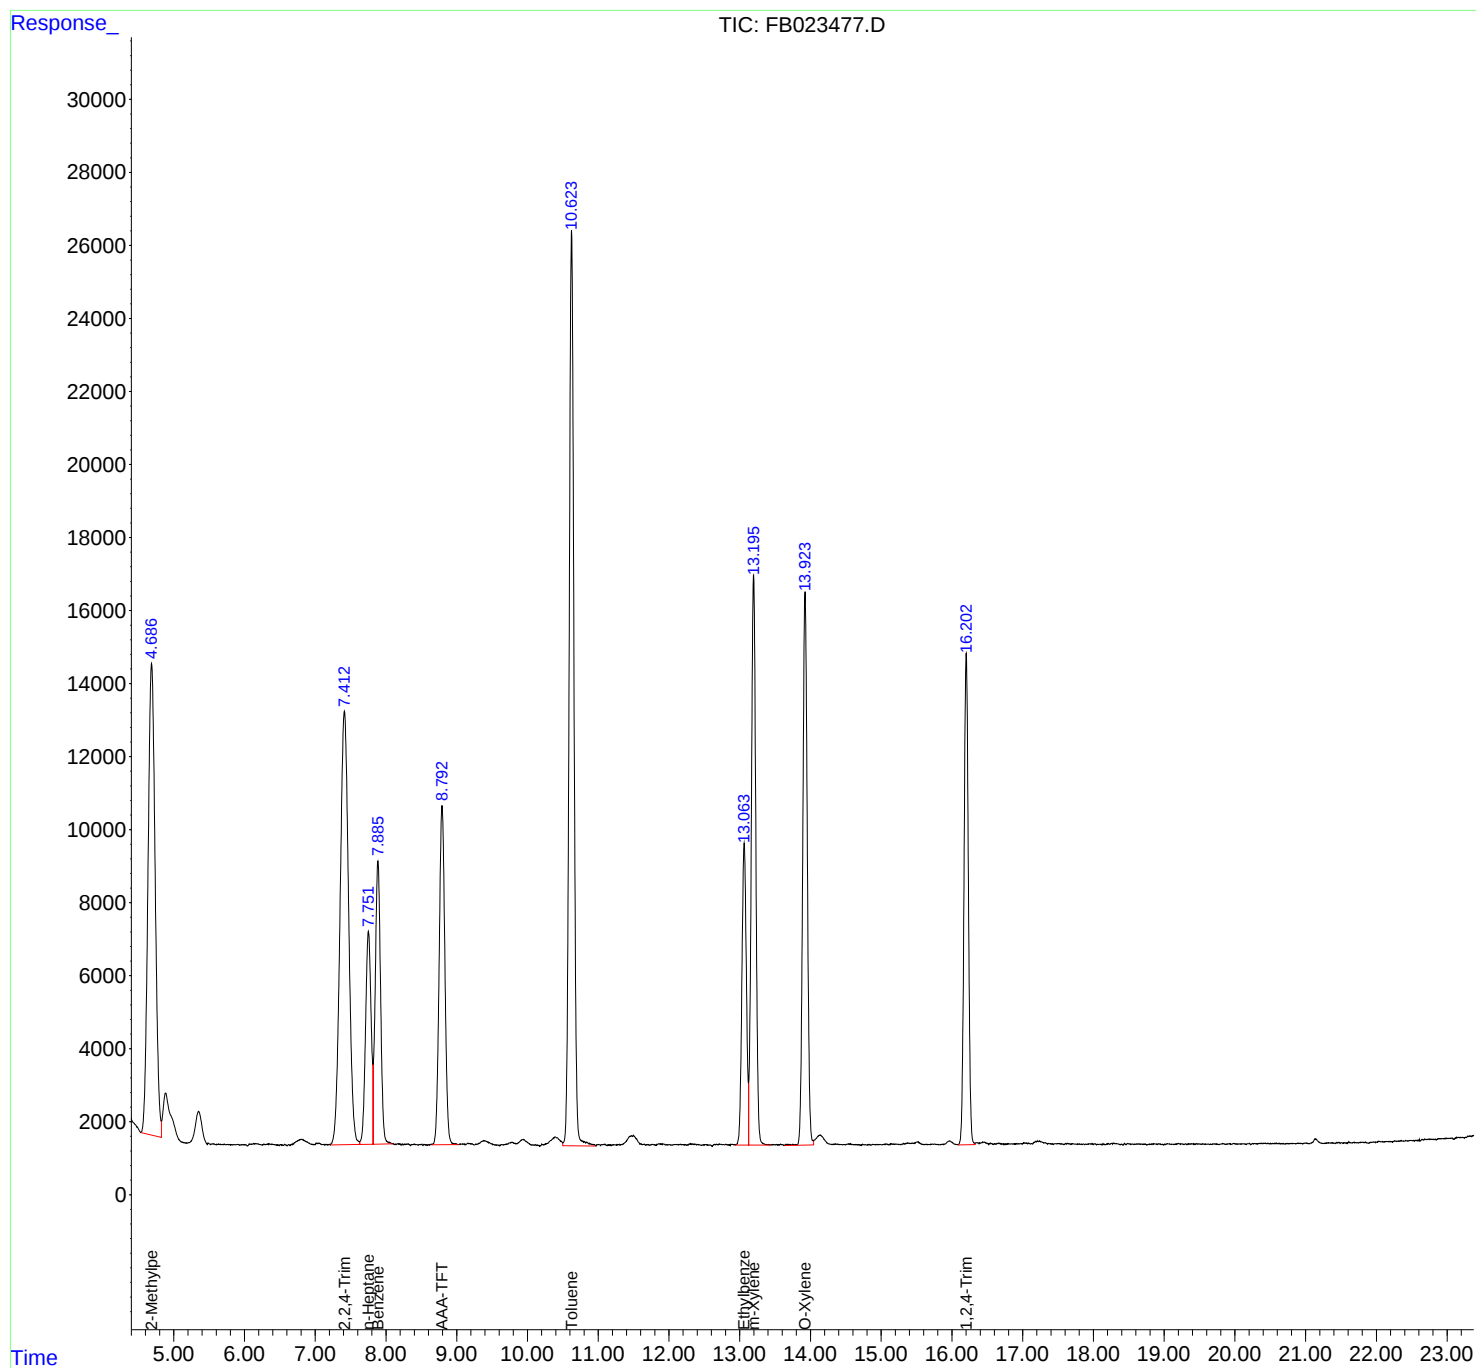

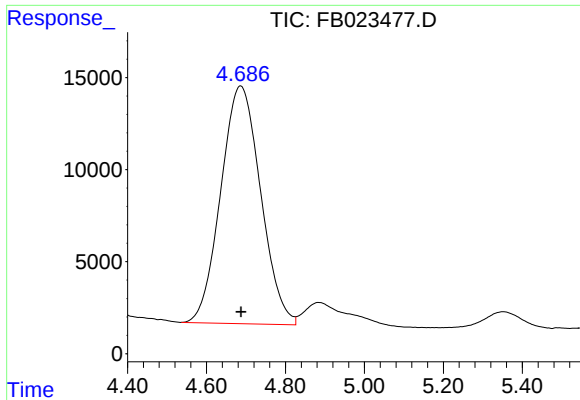


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 905233
Conc: 28.65 ng/ml

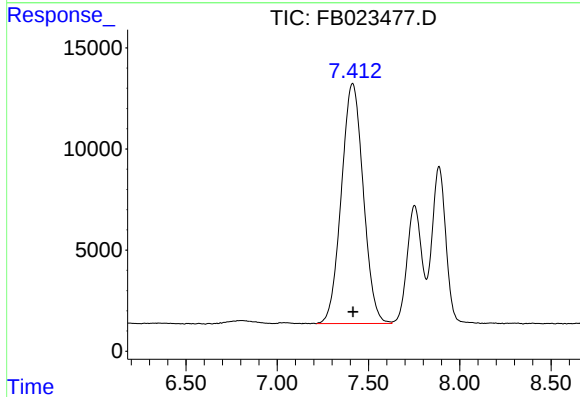


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.002 min
Response: 989469
Conc: 29.14 ng/ml

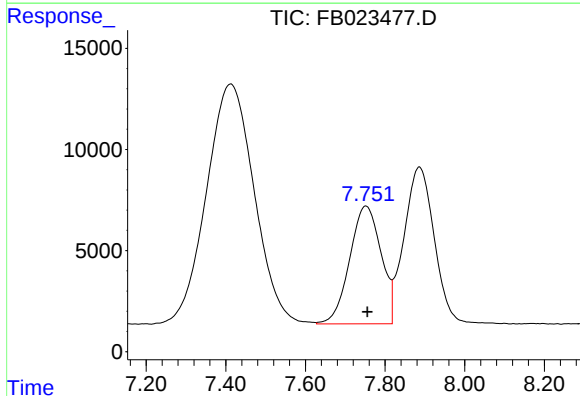


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 319016
Conc: 9.53 ng/ml

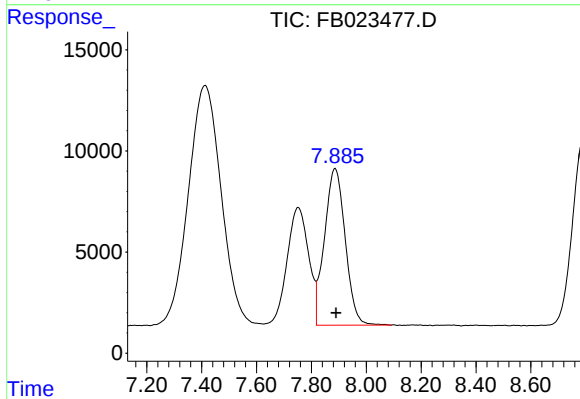


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 407087
Conc: 9.97 ng/ml

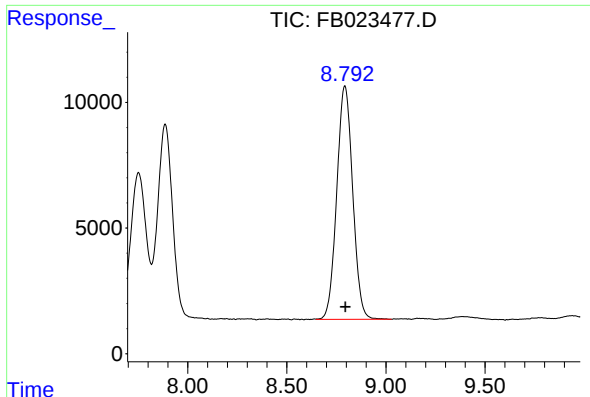


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 518372
Conc: 21.82 ng/ml

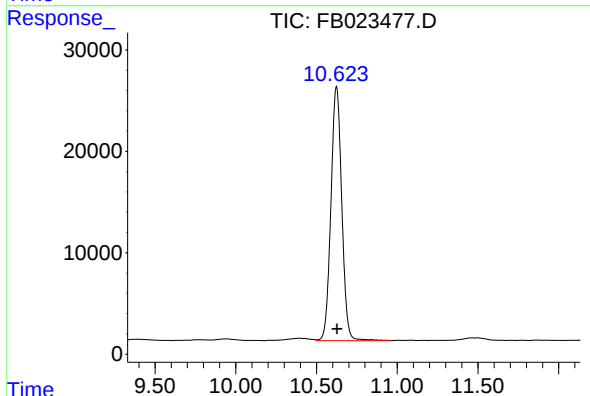


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 1170114
Conc: 29.61 ng/ml

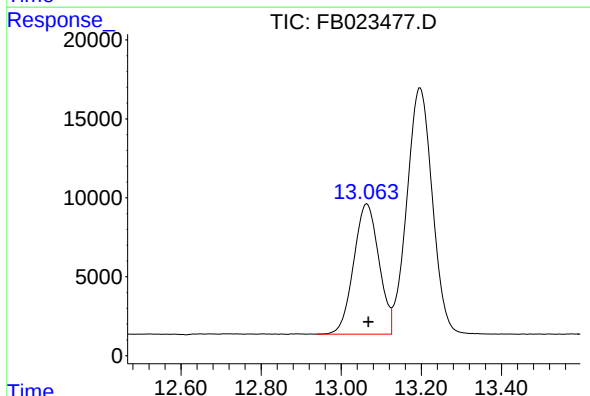


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.004 min
Response: 361051
Conc: 9.67 ng/ml

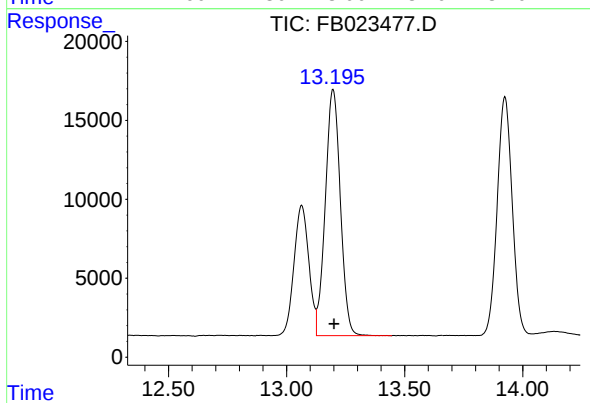


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.004 min
Response: 691286
Conc: 19.44 ng/ml

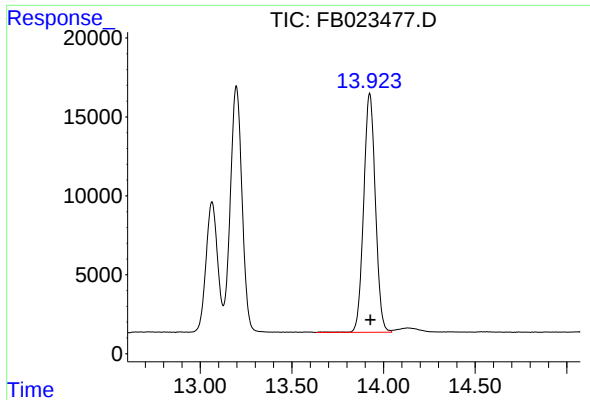

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.004 min
Response: 673764
Conc: 19.50 ng/ml

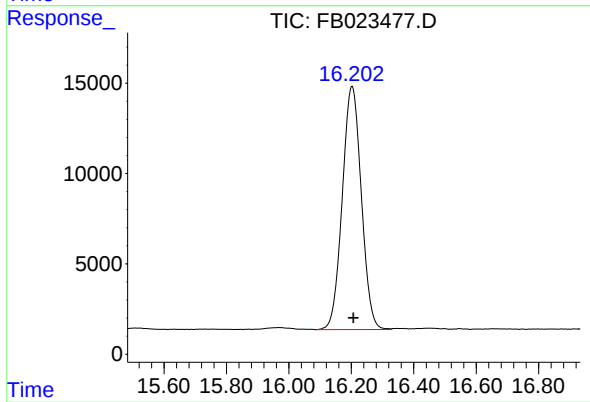

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.004 min
Response: 570208
Conc: 19.50 ng/ml