

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012220\
 Data File : FB023472.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jan 2020 9:38
 Operator : DD/AJ
 Sample : BSF0122S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 23 00:17:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	452001	19.029 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	860587	27.233 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	950760	28.002 ng/ml
3) t n-Heptane	7.752	308608	9.216 ng/ml
4) t Benzene	7.886	378470	9.268 ng/ml
6) t Toluene	10.624	1119639	28.332 ng/ml
7) t Ethylbenzene	13.063	356087	9.534 ng/ml
8) t m-Xylene	13.197	688333	19.356 ng/ml
9) t O-Xylene	13.924	666142	19.279 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	574815	19.658 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012220\
Data File : FB023472.D
Signal(s) : FID2B.CH
Acq On : 22 Jan 2020 9:38
Operator : DD/AJ
Sample : BSF0122S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 23 00:17:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

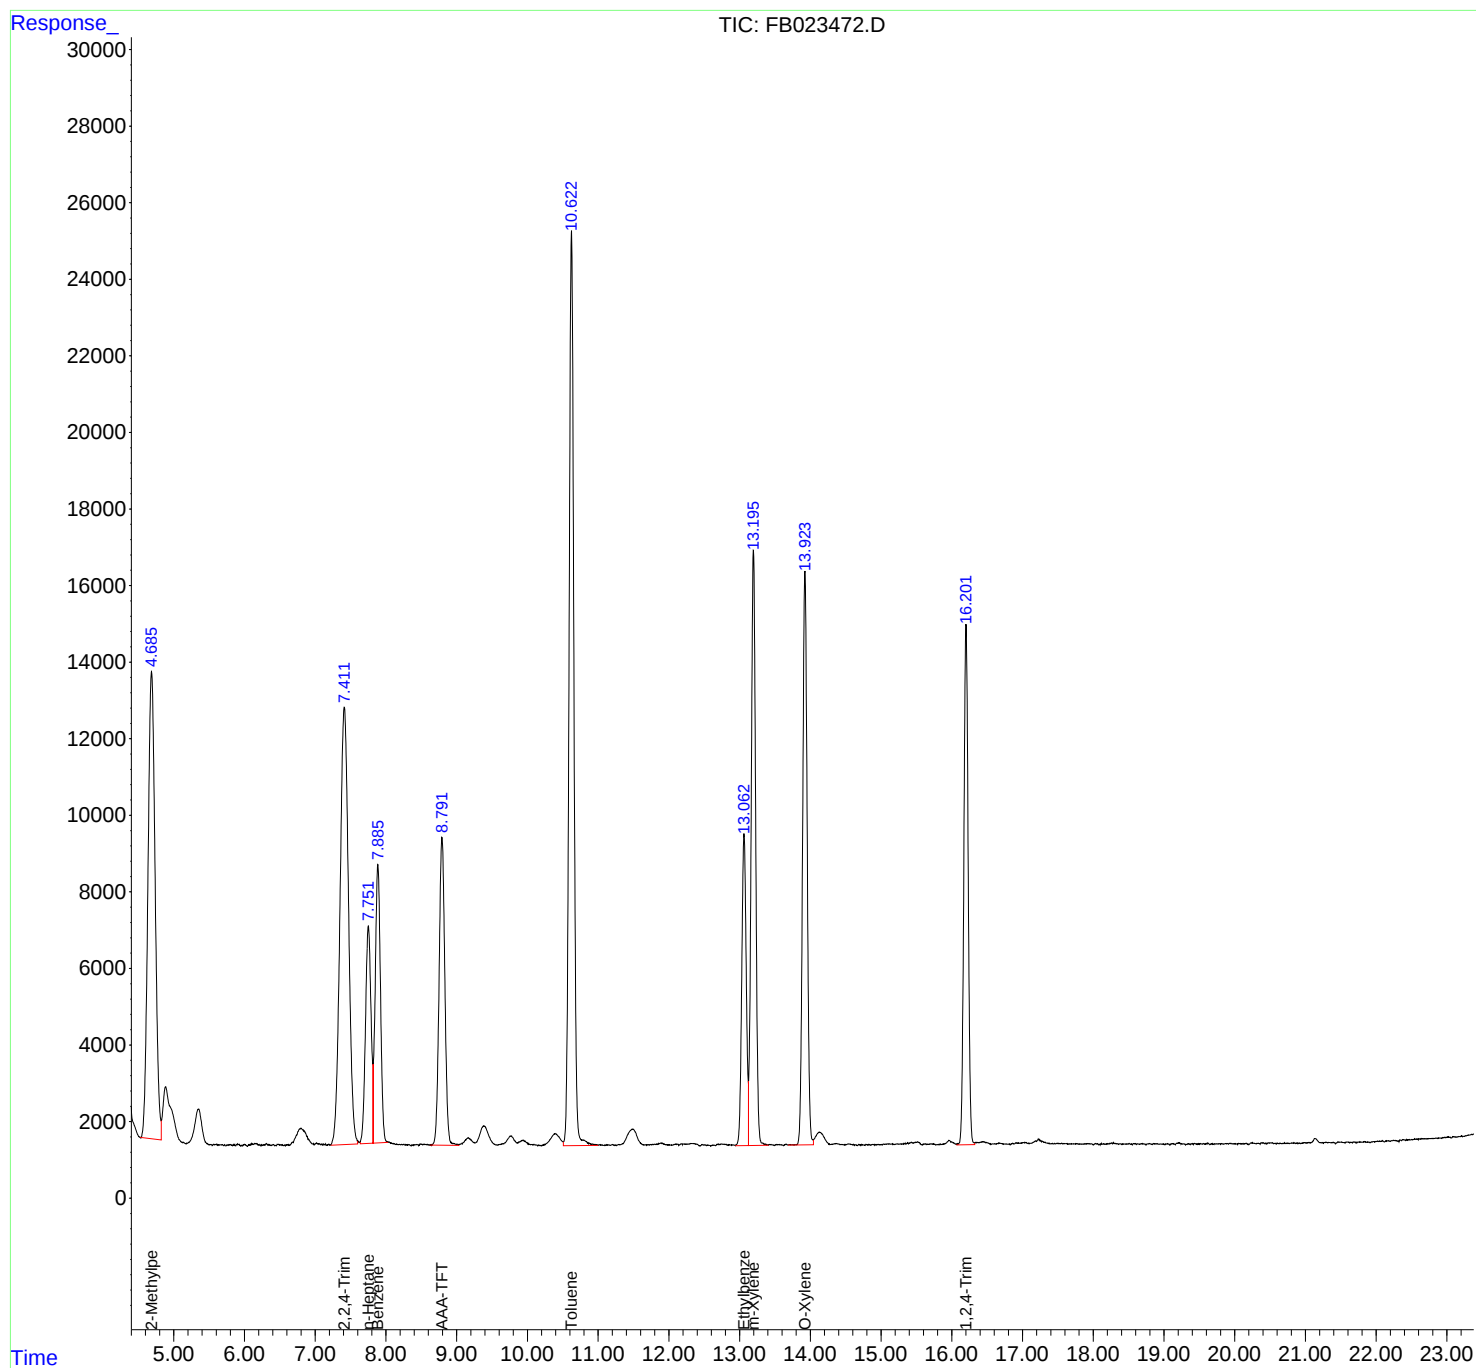

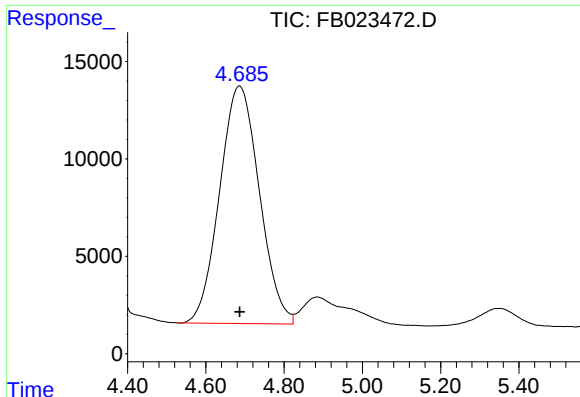


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 860587
Conc: 27.23 ng/ml

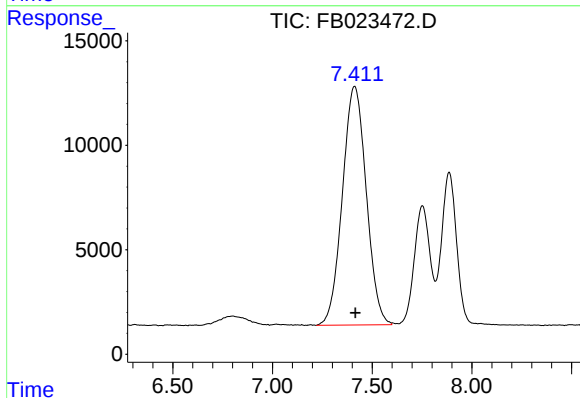


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.003 min
Response: 950760
Conc: 28.00 ng/ml

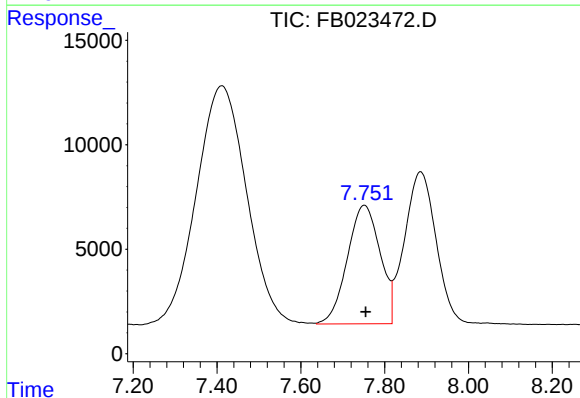


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 308608
Conc: 9.22 ng/ml

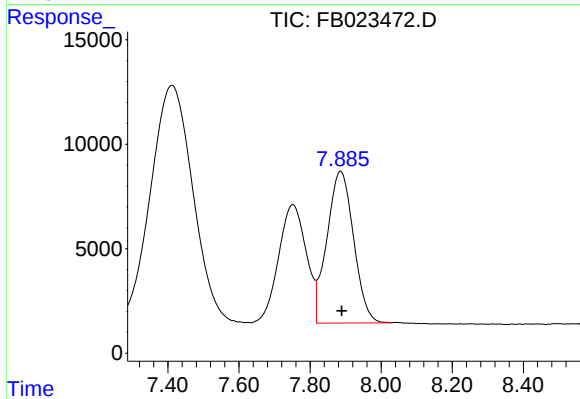


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 378470
Conc: 9.27 ng/ml

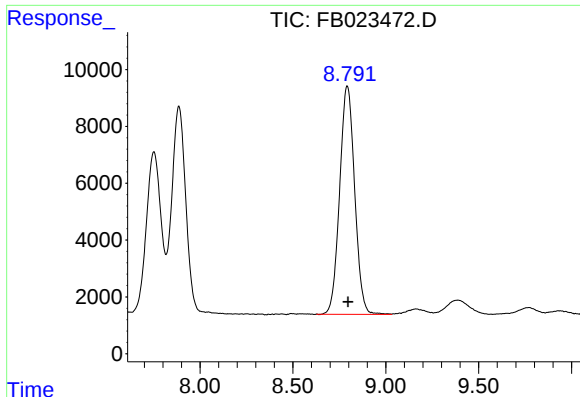


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 452001
Conc: 19.03 ng/ml

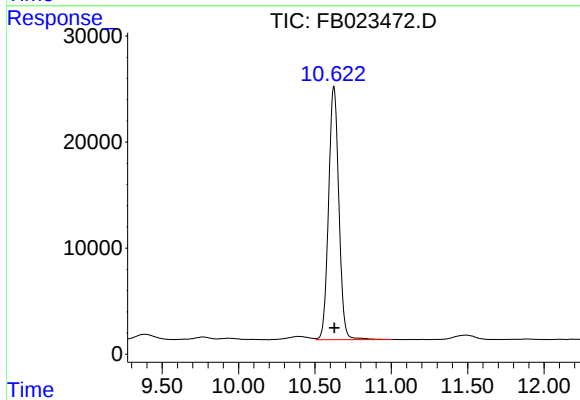


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 1119639
Conc: 28.33 ng/ml

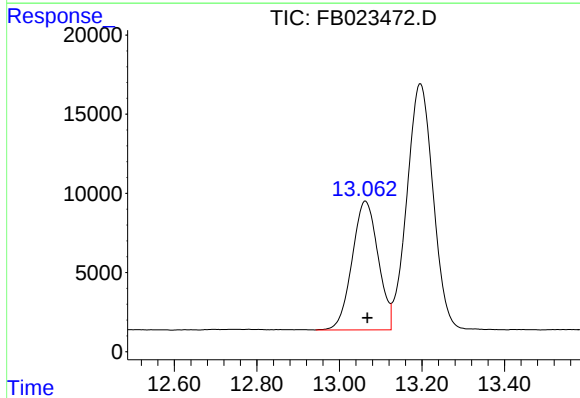


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.005 min
Response: 356087
Conc: 9.53 ng/ml

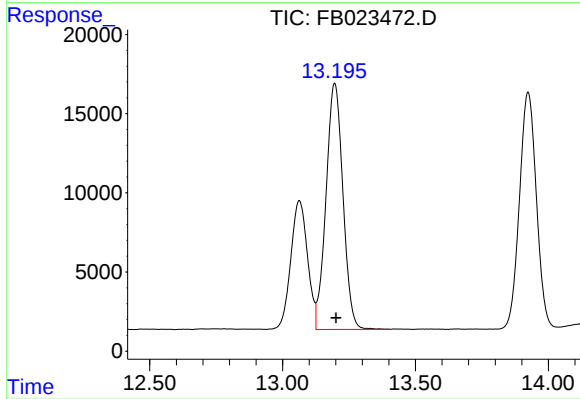


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.004 min
Response: 688333
Conc: 19.36 ng/ml

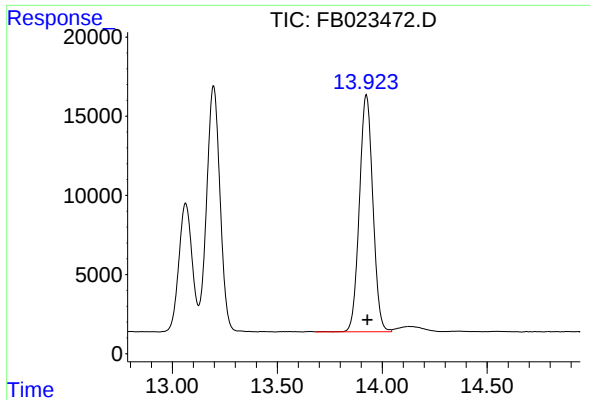

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.004 min
Response: 666142
Conc: 19.28 ng/ml

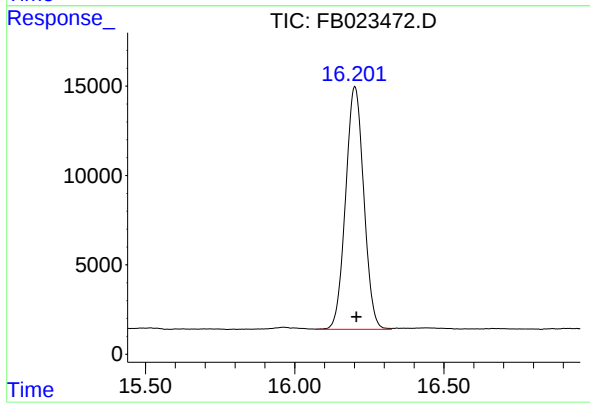

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 574815
Conc: 19.66 ng/ml