

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012320\
 Data File : FB023482.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jan 2020 12:31
 Operator : DD/AJ
 Sample : BSF0123S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 24 00:12:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	506165	21.309 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	965974	30.568 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	1078619	31.768 ng/ml
3) t n-Heptane	7.752	354283	10.580 ng/ml
4) t Benzene	7.887	425484	10.419 ng/ml
6) t Toluene	10.624	1215193	30.750 ng/ml
7) t Ethylbenzene	13.064	385174	10.313 ng/ml
8) t m-Xylene	13.197	733826	20.636 ng/ml
9) t O-Xylene	13.925	707095	20.464 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	610312	20.872 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012320\
Data File : FB023482.D
Signal(s) : FID2B.CH
Acq On : 23 Jan 2020 12:31
Operator : DD/AJ
Sample : BSF0123S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 24 00:12:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

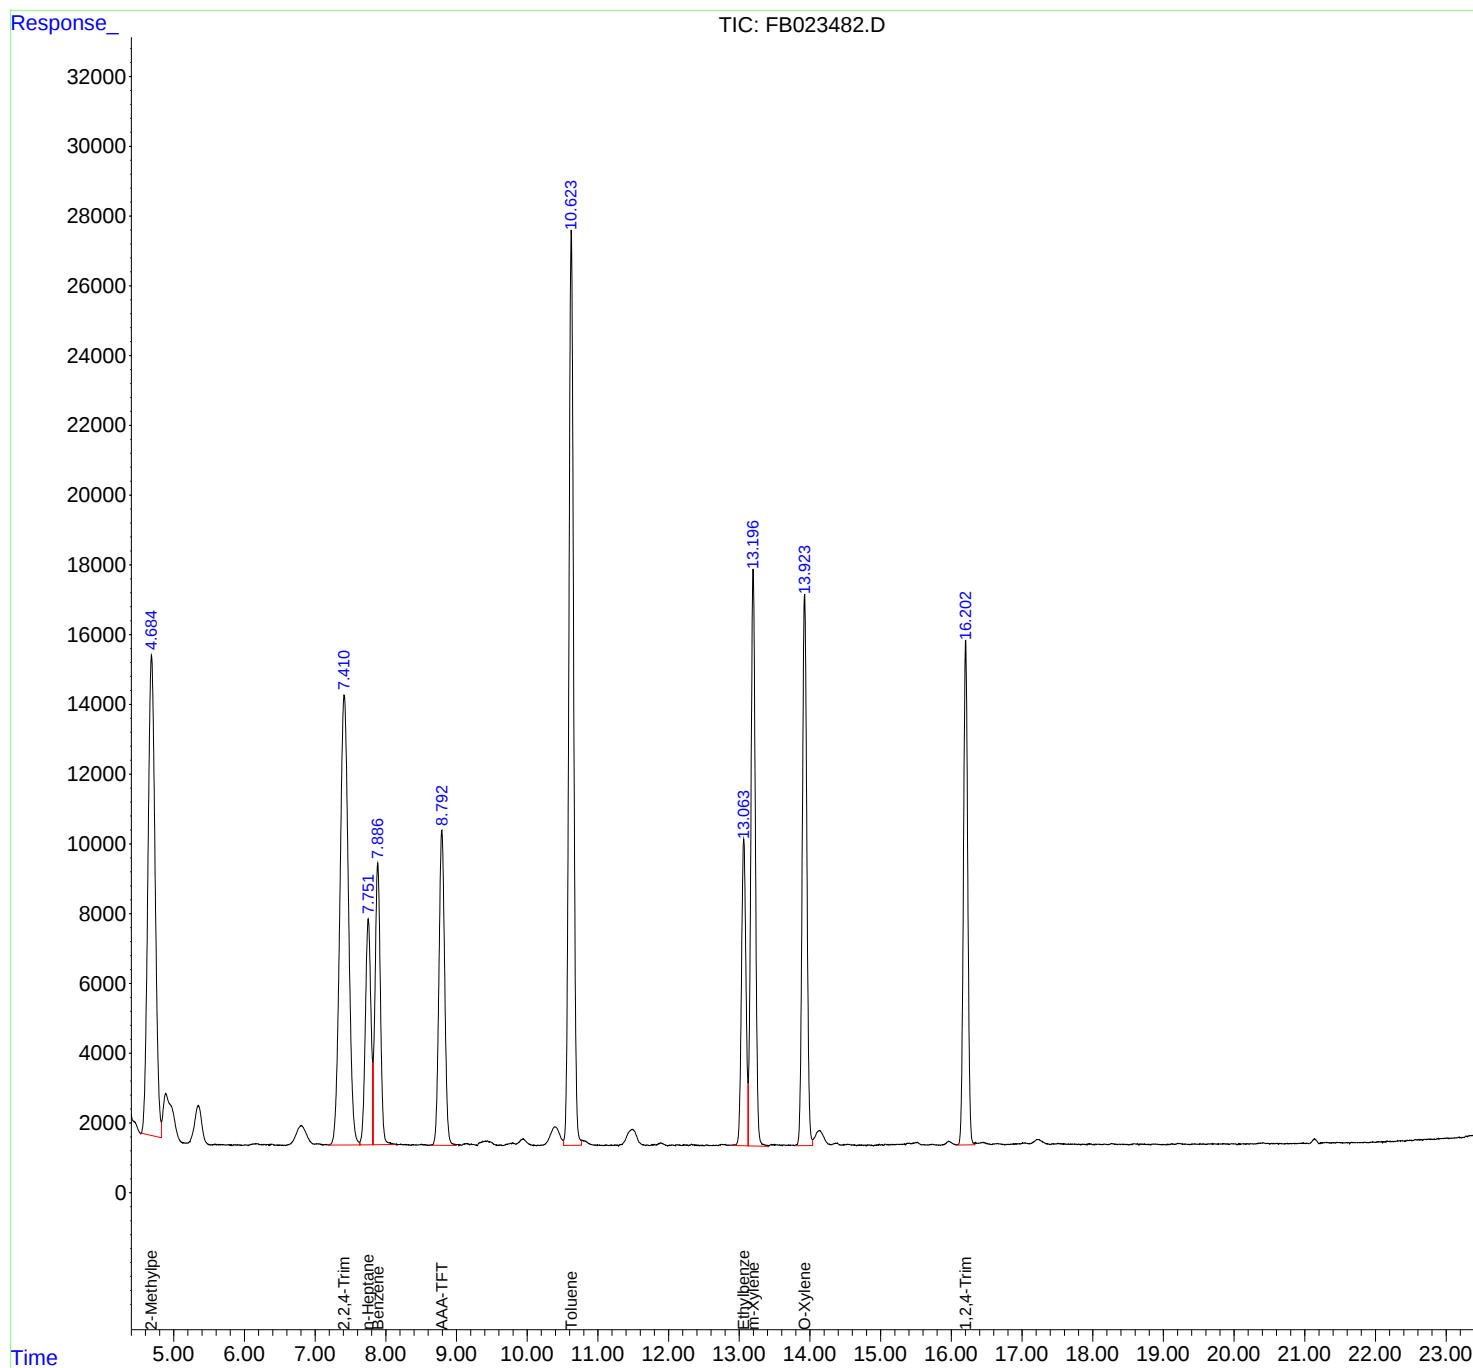

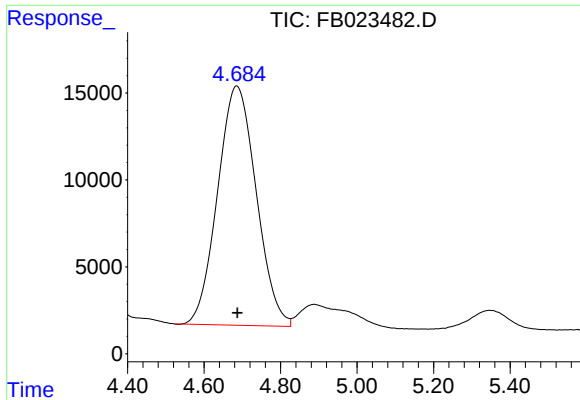


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.001 min
Response: 965974
Conc: 30.57 ng/ml

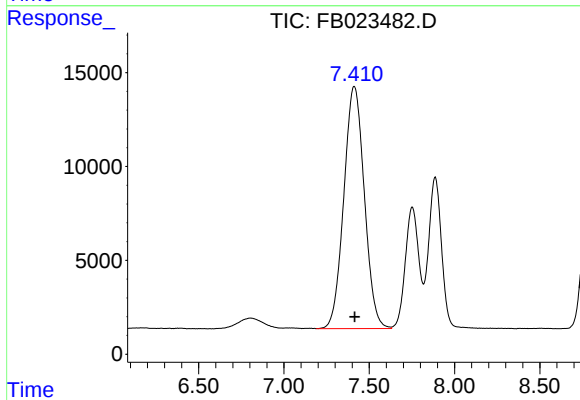


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.004 min
Response: 1078619
Conc: 31.77 ng/ml

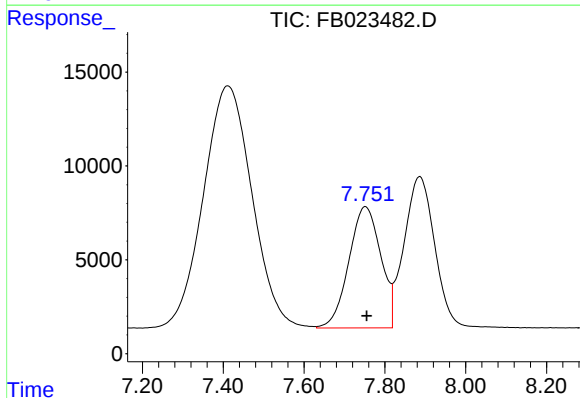


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 354283
Conc: 10.58 ng/ml

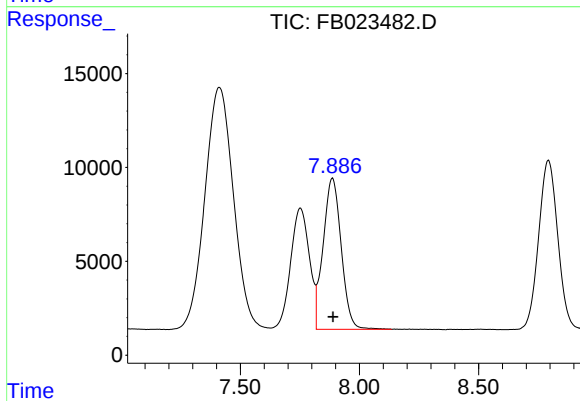


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 425484
Conc: 10.42 ng/ml

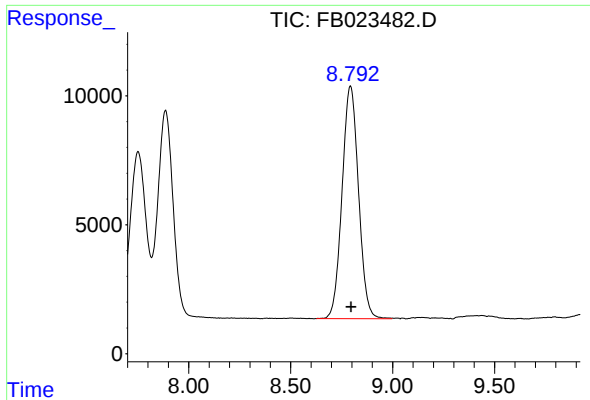


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.003 min
Response: 506165
Conc: 21.31 ng/ml

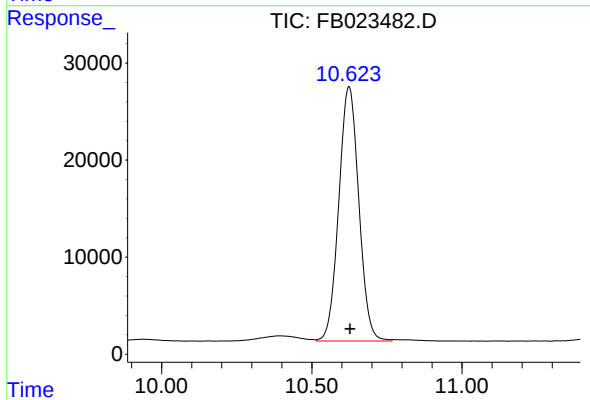


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 1215193
Conc: 30.75 ng/ml

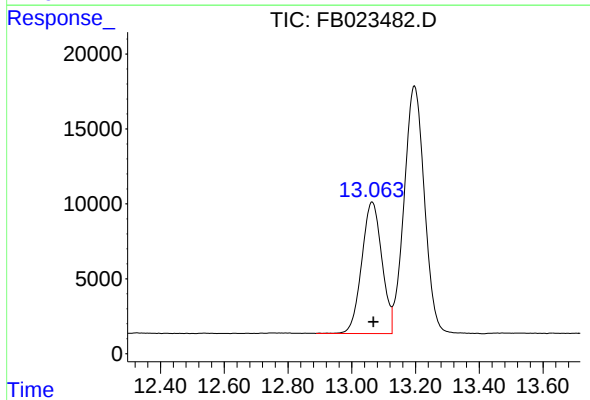


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.004 min
Response: 385174
Conc: 10.31 ng/ml

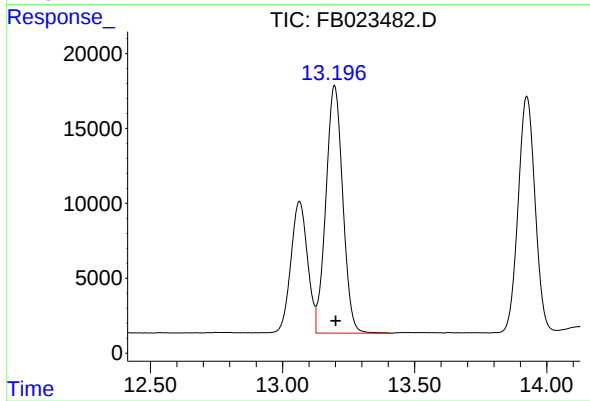


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.004 min
Response: 733826
Conc: 20.64 ng/ml

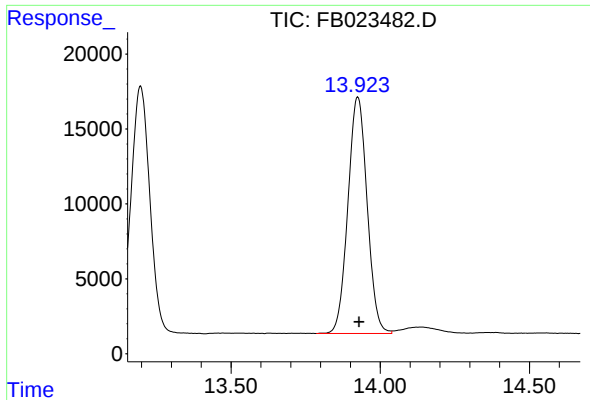

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.004 min
Response: 707095
Conc: 20.46 ng/ml

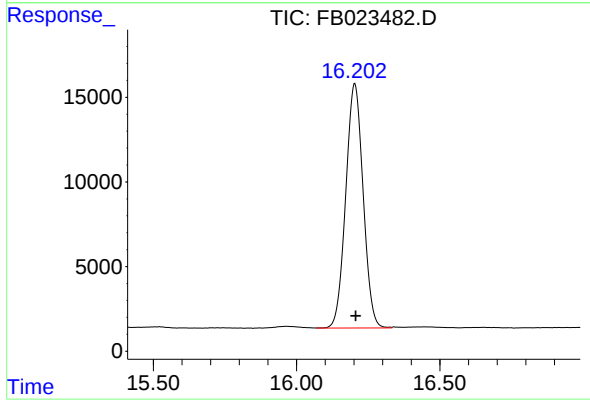

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.004 min
Response: 610312
Conc: 20.87 ng/ml