

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012320\
 Data File : FB023483.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jan 2020 13:14
 Operator : DD/AJ
 Sample : L1161-01
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 24 00:12:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	21165	0.891 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	50179	1.588 ng/ml
2) t	2,2,4-Trimethylpentane	7.405	44656	1.315 ng/ml
3) t	n-Heptane	7.756	13960	0.417 ng/ml
4) t	Benzene	7.887	19250	0.471 ng/ml
6) t	Toluene	10.626	59349	1.502 ng/ml
7) t	Ethylbenzene	13.065	19686	0.527 ng/ml
8) t	m-Xylene	13.199	36963	1.039 ng/ml
9) t	O-Xylene	13.925	37952	1.098 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	33480	1.145 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012320\
Data File : FB023483.D
Signal(s) : FID2B.CH
Acq On : 23 Jan 2020 13:14
Operator : DD/AJ
Sample : L1161-01
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 24 00:12:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

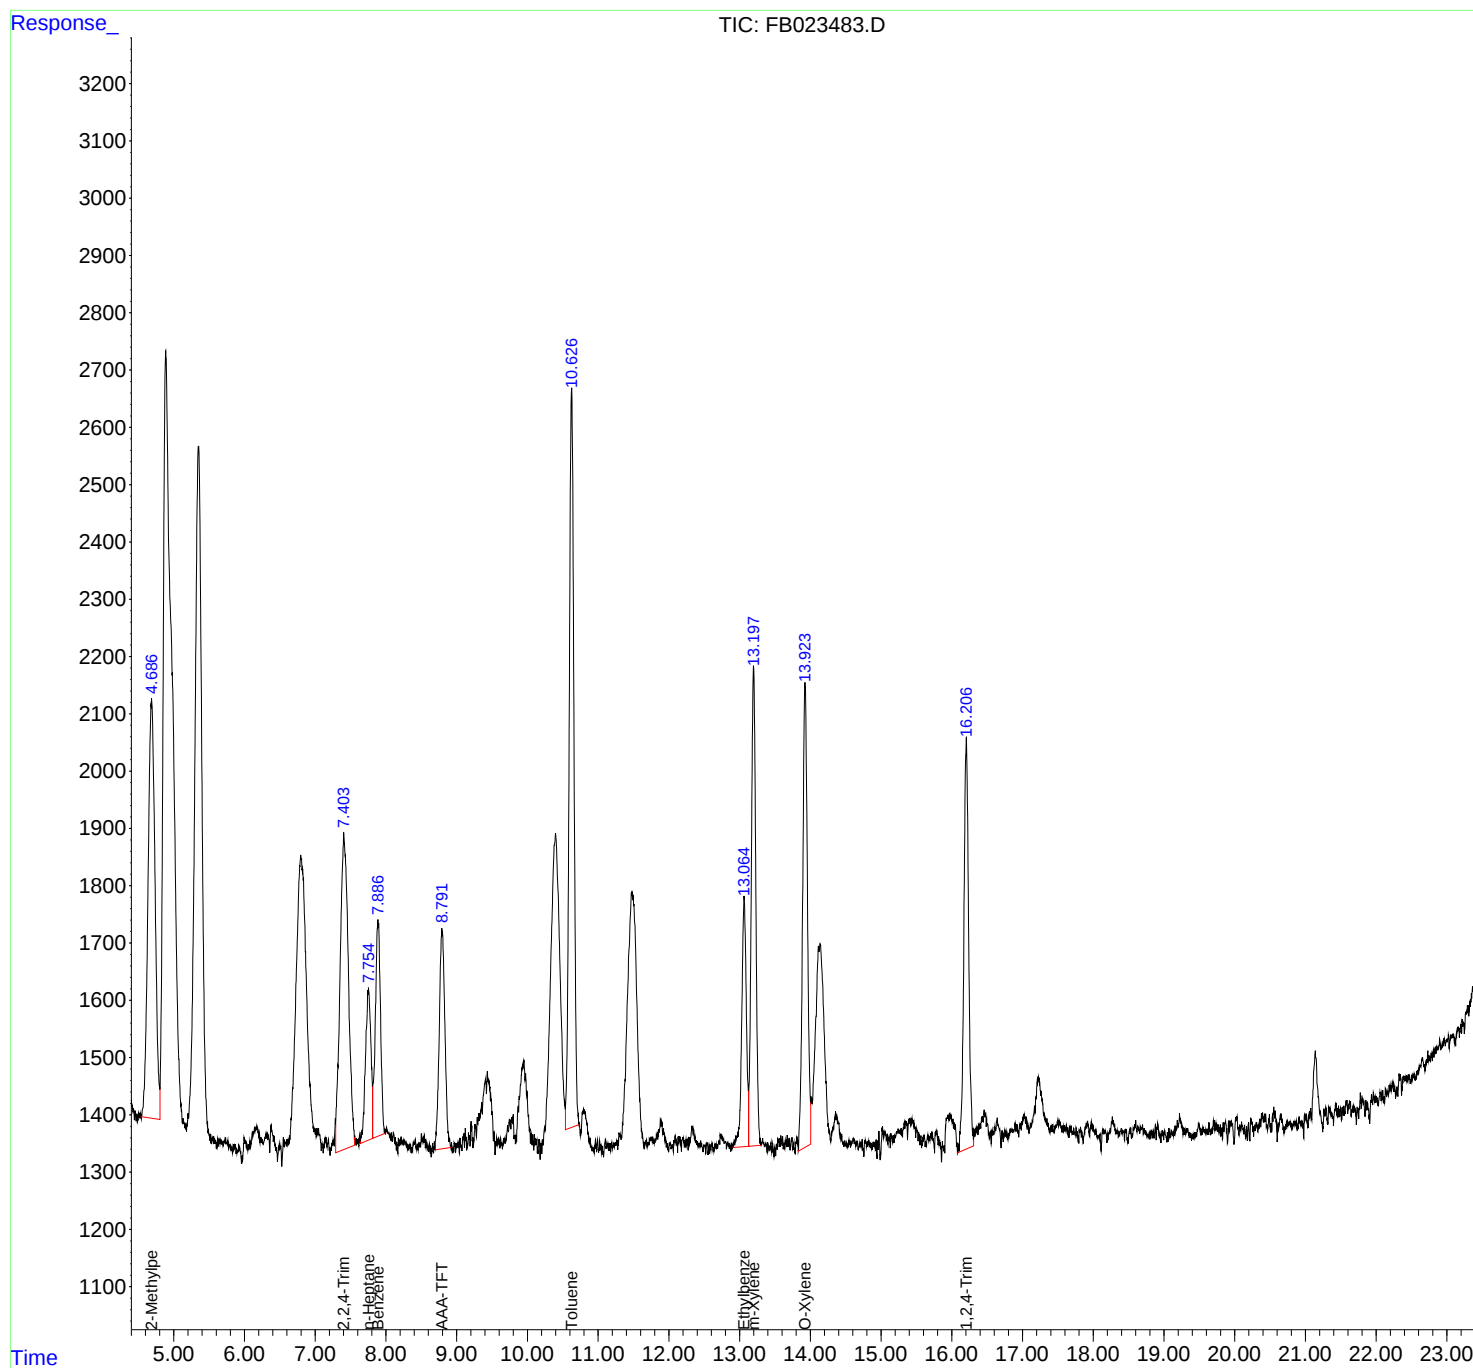

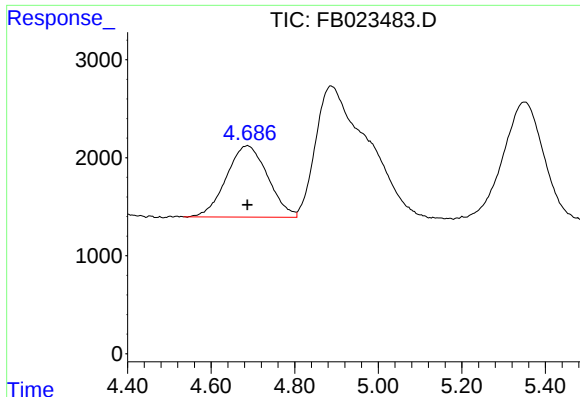


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 50179
Conc: 1.59 ng/ml

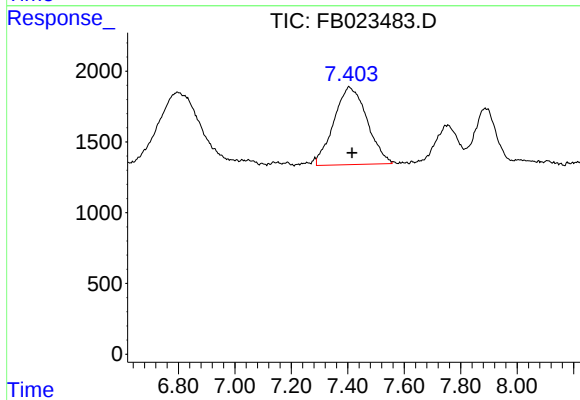


#2 2,2,4-Trimethylpentane

R.T.: 7.405 min
Delta R.T.: -0.010 min
Response: 44656
Conc: 1.32 ng/ml

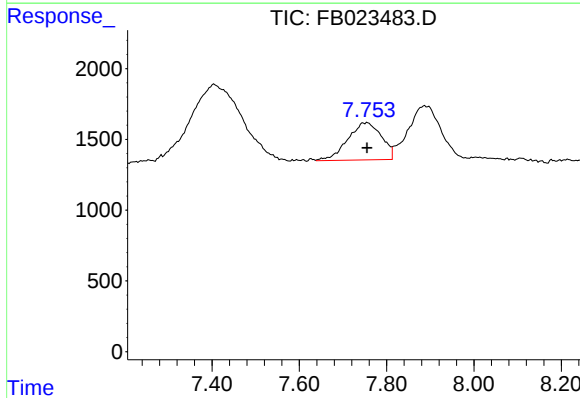


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 13960
Conc: 0.42 ng/ml

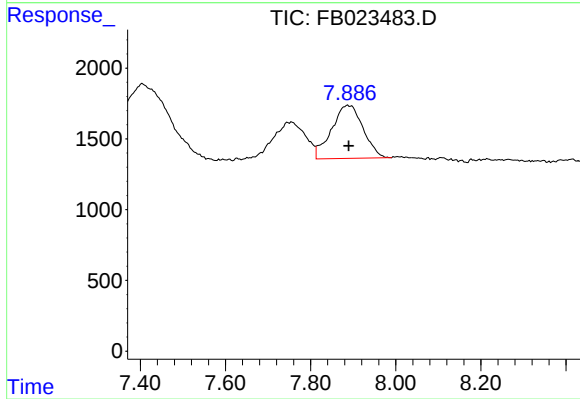


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.002 min
Response: 19250
Conc: 0.47 ng/ml

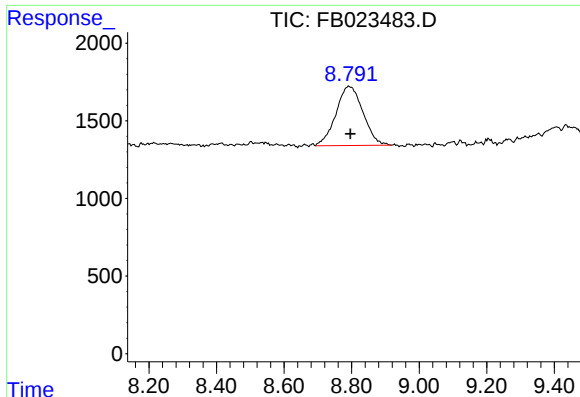


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.004 min
Response: 21165
Conc: 0.89 ng/ml

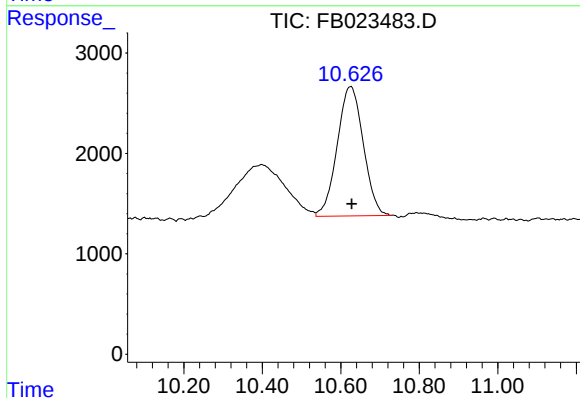


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 59349
Conc: 1.50 ng/ml

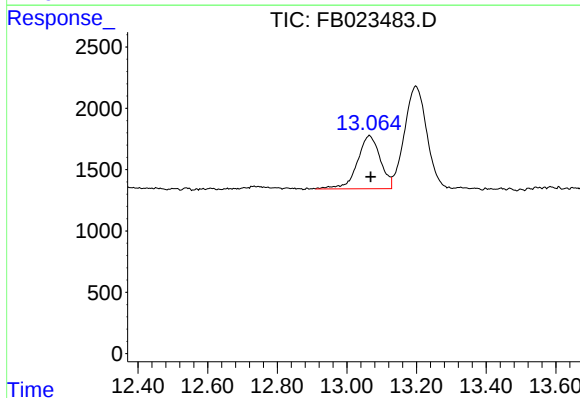


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 19686
Conc: 0.53 ng/ml

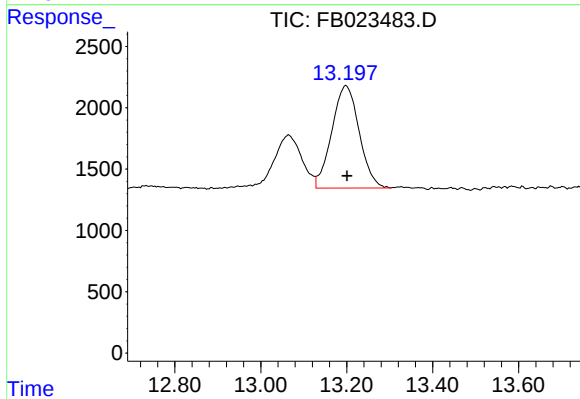


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 36963
Conc: 1.04 ng/ml

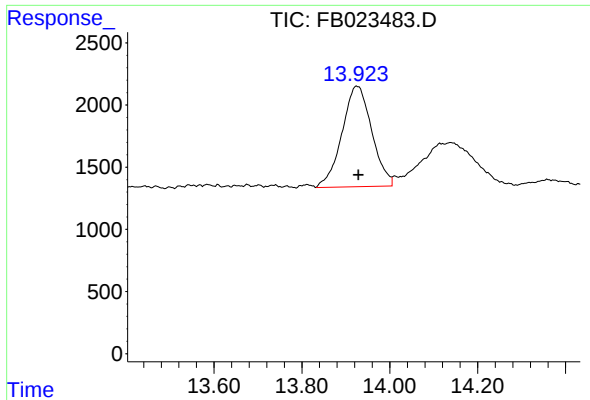

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.004 min
Response: 37952
Conc: 1.10 ng/ml

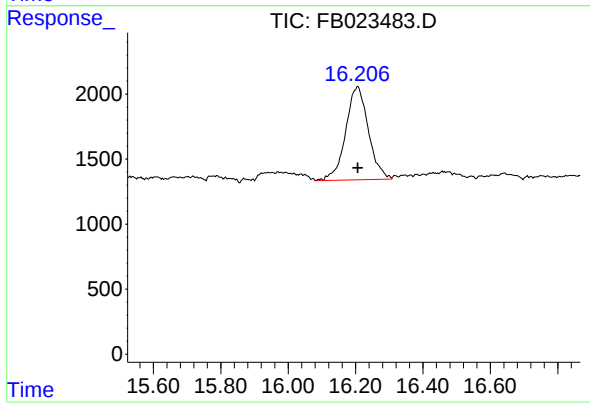

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 33480
Conc: 1.14 ng/ml