

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012323\
 Data File : FB029158.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jan 2023 12:22
 Operator : AJ/MA
 Sample : BSF0123S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 23 23:50:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	226729	18.555 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	345277	23.584 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	412465	25.996 ng/ml
3) t n-Heptane	7.752	122385	7.324 ng/ml
4) t Benzene	7.888	168066	7.905 ng/ml
6) t Toluene	10.622	491497	24.385 ng/ml
7) t Ethylbenzene	13.059	157400	8.206 ng/ml
8) t m-Xylene	13.192	315488	16.862 ng/ml
9) t O-Xylene	13.918	314585	17.482 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	327677	18.380 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012323\
Data File : FB029158.D
Signal(s) : FID2B.CH
Acq On : 23 Jan 2023 12:22
Operator : AJ/MA
Sample : BSF0123S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 23 23:50:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

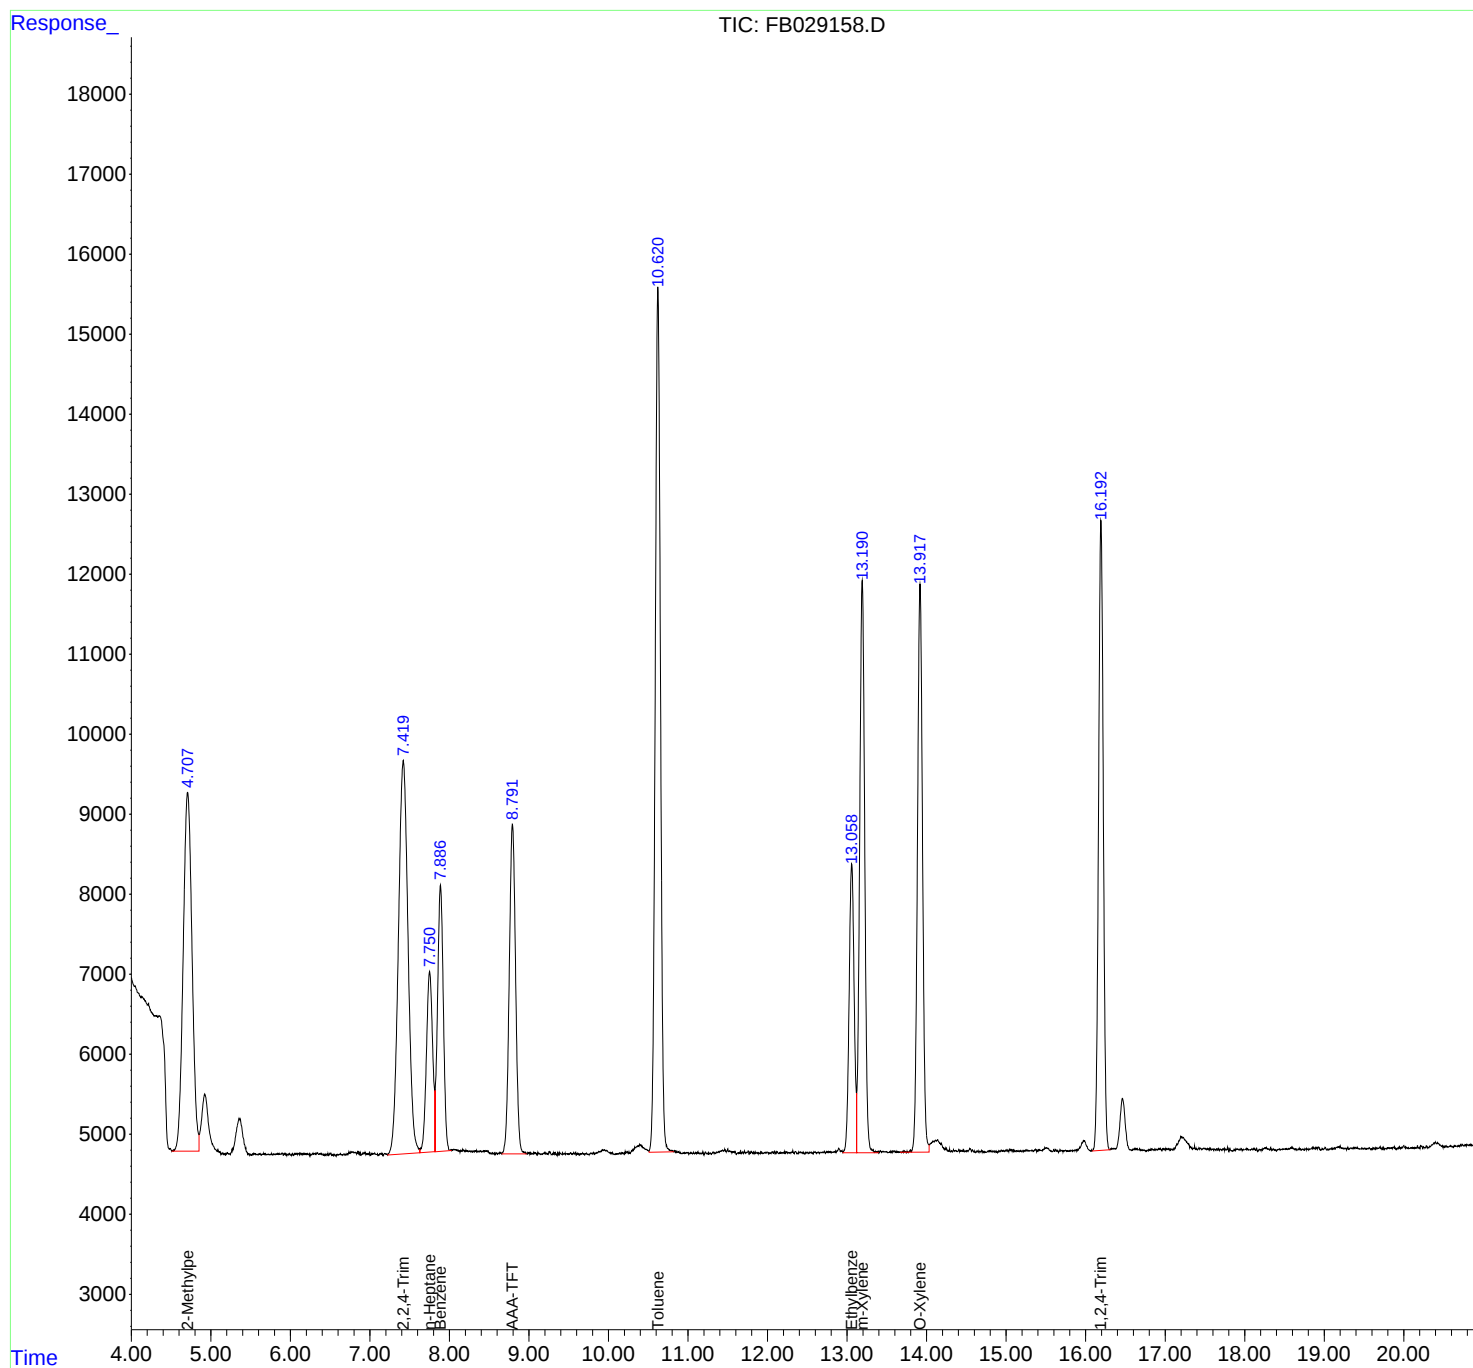

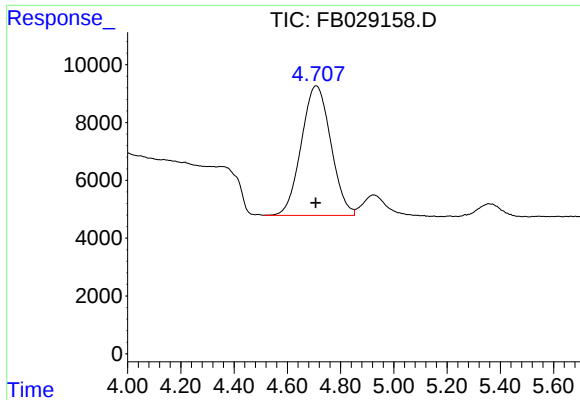


#1 2-Methylpentane

R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 345277
Conc: 23.58 ng/ml

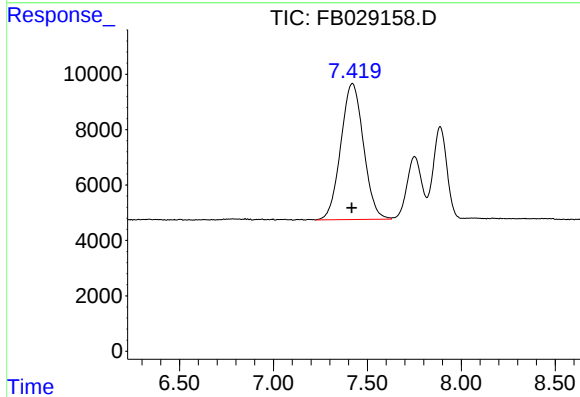


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.003 min
Response: 412465
Conc: 26.00 ng/ml

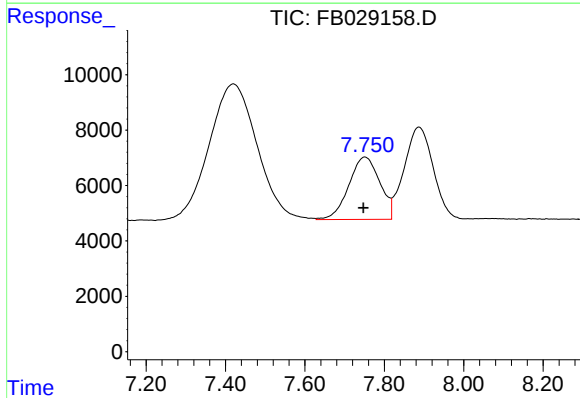


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.004 min
Response: 122385
Conc: 7.32 ng/ml

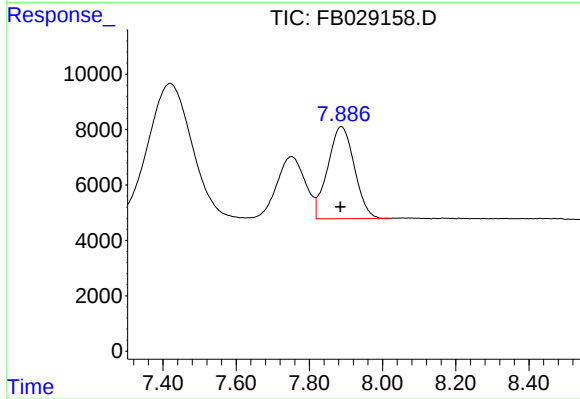


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.003 min
Response: 168066
Conc: 7.91 ng/ml

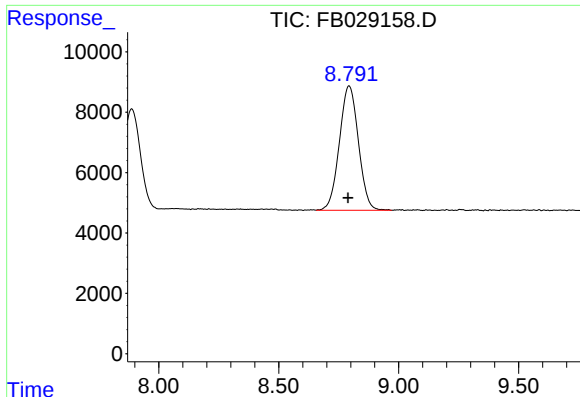


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.004 min
Response: 226729
Conc: 18.55 ng/ml

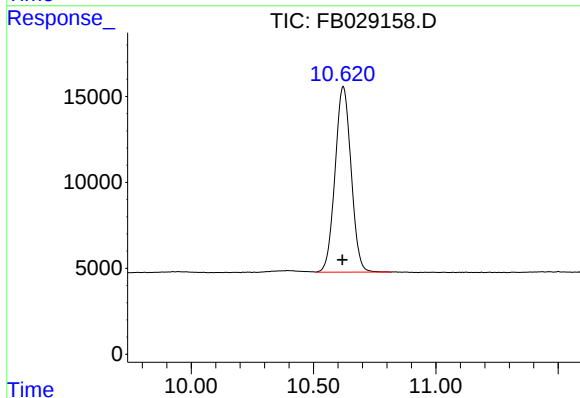


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.004 min
Response: 491497
Conc: 24.39 ng/ml

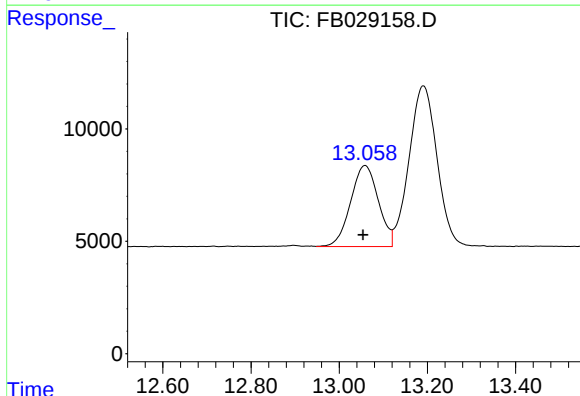


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.005 min
Response: 157400
Conc: 8.21 ng/ml

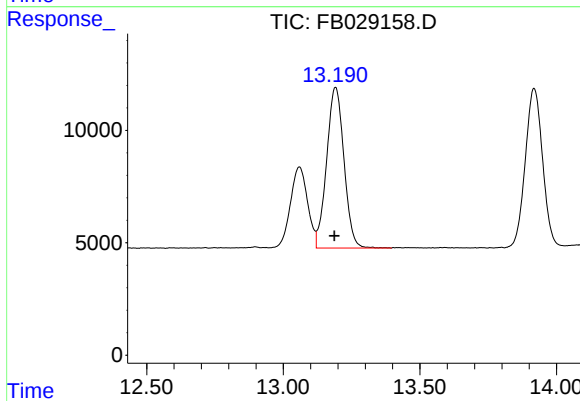


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 315488
Conc: 16.86 ng/ml

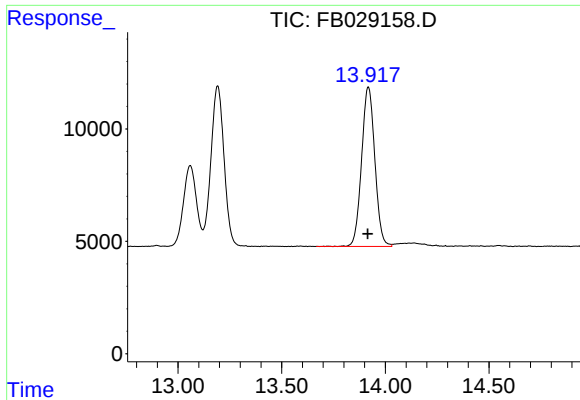

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.004 min
Response: 314585
Conc: 17.48 ng/ml

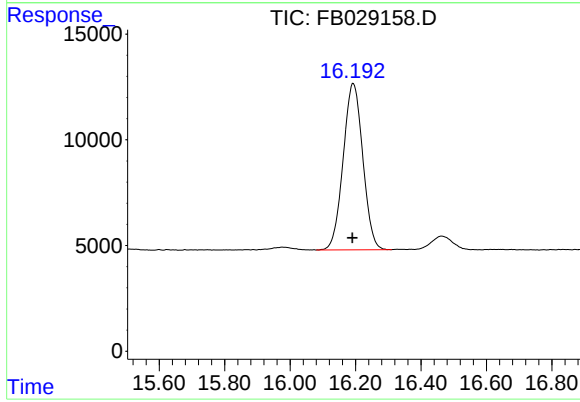

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.004 min
Response: 327677
Conc: 18.38 ng/ml