

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012323\
 Data File : FB029160.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jan 2023 13:39
 Operator : AJ/MA
 Sample : BSF0123S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 23 23:50:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.795	221829	18.154 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.710	378036	25.821 ng/ml
2) t	2,2,4-Trimethylpentane	7.422	460083	28.997 ng/ml
3) t	n-Heptane	7.755	137145	8.208 ng/ml
4) t	Benzene	7.890	187837	8.835 ng/ml
6) t	Toluene	10.623	538480	26.716 ng/ml
7) t	Ethylbenzene	13.059	167789	8.748 ng/ml
8) t	m-Xylene	13.193	334686	17.888 ng/ml
9) t	O-Xylene	13.919	330713	18.378 ng/ml
10) t	1,2,4-Trimethylbenzene	16.195	327530	18.372 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012323\
Data File : FB029160.D
Signal(s) : FID2B.CH
Acq On : 23 Jan 2023 13:39
Operator : AJ/MA
Sample : BSF0123S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 23 23:50:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

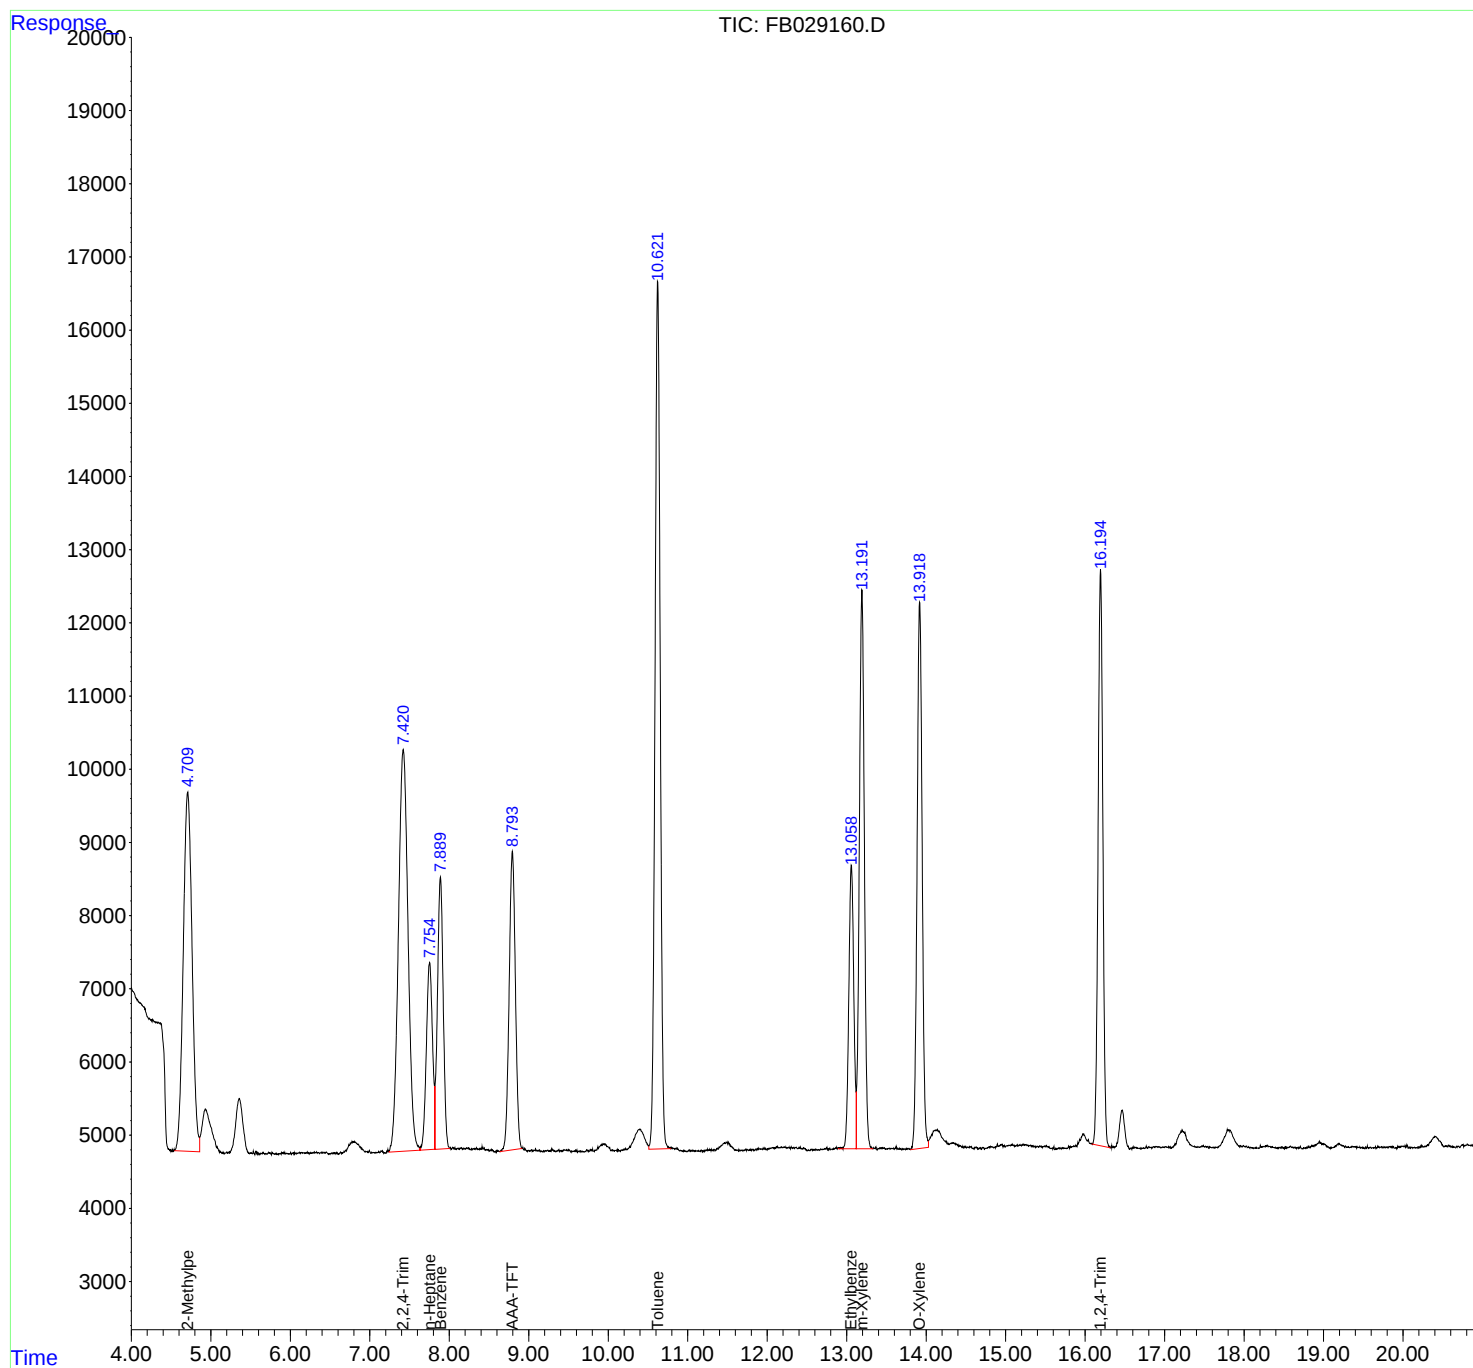

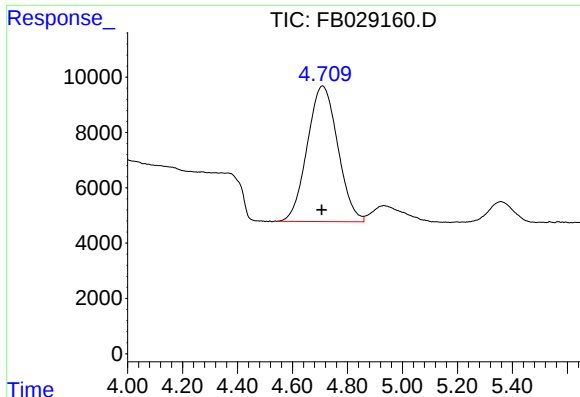


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 378036
Conc: 25.82 ng/ml

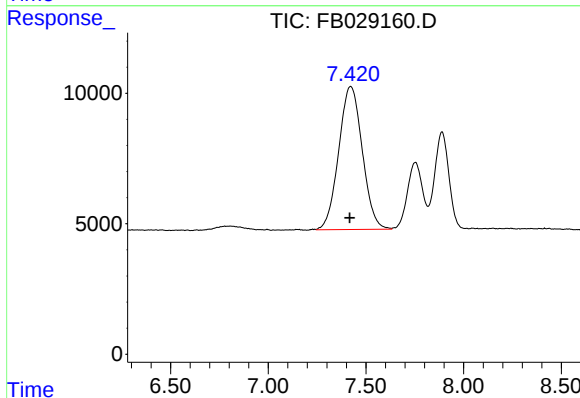


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.004 min
Response: 460083
Conc: 29.00 ng/ml

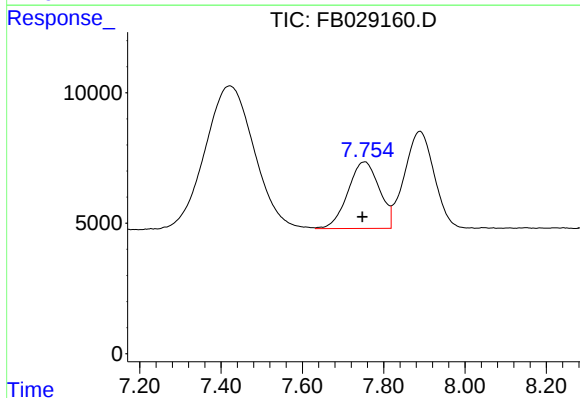


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.007 min
Response: 137145
Conc: 8.21 ng/ml

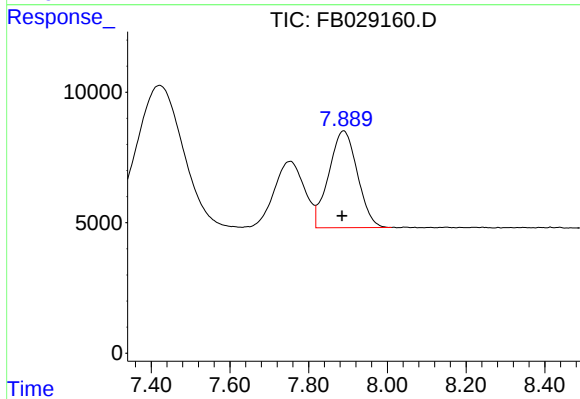


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 187837
Conc: 8.83 ng/ml

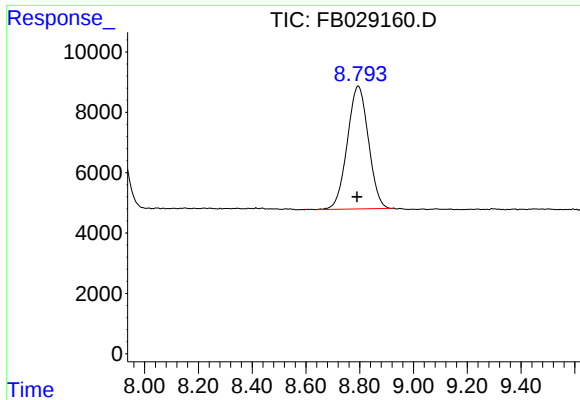


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.005 min
Response: 221829
Conc: 18.15 ng/ml

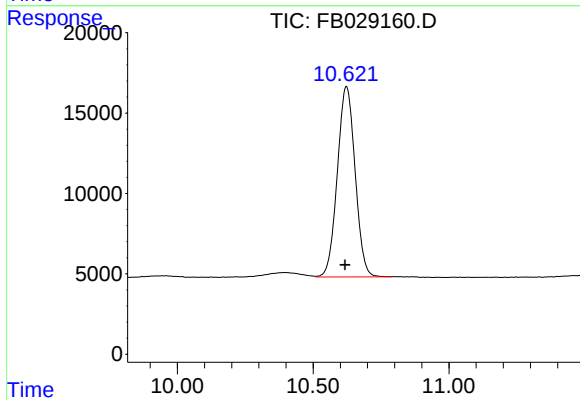


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.005 min
Response: 538480
Conc: 26.72 ng/ml

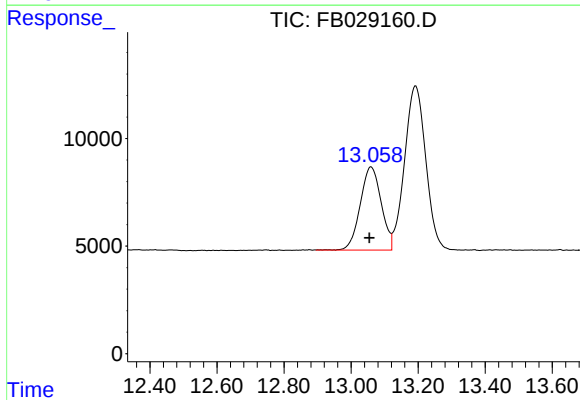


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.005 min
Response: 167789
Conc: 8.75 ng/ml

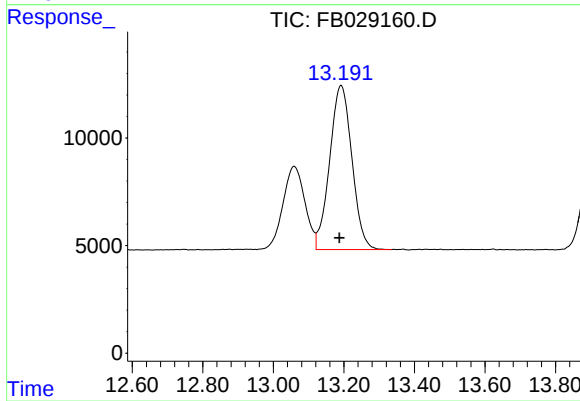

#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.005 min
Response: 334686
Conc: 17.89 ng/ml

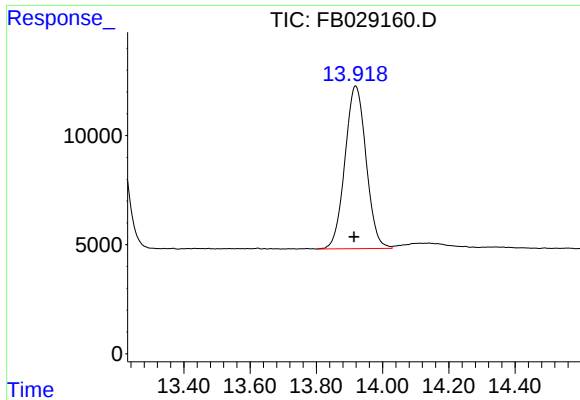


#9 O-Xylene

R.T.: 13.919 min

Delta R.T.: 0.005 min

Response: 330713

Conc: 18.38 ng/ml

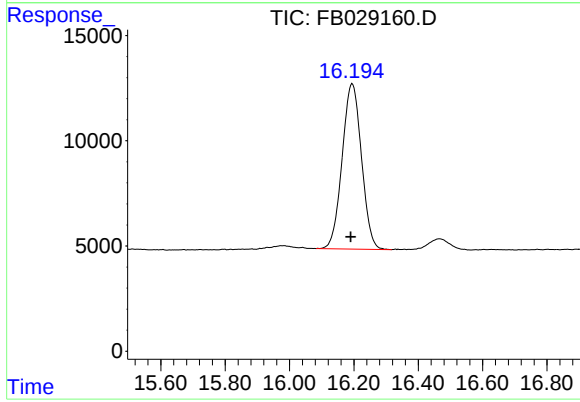

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min

Delta R.T.: 0.005 min

Response: 327530

Conc: 18.37 ng/ml