

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023495.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 10:14
 Operator : DD/AJ
 Sample : L1240-02
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 24 21:46:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	544785	22.935 ng/ml
Target Compounds			
6) t Toluene	10.618	3592	0.091 ng/ml
7) t Ethylbenzene	13.065	3647	0.098 ng/ml
8) t m-Xylene	13.196	9195	0.259 ng/ml
9) t O-Xylene	13.924	8311	0.241 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	8562	0.293 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023495.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 10:14
Operator : DD/AJ
Sample : L1240-02
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 24 21:46:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

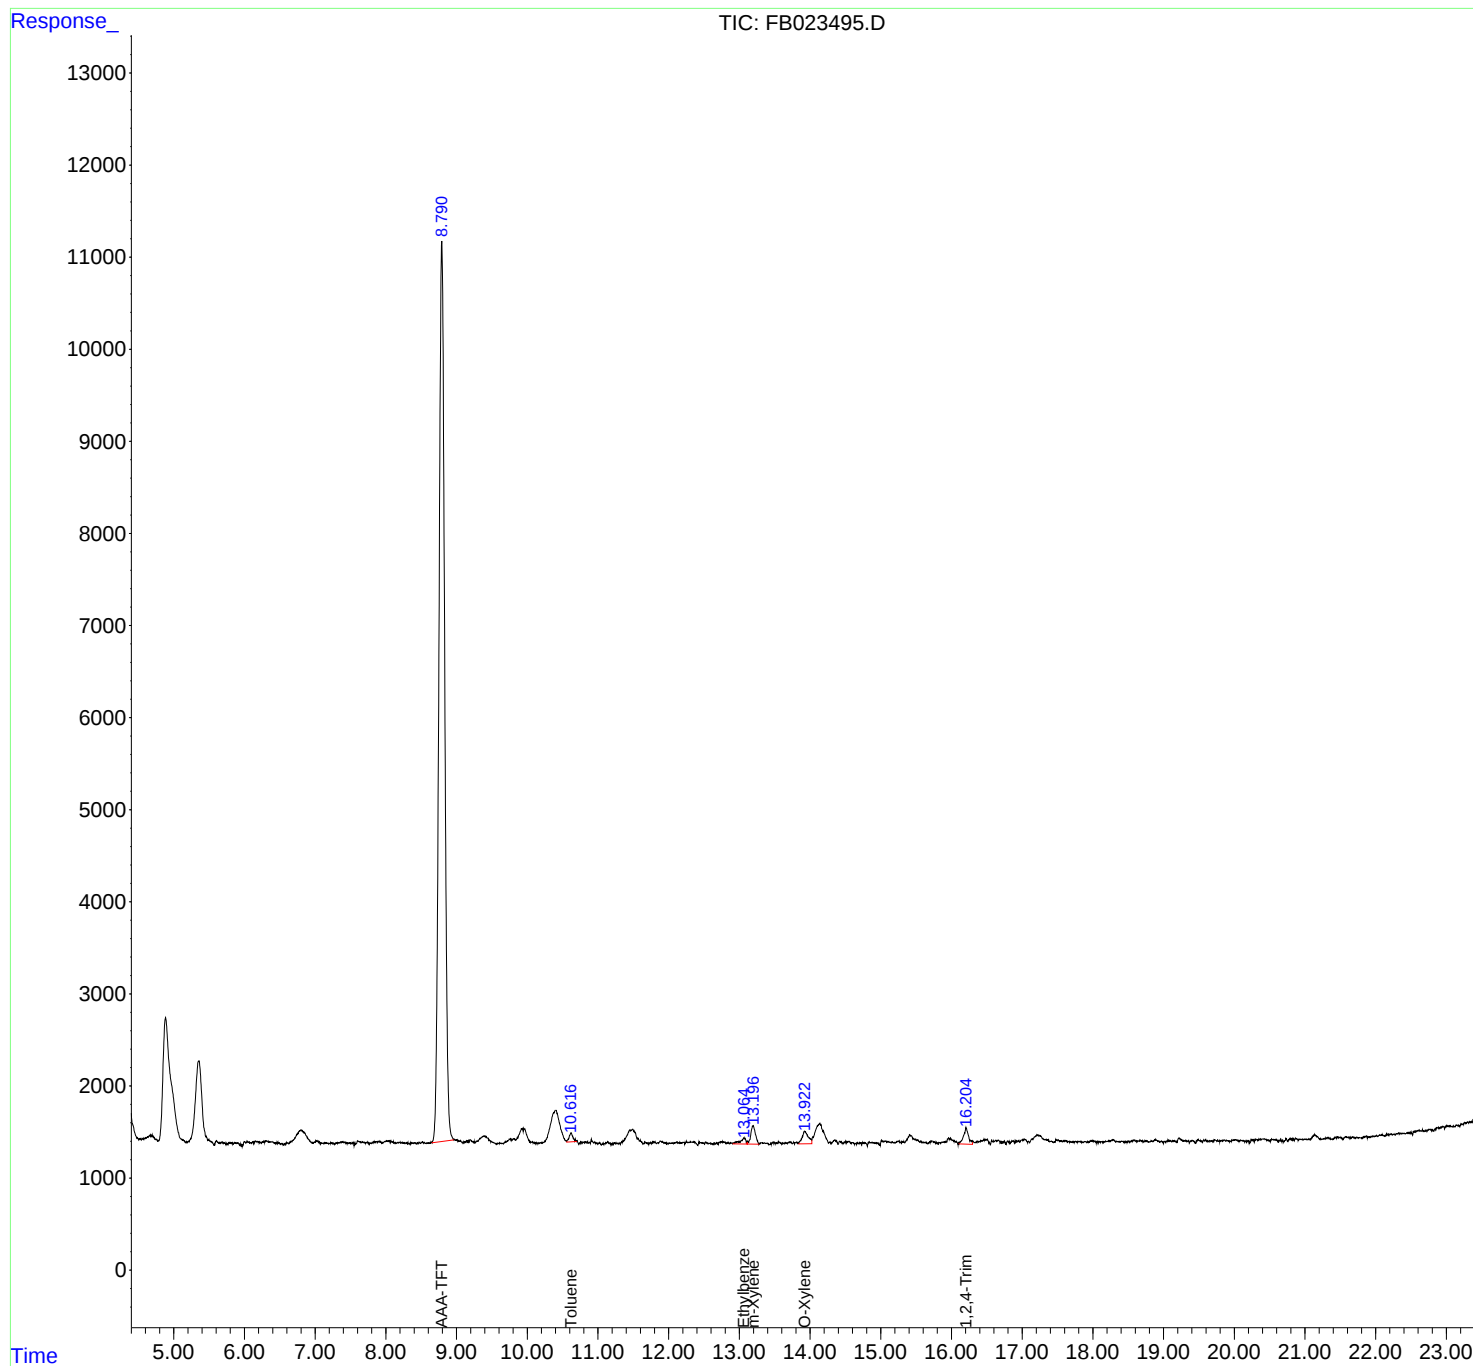


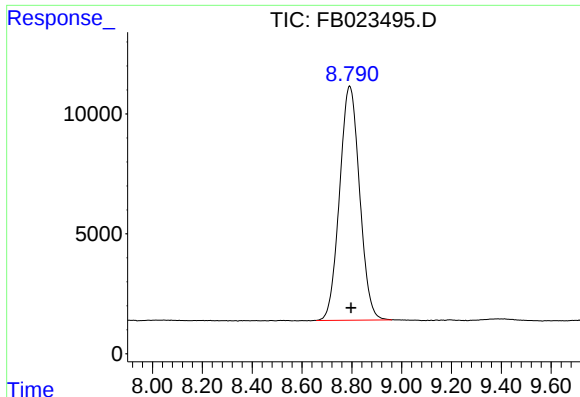

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.005 min
Response: 544785
Conc: 22.93 ng/ml

Instrument :
FID_B
ClientSampleId :

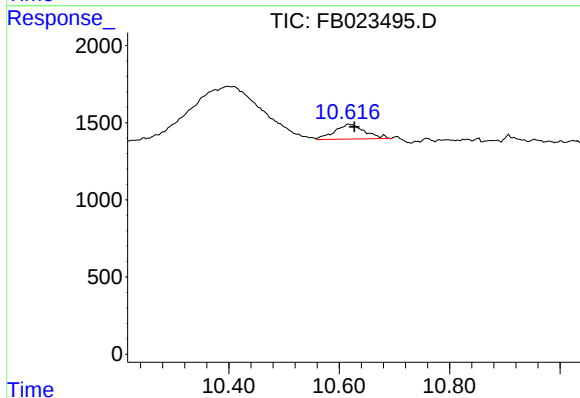


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.009 min
Response: 3592
Conc: 0.09 ng/ml

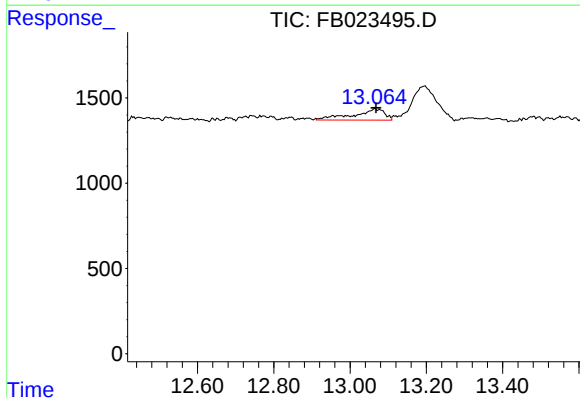


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 3647
Conc: 0.10 ng/ml

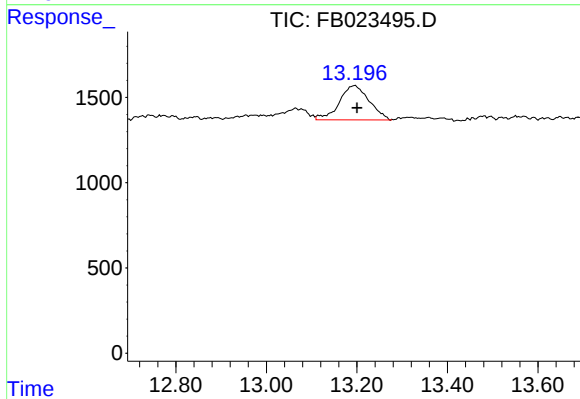

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.005 min
Response: 9195
Conc: 0.26 ng/ml

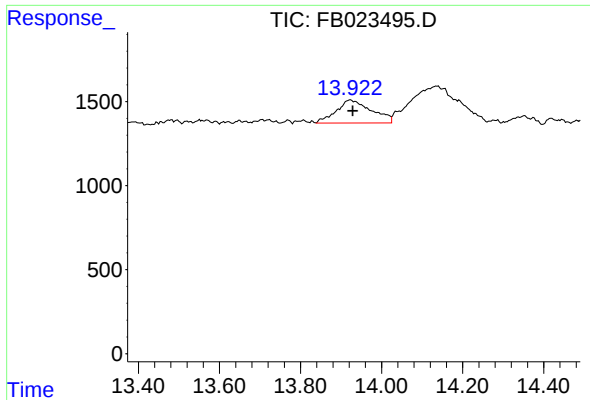

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.005 min
Response: 8311
Conc: 0.24 ng/ml

Instrument :
FID_B
ClientSampleId :

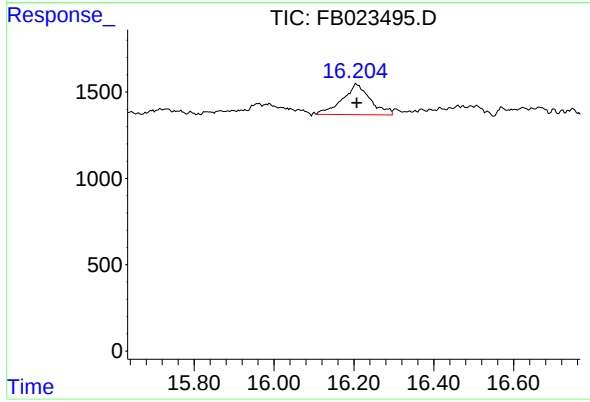

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 8562
Conc: 0.29 ng/ml