

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023499.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 12:14
 Operator : DD/AJ
 Sample : L1007-20
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 24 21:47:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	551212	23.205 ng/ml
Target Compounds			
6) t Toluene	10.631	4830	0.122 ng/ml
8) t m-Xylene	13.208	213	0.006 ng/ml
10) t 1,2,4-Trimethylbenzene	16.215	893	0.031 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023499.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 12:14
Operator : DD/AJ
Sample : L1007-20
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 24 21:47:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

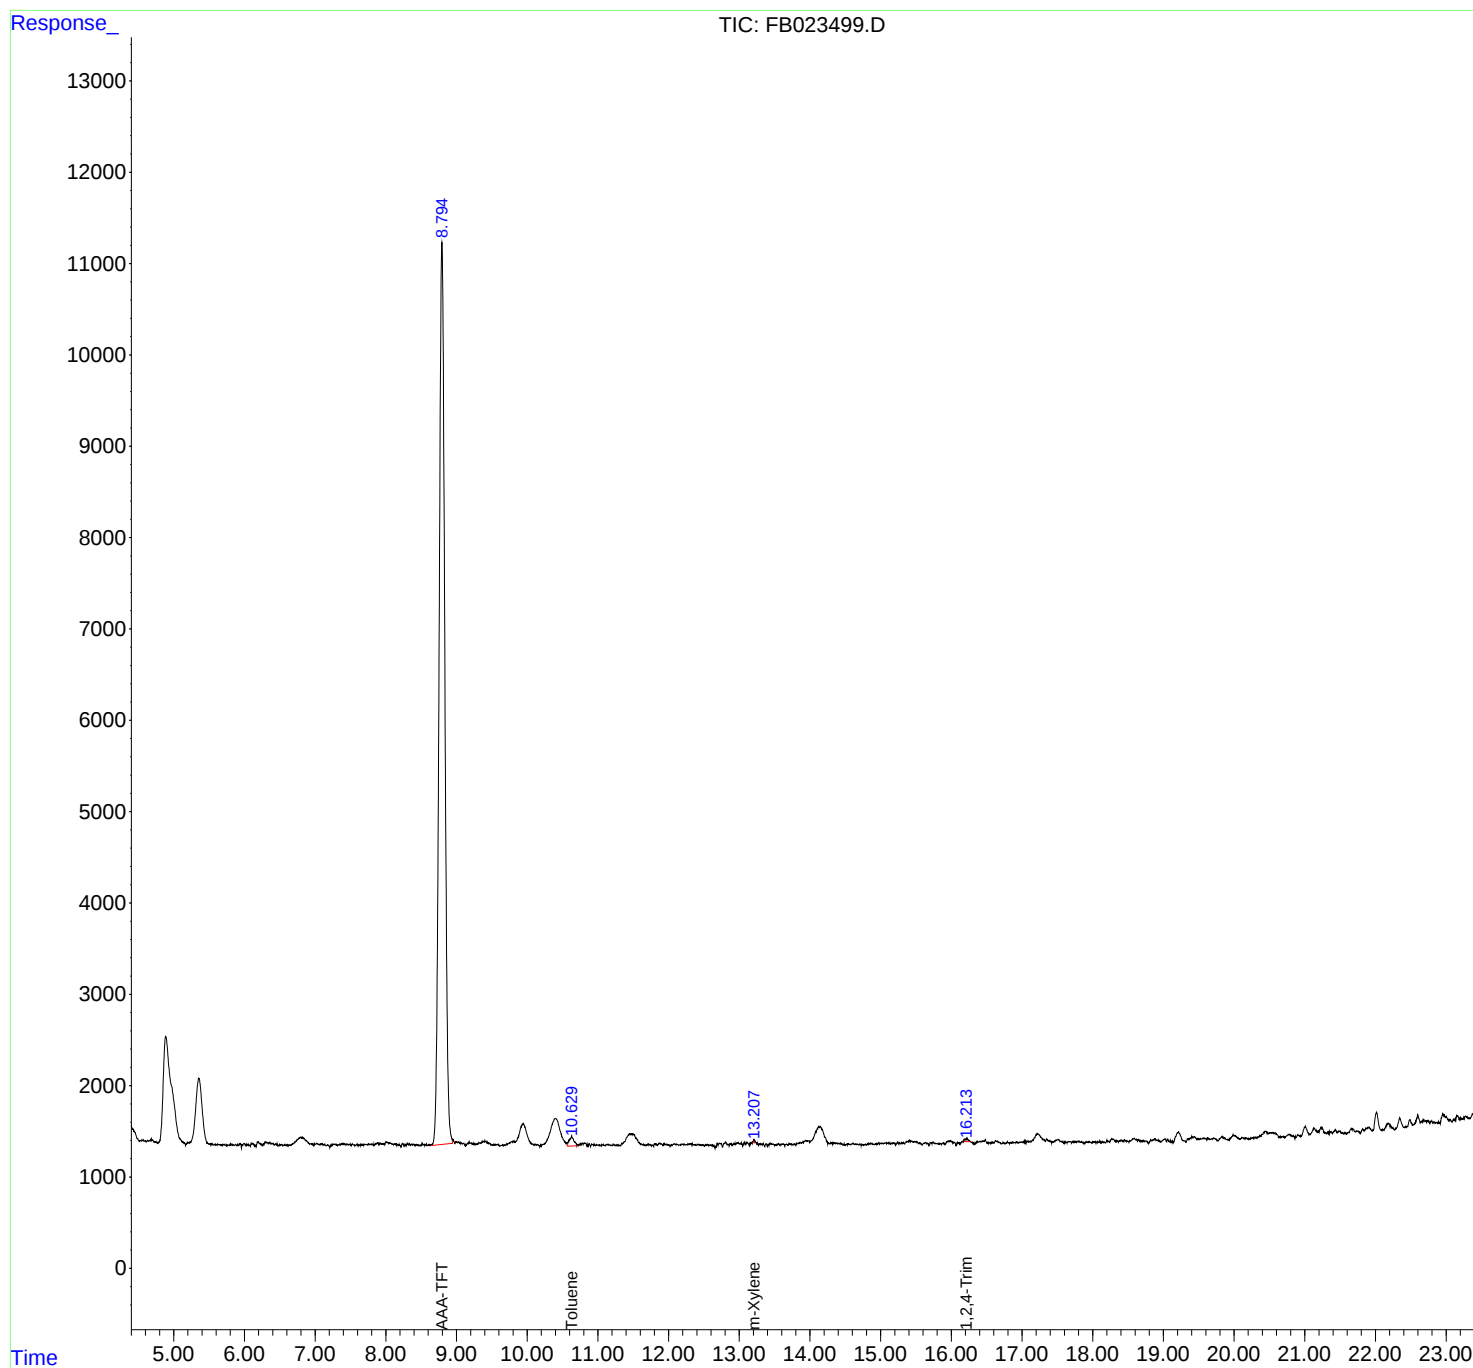


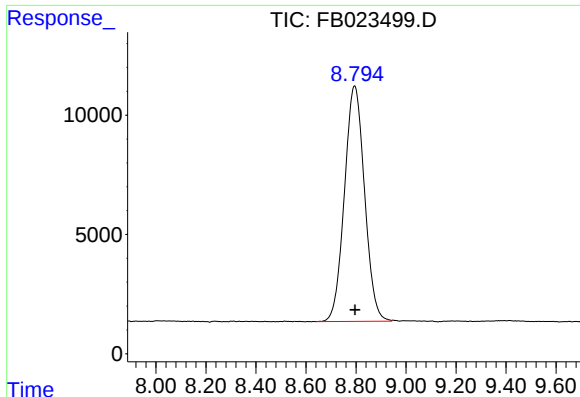

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 551212
Conc: 23.21 ng/ml

Instrument :
FID_B
ClientSampleId :

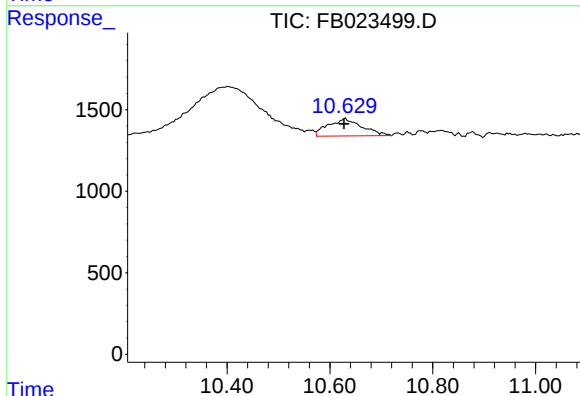


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.003 min
Response: 4830
Conc: 0.12 ng/ml

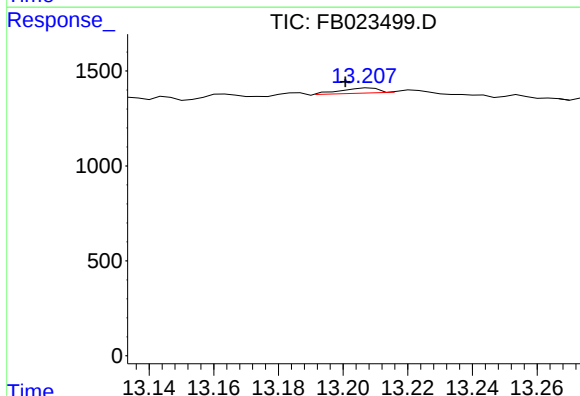

#8 m-Xylene

R.T.: 13.208 min
Delta R.T.: 0.008 min
Response: 213
Conc: 0.01 ng/ml

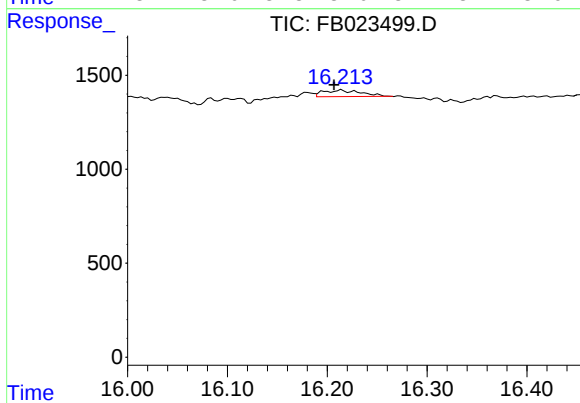

#10 1,2,4-Trimethylbenzene

R.T.: 16.215 min
Delta R.T.: 0.008 min
Response: 893
Conc: 0.03 ng/ml