

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023502.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 13:44
 Operator : DD/AJ
 Sample : L1007-02MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 24 21:47:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	468504	19.723 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	752217	23.804 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	697742	20.550 ng/ml
3) t n-Heptane	7.754	237119	7.081 ng/ml
4) t Benzene	7.889	395673	9.689 ng/ml
6) t Toluene	10.626	1134360	28.705 ng/ml
7) t Ethylbenzene	13.066	338091	9.052 ng/ml
8) t m-Xylene	13.199	653453	18.376 ng/ml
9) t O-Xylene	13.927	612368	17.722 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	512641	17.532 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023502.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 13:44
Operator : DD/AJ
Sample : L1007-02MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 24 21:47:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

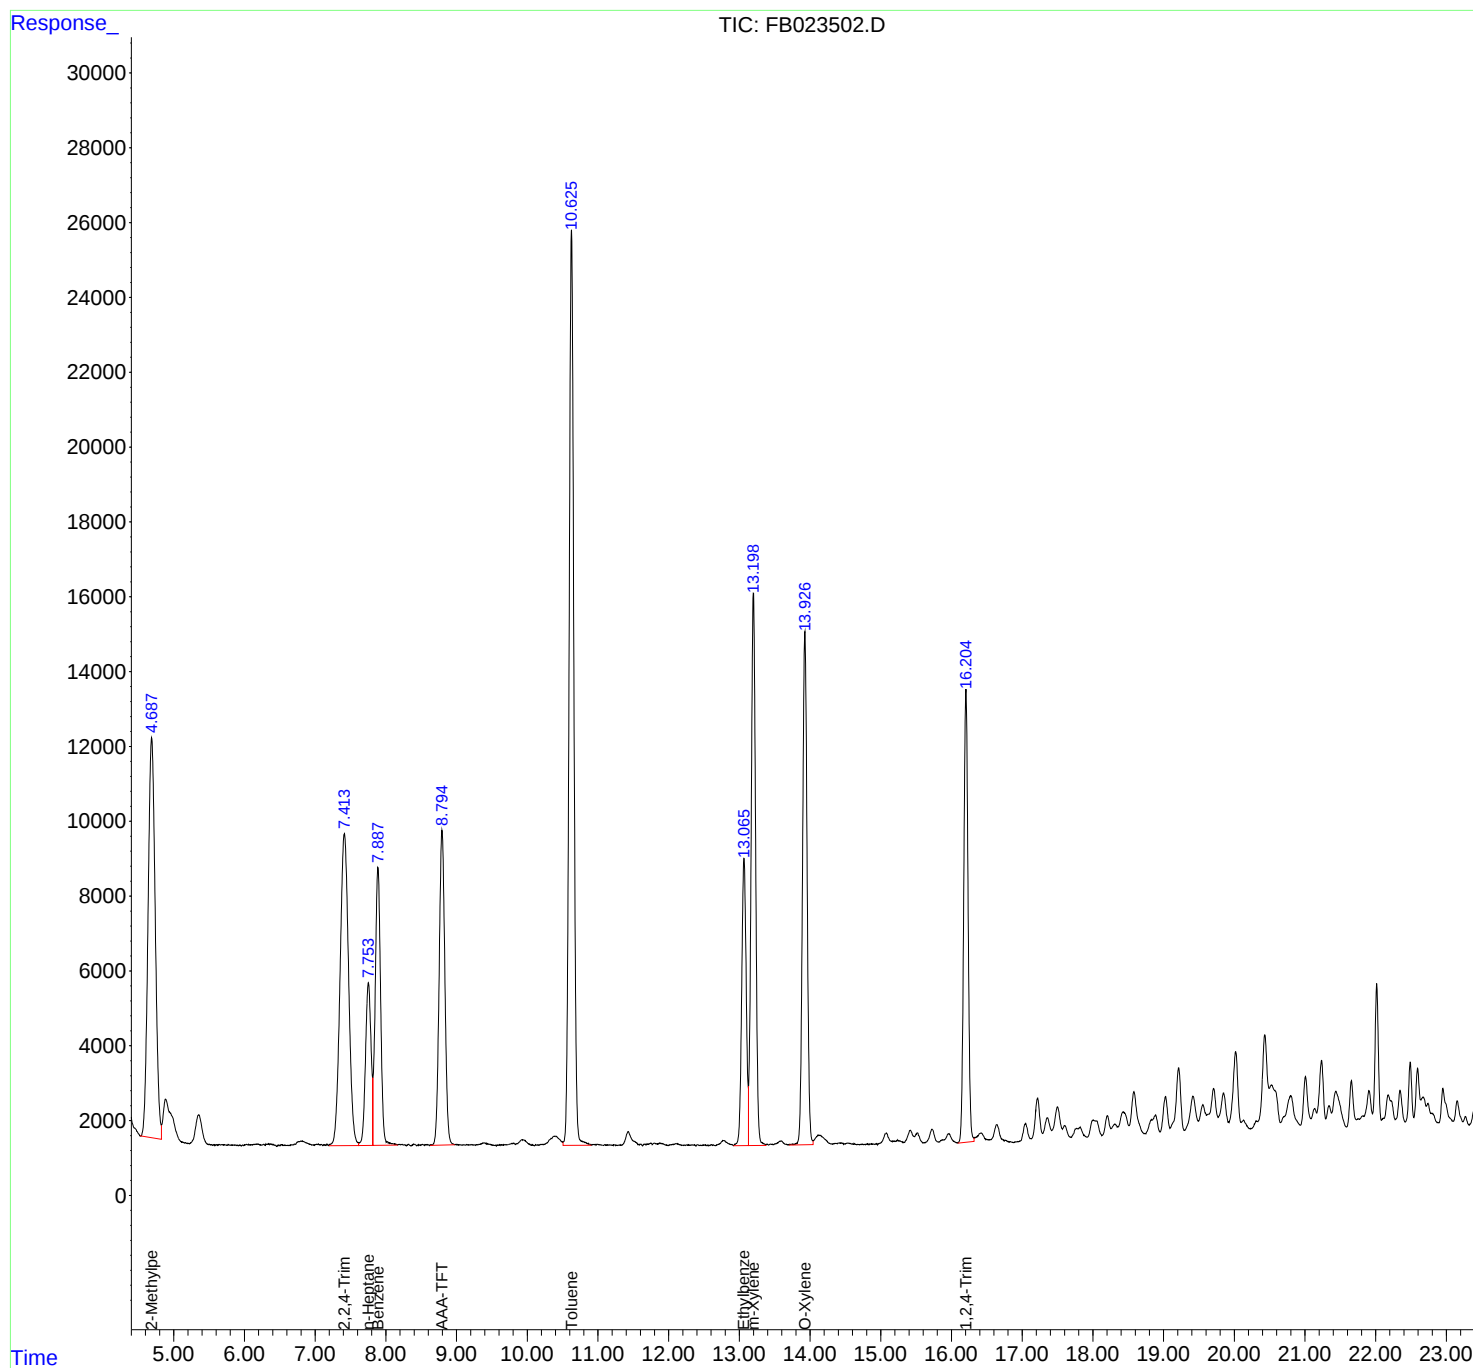


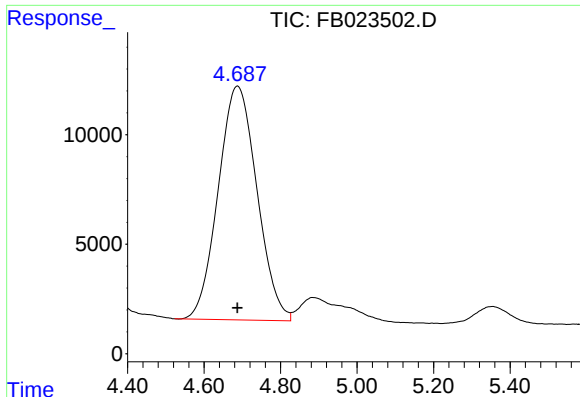

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.001 min
Response: 752217
Conc: 23.80 ng/ml

Instrument :
FID_B
ClientSampleId :

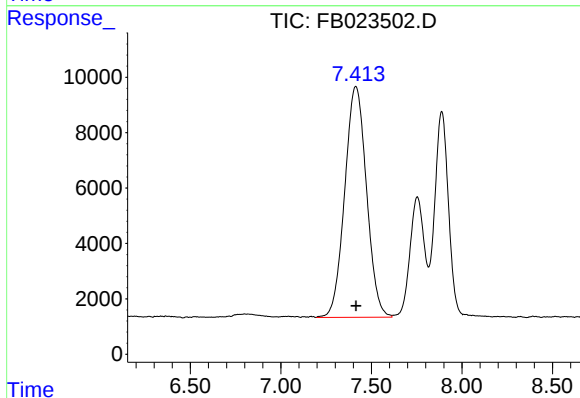


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 697742
Conc: 20.55 ng/ml

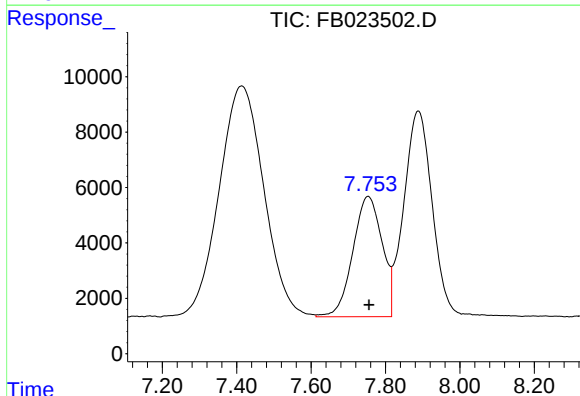


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.002 min
Response: 237119
Conc: 7.08 ng/ml

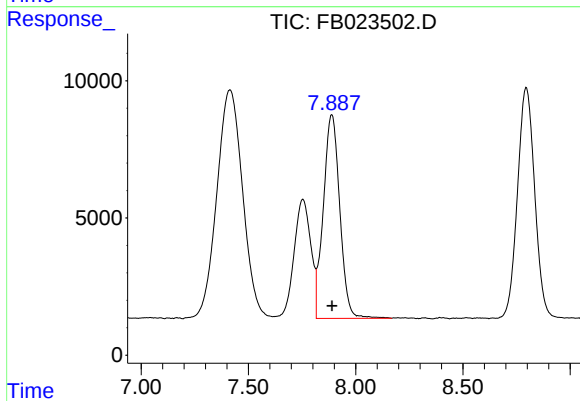

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 395673
Conc: 9.69 ng/ml

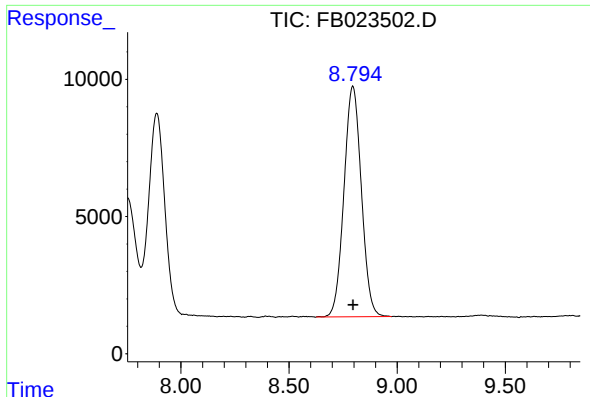

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 468504
Conc: 19.72 ng/ml

Instrument :
FID_B
ClientSampleId :

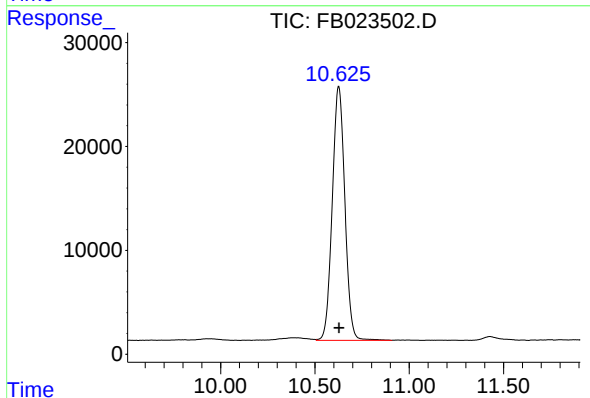


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 1134360
Conc: 28.70 ng/ml

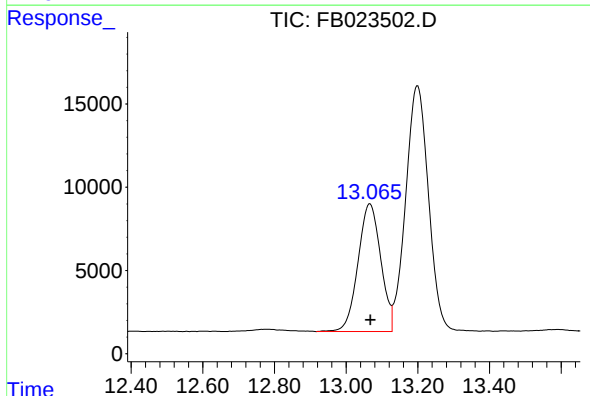


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.002 min
Response: 338091
Conc: 9.05 ng/ml

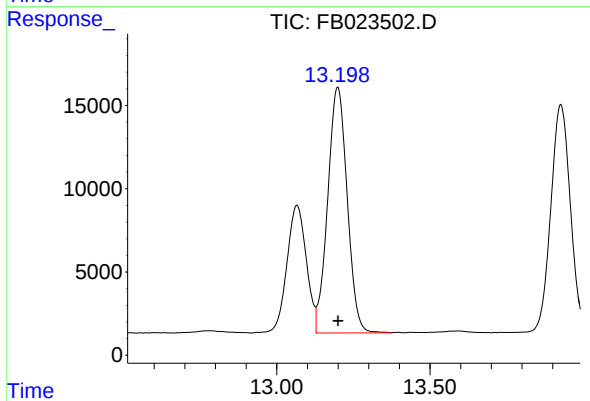

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.001 min
Response: 653453
Conc: 18.38 ng/ml

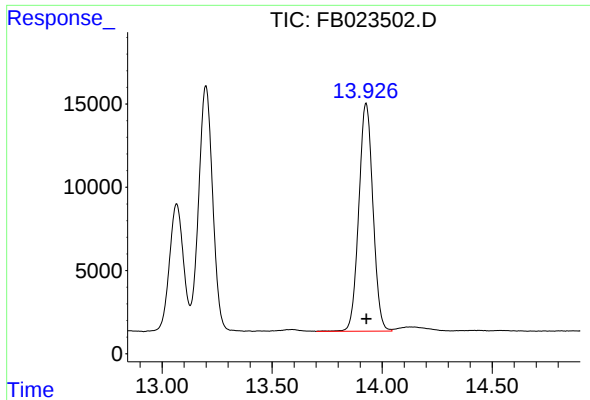

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 612368
Conc: 17.72 ng/ml

Instrument :
FID_B
ClientSampleId :

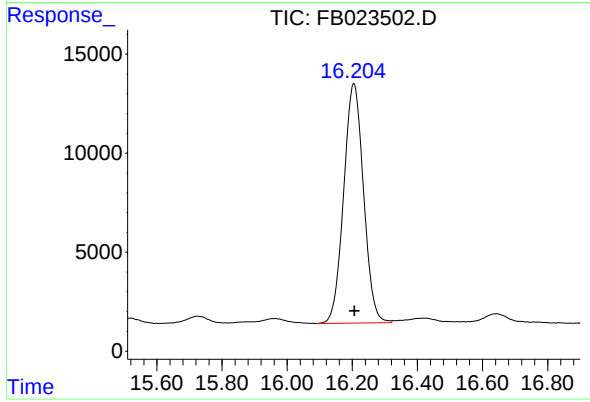

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.001 min
Response: 512641
Conc: 17.53 ng/ml