

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023505.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 15:29
 Operator : DD/AJ
 Sample : L1247-05
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 24 21:48:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	574771	24.197 ng/ml
Target Compounds			
6) t Toluene	10.625	4430	0.112 ng/ml
8) t m-Xylene	13.206	3051	0.086 ng/ml
9) t O-Xylene	13.919	1146	0.033 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	333	0.011 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023505.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 15:29
Operator : DD/AJ
Sample : L1247-05
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 24 21:48:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

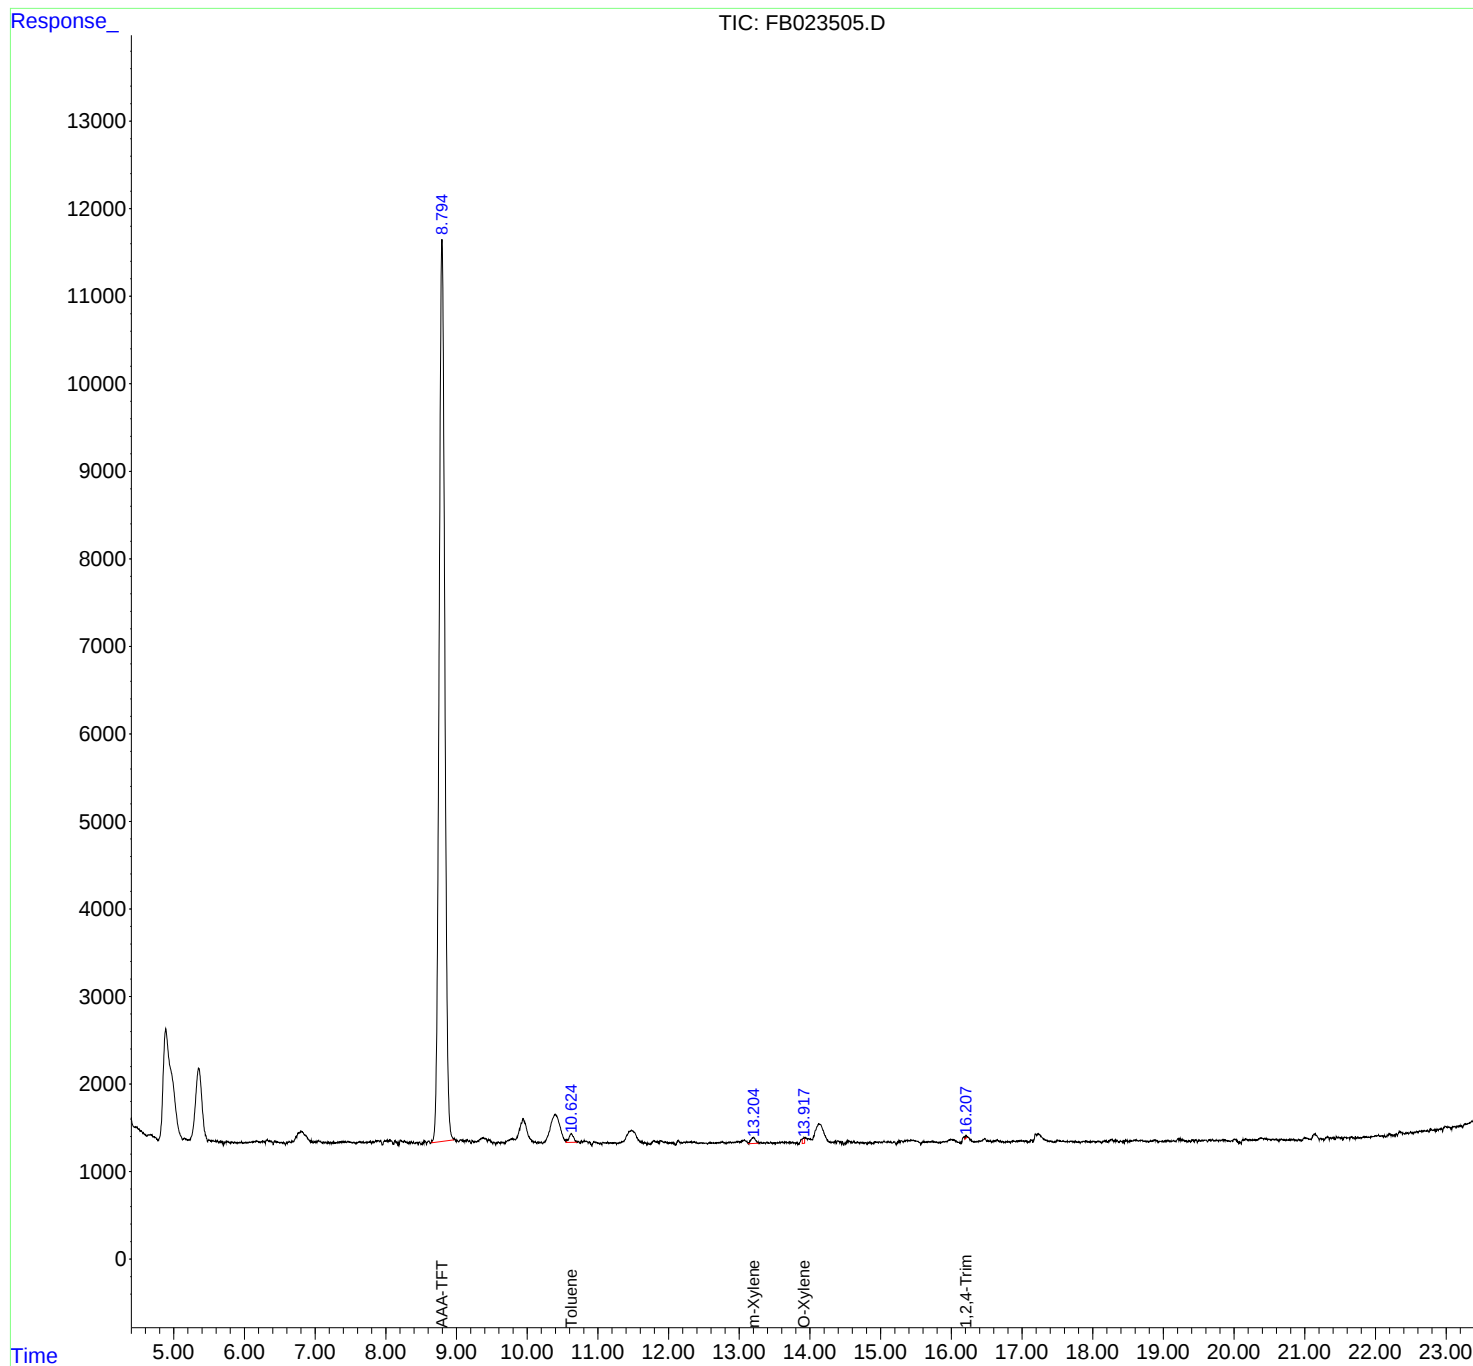


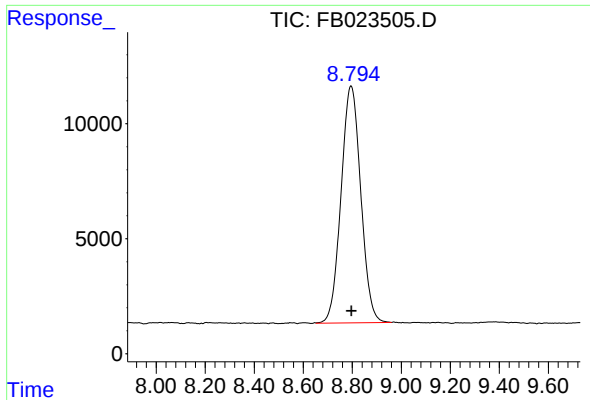

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.001 min
Response: 574771
Conc: 24.20 ng/ml

Instrument :
FID_B
ClientSampleId :

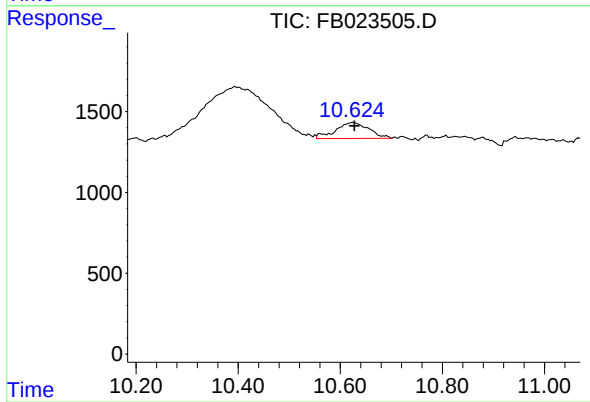


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 4430
Conc: 0.11 ng/ml

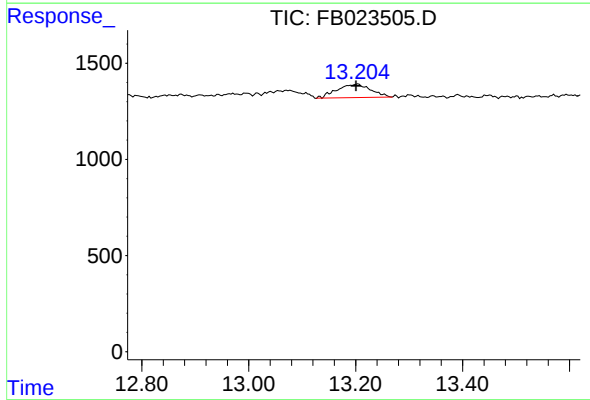


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.005 min
Response: 3051
Conc: 0.09 ng/ml

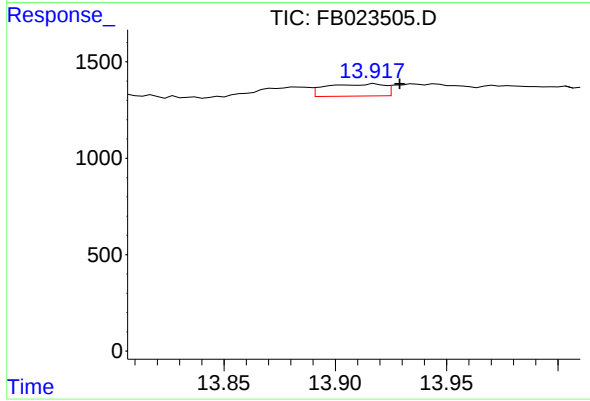

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.010 min
Response: 1146
Conc: 0.03 ng/ml

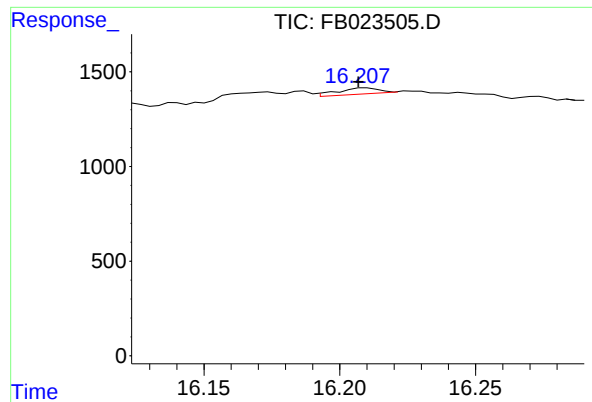

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 333
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :