

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023506.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 15:59
 Operator : DD/AJ
 Sample : L1247-06
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 24 21:48:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	573495	24.143 ng/ml
Target Compounds			
4) t Benzene	7.901	1025	0.025 ng/ml
6) t Toluene	10.626	4958	0.125 ng/ml
9) t O-Xylene	13.940	790	0.023 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023506.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 15:59
Operator : DD/AJ
Sample : L1247-06
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 24 21:48:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

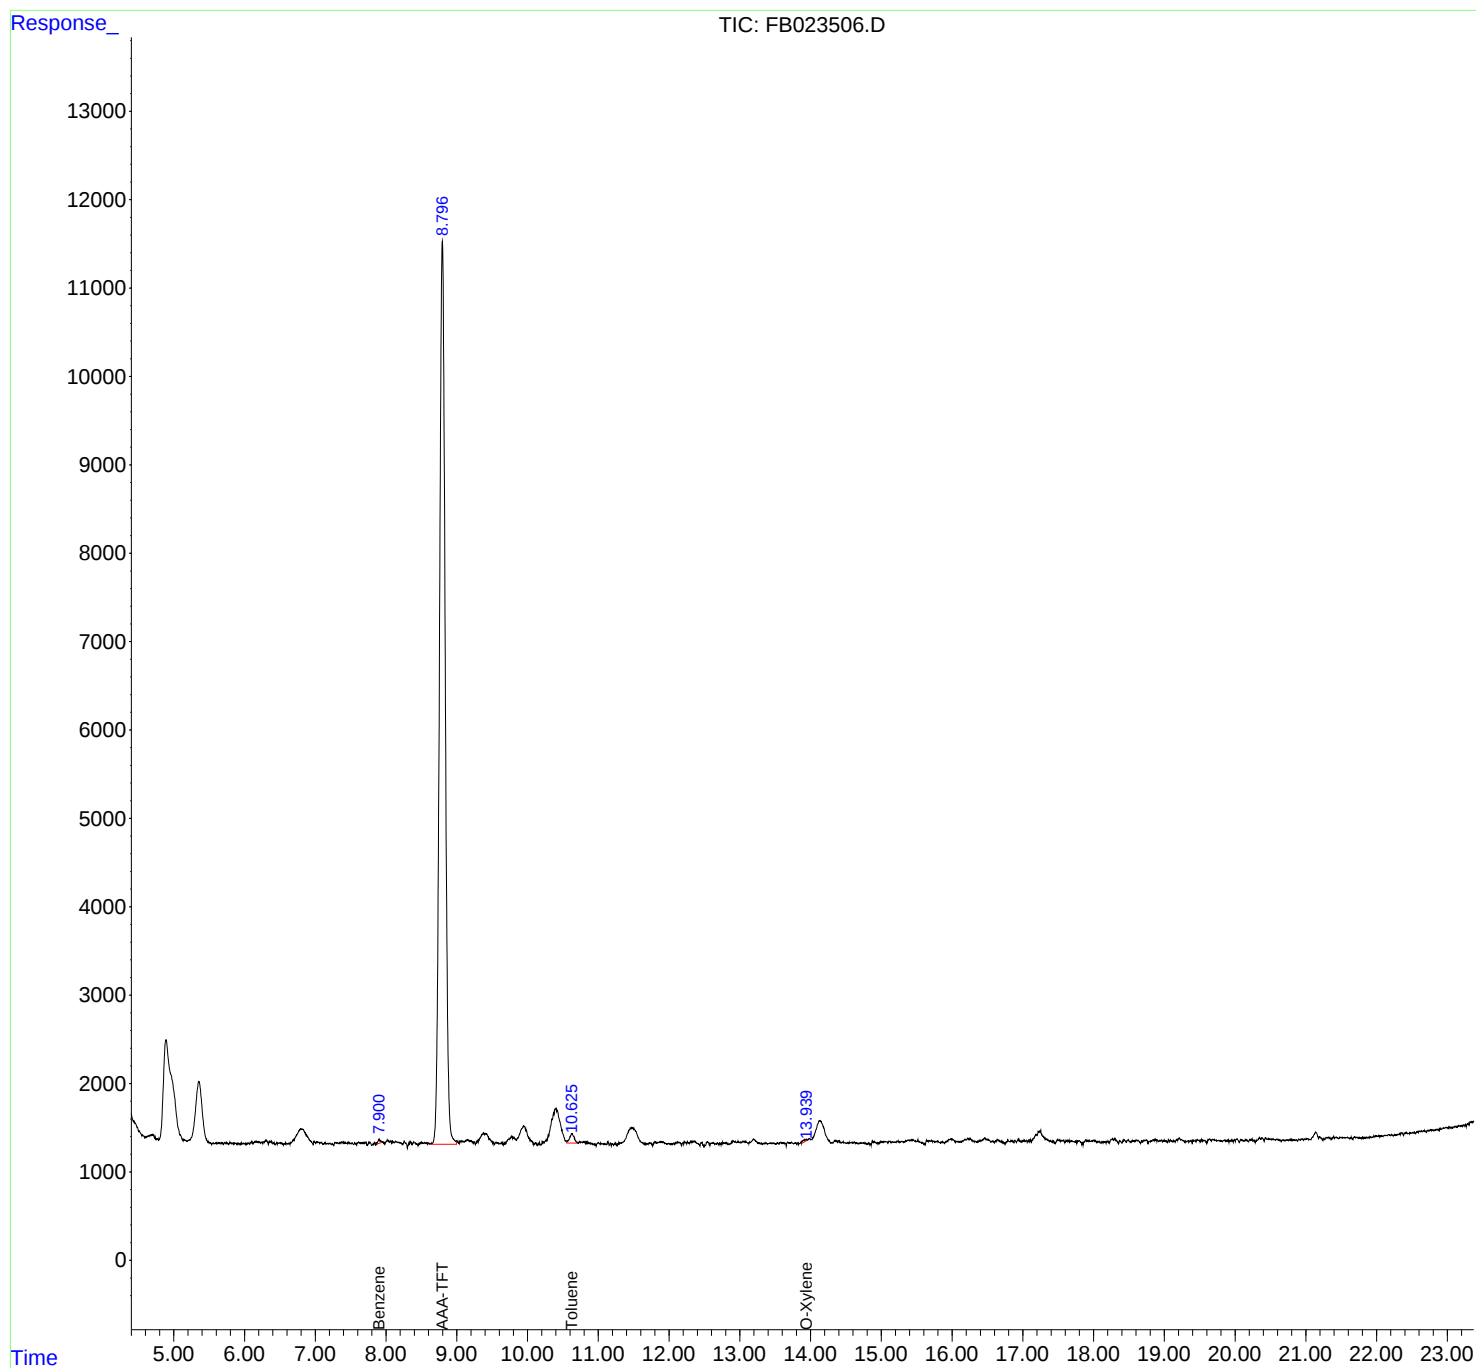


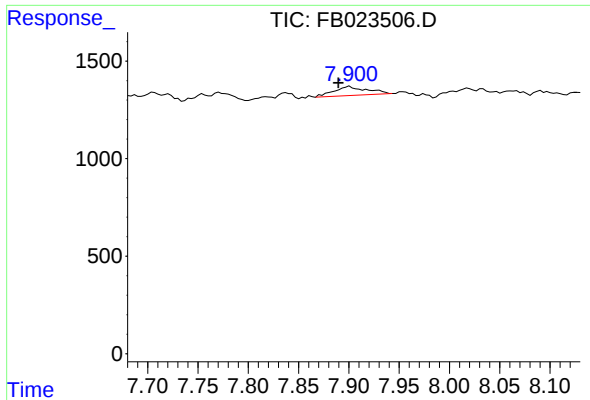

#4 Benzene


R.T.: 7.901 min
Delta R.T.: 0.012 min
Response: 1025
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :

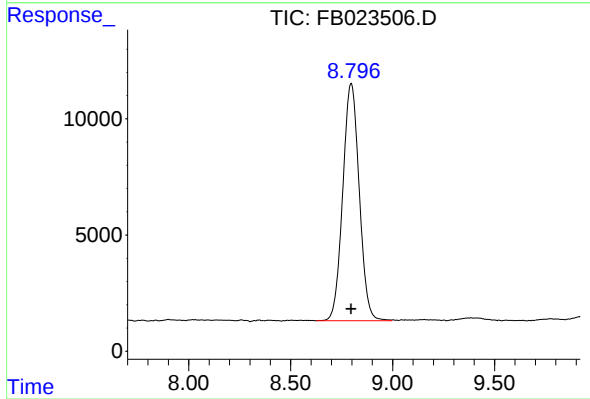


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 573495
Conc: 24.14 ng/ml

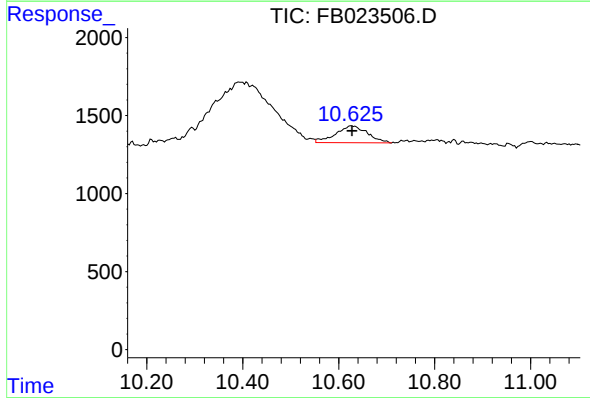

#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 4958
Conc: 0.13 ng/ml

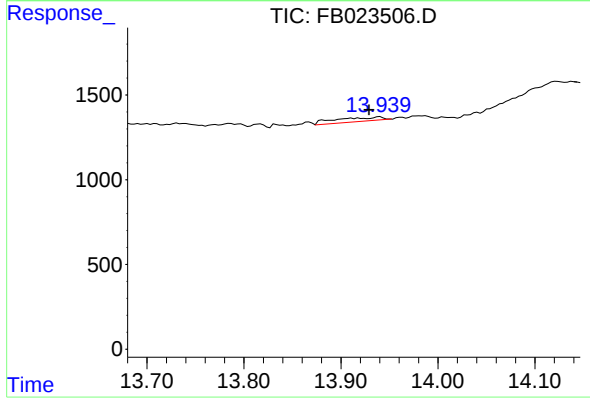

#9 O-Xylene

R.T.: 13.940 min
Delta R.T.: 0.011 min
Response: 790
Conc: 0.02 ng/ml