

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023512.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 19:01
 Operator : DD/AJ
 Sample : L1247-22
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 24 21:49:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	521521	21.955 ng/ml
Target Compounds			
6) t Toluene	10.625	6201	0.157 ng/ml
8) t m-Xylene	13.185	2559	0.072 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	1117	0.038 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023512.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 19:01
Operator : DD/AJ
Sample : L1247-22
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 24 21:49:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

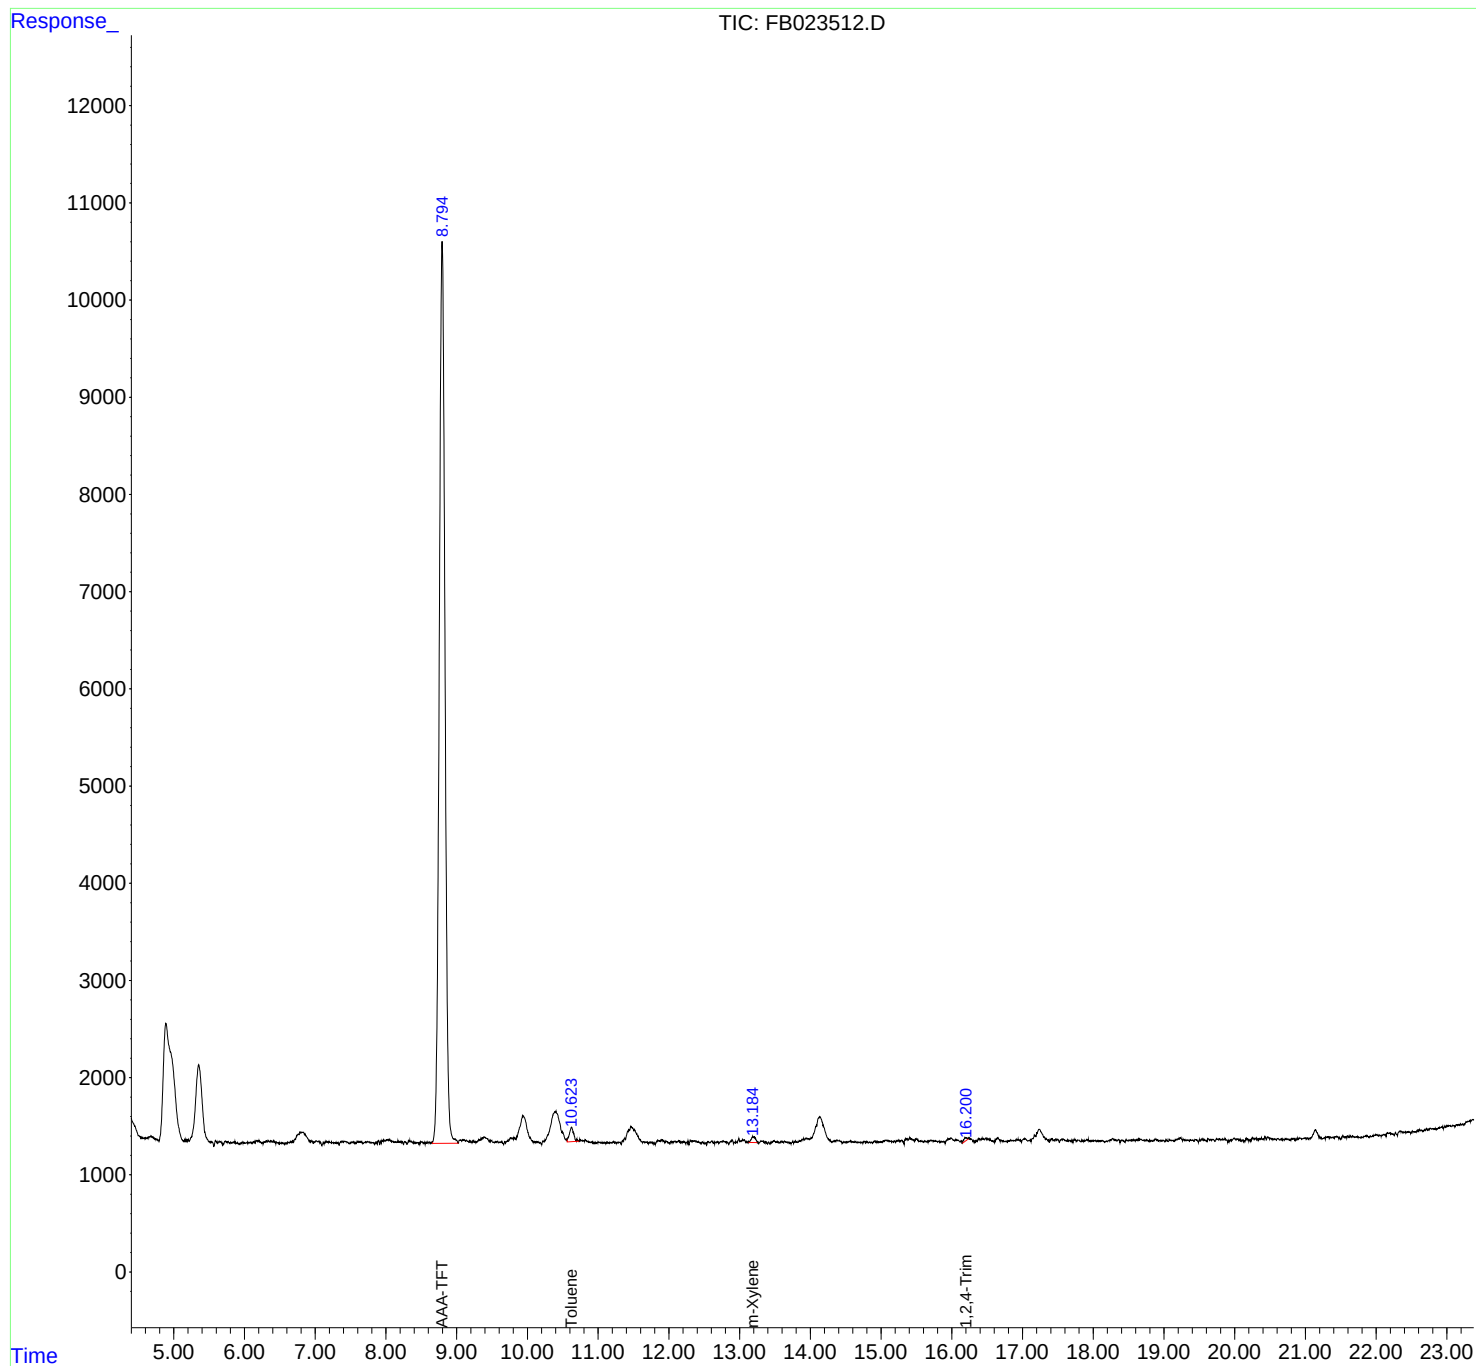


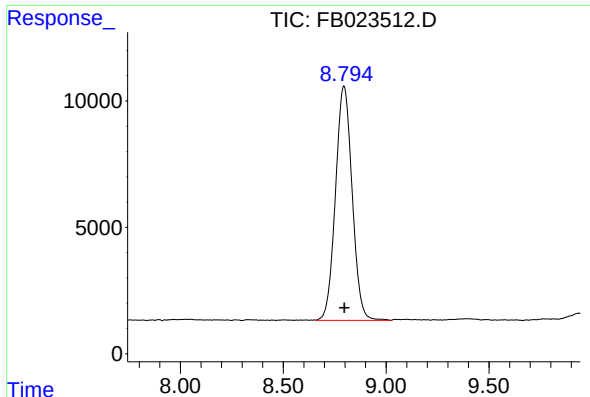

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 521521
Conc: 21.96 ng/ml

Instrument :
FID_B
ClientSampleId :

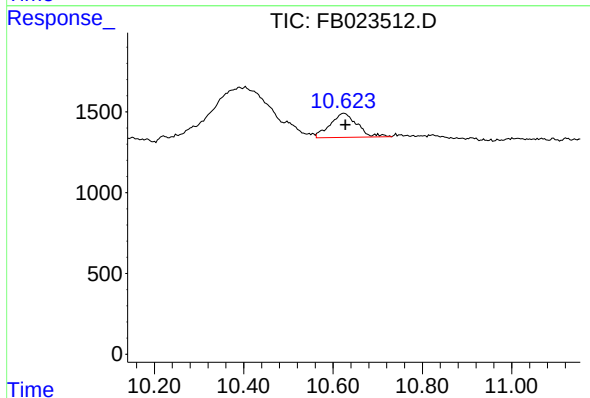


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 6201
Conc: 0.16 ng/ml

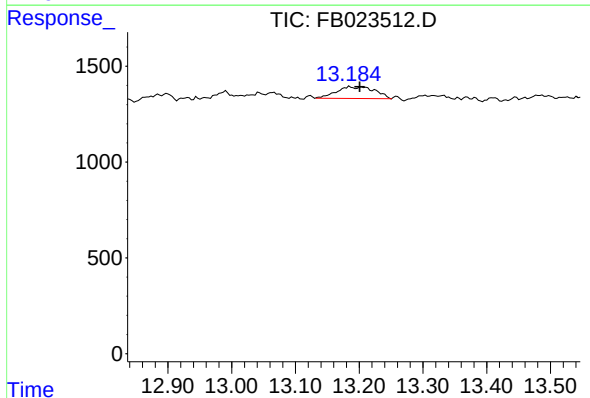

#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.015 min
Response: 2559
Conc: 0.07 ng/ml

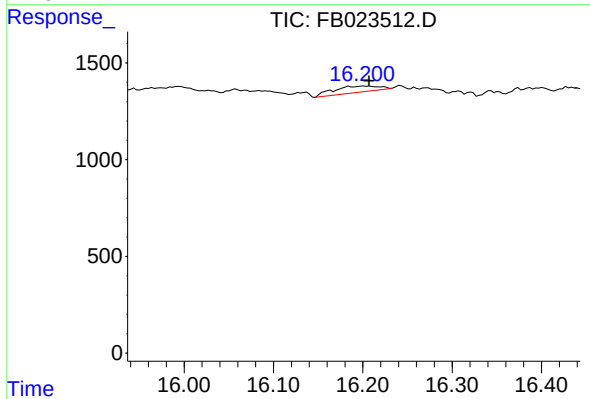

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 1117
Conc: 0.04 ng/ml