

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB012420\  
 Data File : FB023514.D  
 Signal(s) : FID2B.CH  
 Acq On : 24 Jan 2020 20:32  
 Operator : DD/AJ  
 Sample : L1247-23  
 Misc : 5.07g/5.00ml DI WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Jan 24 21:49:48 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011620.M  
 Quant Title :  
 QLast Update : Thu Jan 16 11:42:55 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.797  | 559108   | 23.538 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.632 | 6052     | 0.153 ng/ml  |
| 8) t m-Xylene                | 13.198 | 118      | 0.003 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.217 | 2679     | 0.092 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB012420\  
Data File : FB023514.D  
Signal(s) : FID2B.CH  
Acq On : 24 Jan 2020 20:32  
Operator : DD/AJ  
Sample : L1247-23  
Misc : 5.07g/5.00ml DI WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jan 24 21:49:48 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011620.M  
Quant Title :  
QLast Update : Thu Jan 16 11:42:55 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

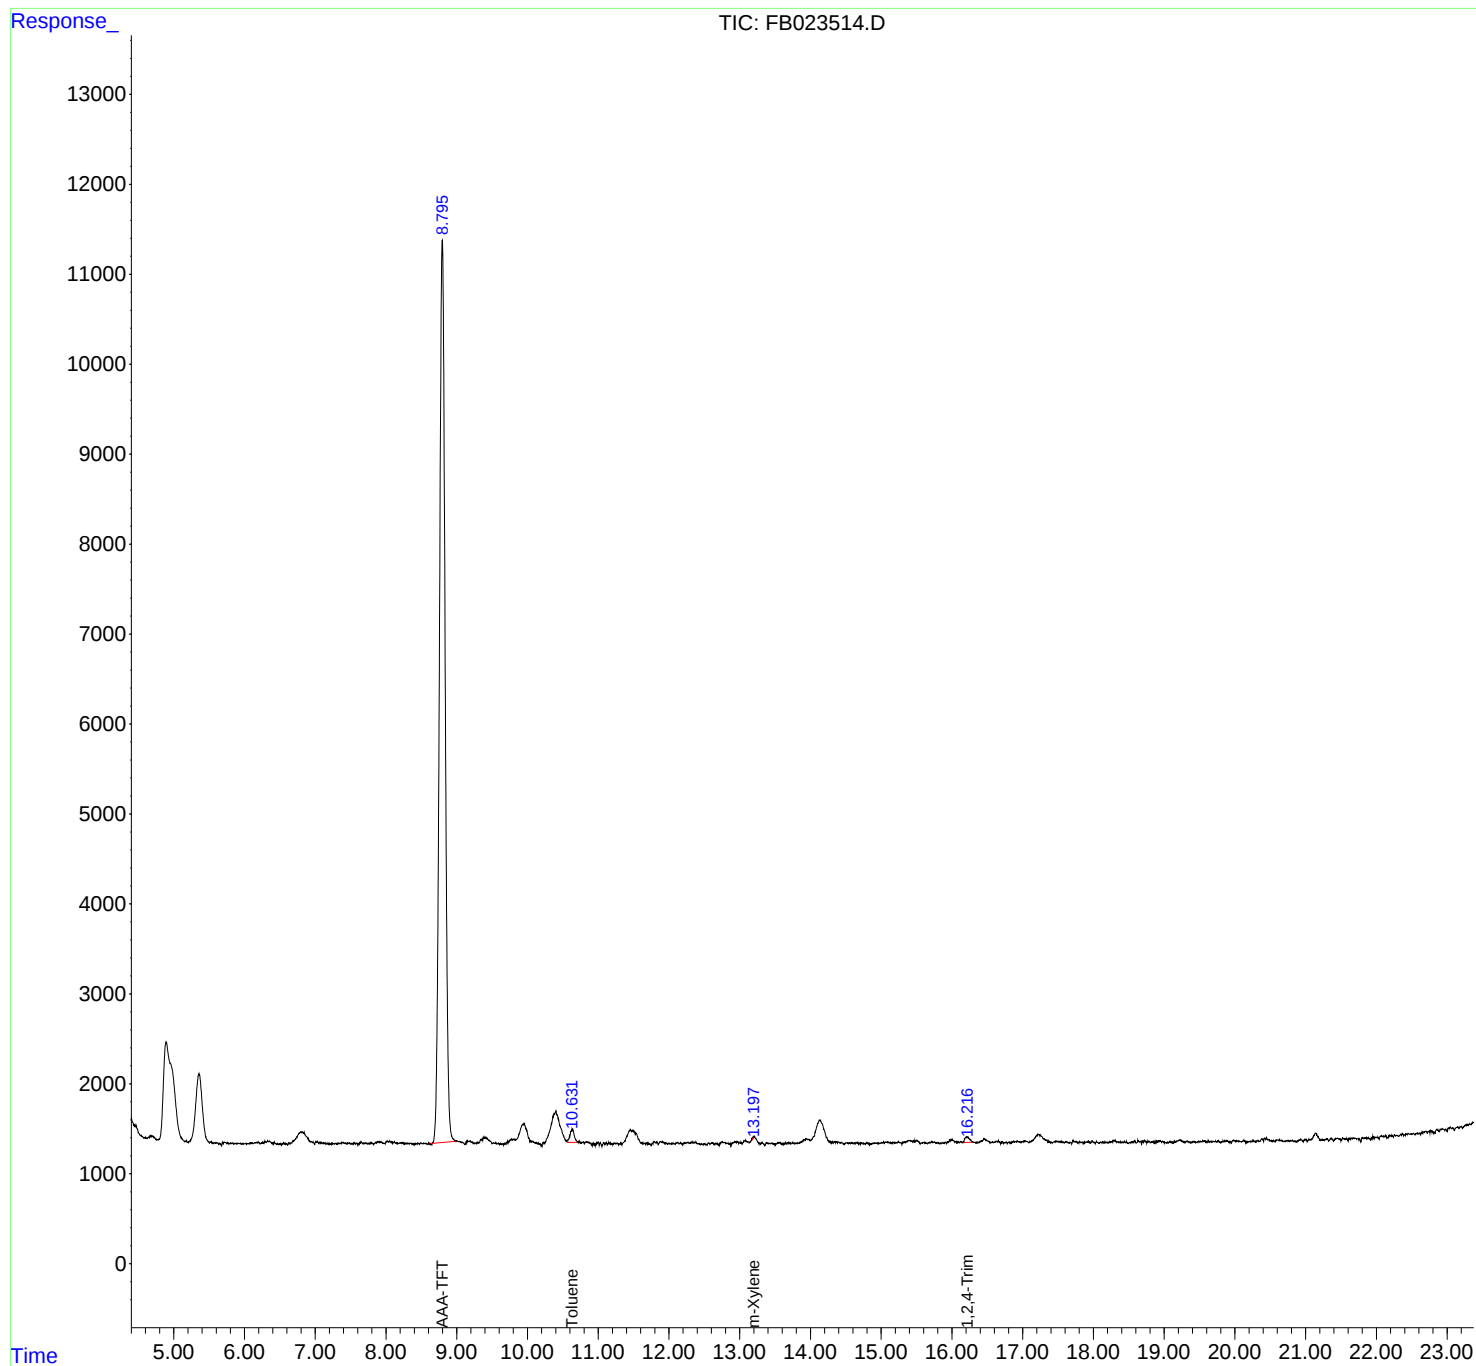


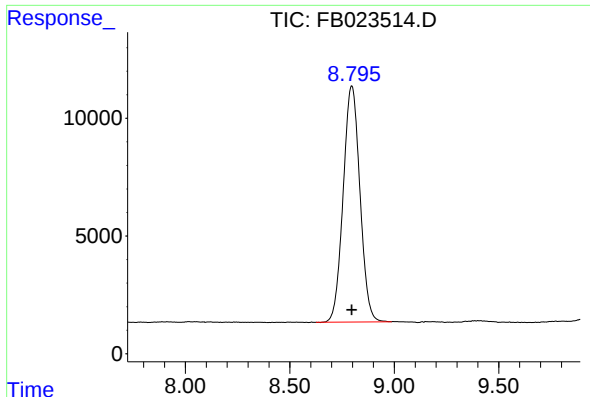

#5 AAA-TFT


R.T.: 8.797 min  
Delta R.T.: 0.000 min  
Response: 559108  
Conc: 23.54 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

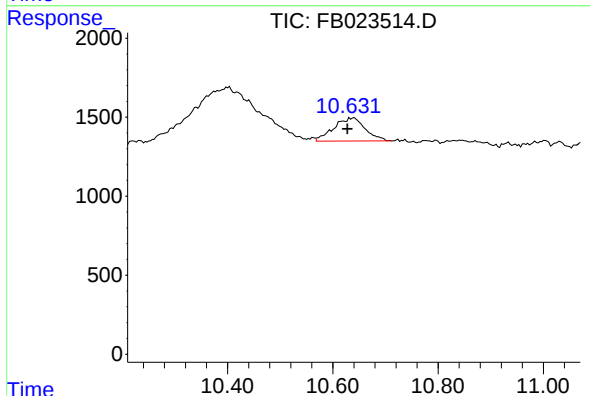


#6 Toluene

R.T.: 10.632 min  
Delta R.T.: 0.005 min  
Response: 6052  
Conc: 0.15 ng/ml

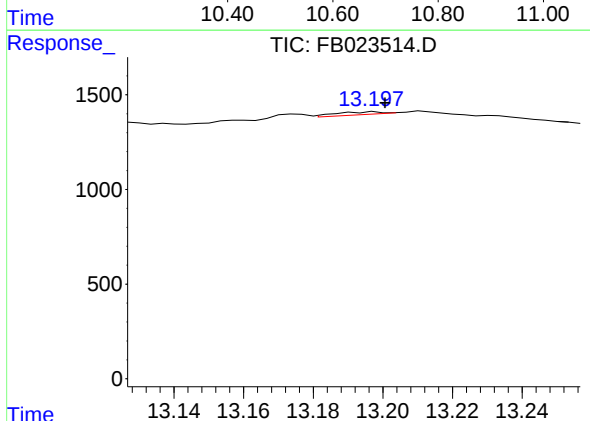

#8 m-Xylene

R.T.: 13.198 min  
Delta R.T.: -0.003 min  
Response: 118  
Conc: 0.00 ng/ml

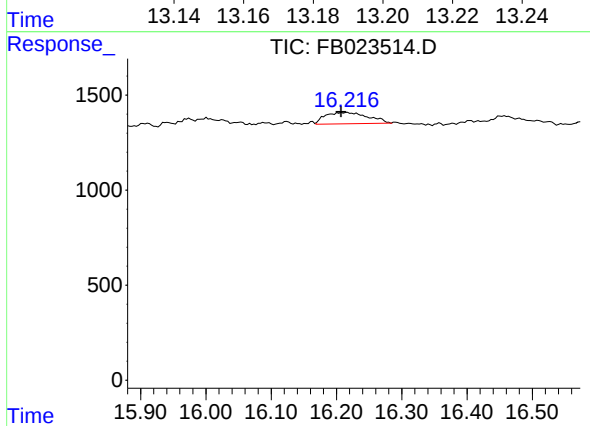

#10 1,2,4-Trimethylbenzene

R.T.: 16.217 min  
Delta R.T.: 0.010 min  
Response: 2679  
Conc: 0.09 ng/ml