

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023494.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 9:29
 Operator : DD/AJ
 Sample : BSF0124S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0124S1

Integration File: Calibration.e
 Quant Time: Jan 24 21:46:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	502493	21.154 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	940681	29.768 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	1053847	31.038 ng/ml
3) t n-Heptane	7.752	342813	10.237 ng/ml
4) t Benzene	7.885	406731	9.960 ng/ml
6) t Toluene	10.624	1201537	30.405 ng/ml
7) t Ethylbenzene	13.065	374911	10.038 ng/ml
8) t m-Xylene	13.197	716822	20.158 ng/ml
9) t O-Xylene	13.925	690946	19.996 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	590637	20.199 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023494.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 9:29
Operator : DD/AJ
Sample : BSF0124S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0124S1

Integration File: Calibration.e
Quant Time: Jan 24 21:46:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

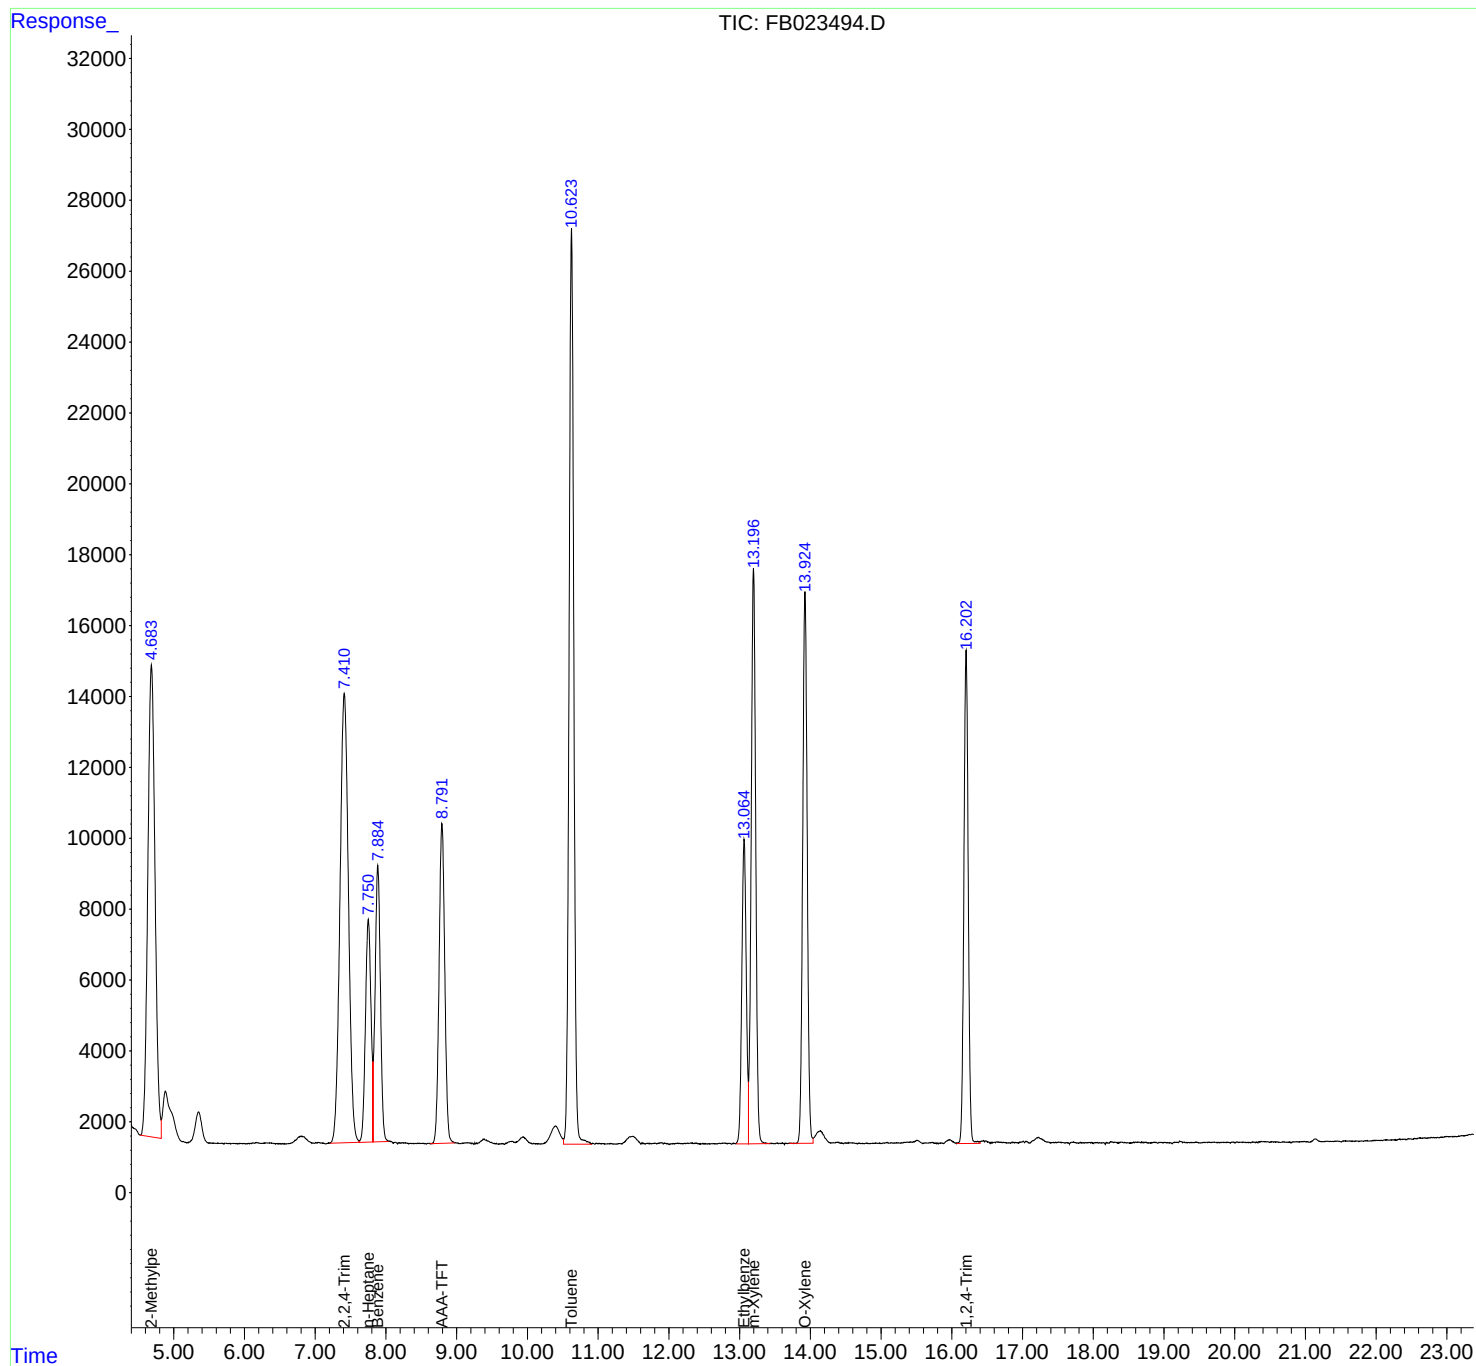


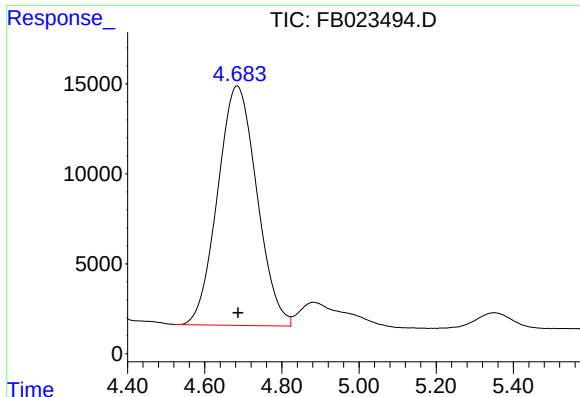

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.002 min
Response: 940681
Conc: 29.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0124S1

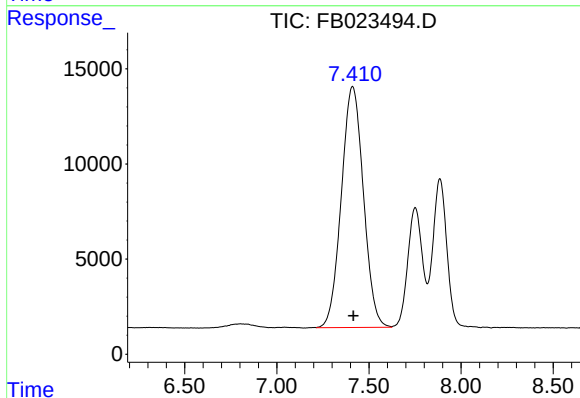


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.004 min
Response: 1053847
Conc: 31.04 ng/ml

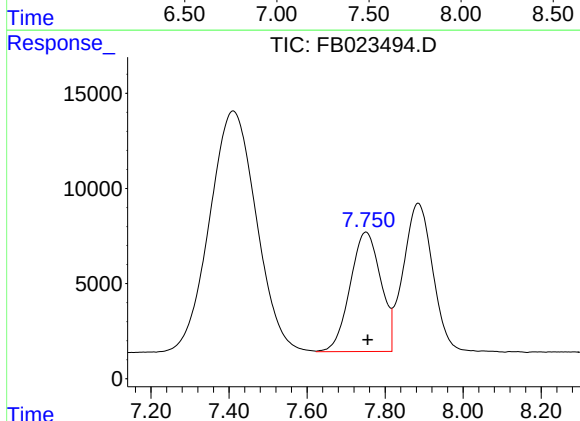


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.004 min
Response: 342813
Conc: 10.24 ng/ml

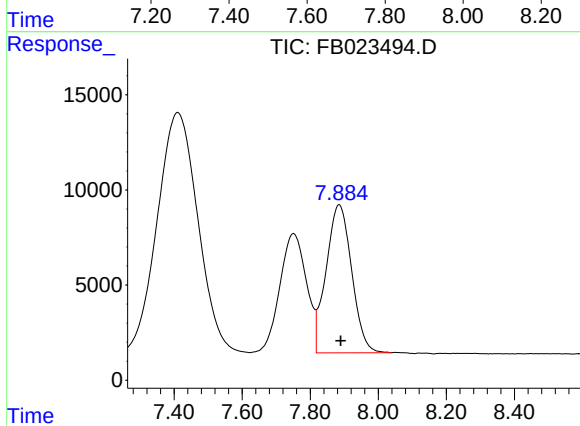

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.004 min
Response: 406731
Conc: 9.96 ng/ml

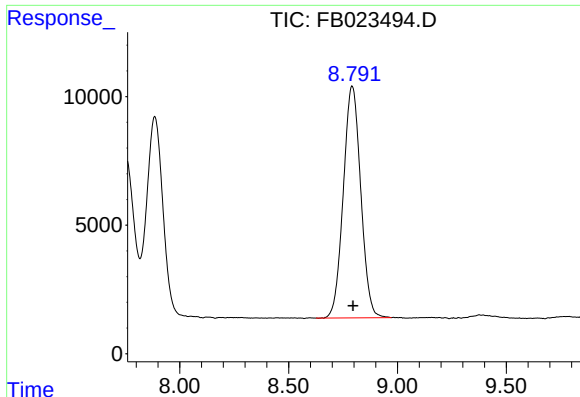

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.004 min
Response: 502493
Conc: 21.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0124S1

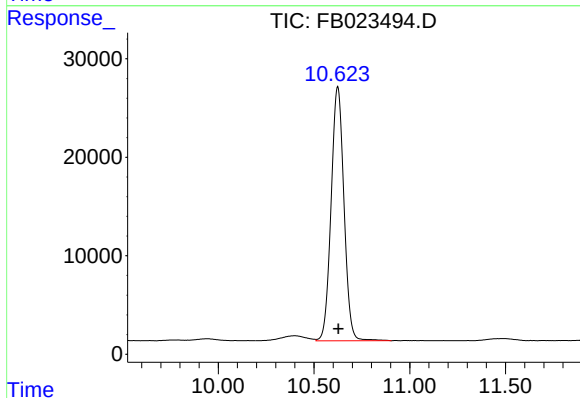


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 1201537
Conc: 30.40 ng/ml

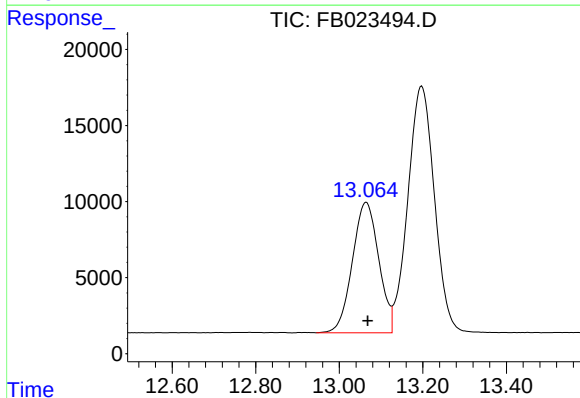


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 374911
Conc: 10.04 ng/ml

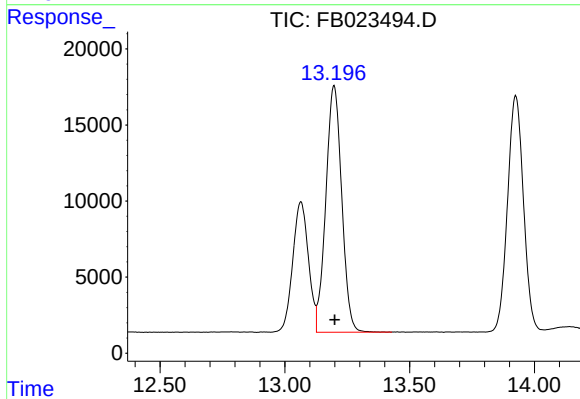

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: -0.003 min
Response: 716822
Conc: 20.16 ng/ml

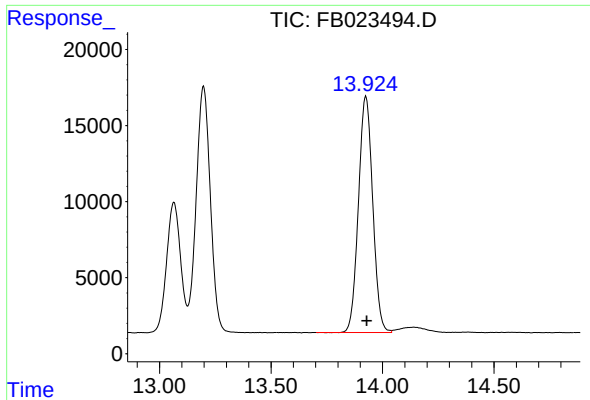

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.004 min
Response: 690946
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0124S1

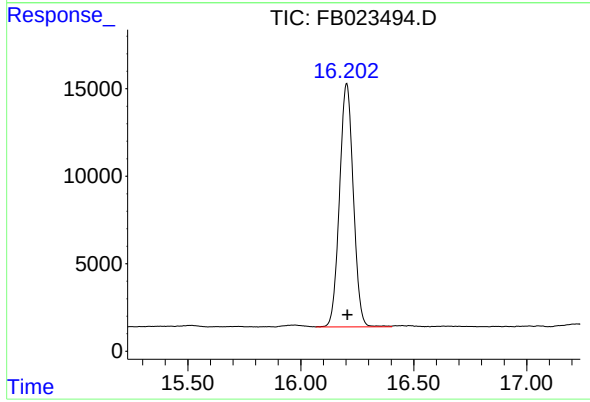

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.004 min
Response: 590637
Conc: 20.20 ng/ml