

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023501.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 13:14
Operator : DD/AJ
Sample : L1007-20MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS

Integration File: Calibration.e
Quant Time: Jan 24 21:47:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023501.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 13:14
Operator : DD/AJ
Sample : L1007-20MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS

Integration File: Calibration.e
Quant Time: Jan 24 21:47:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

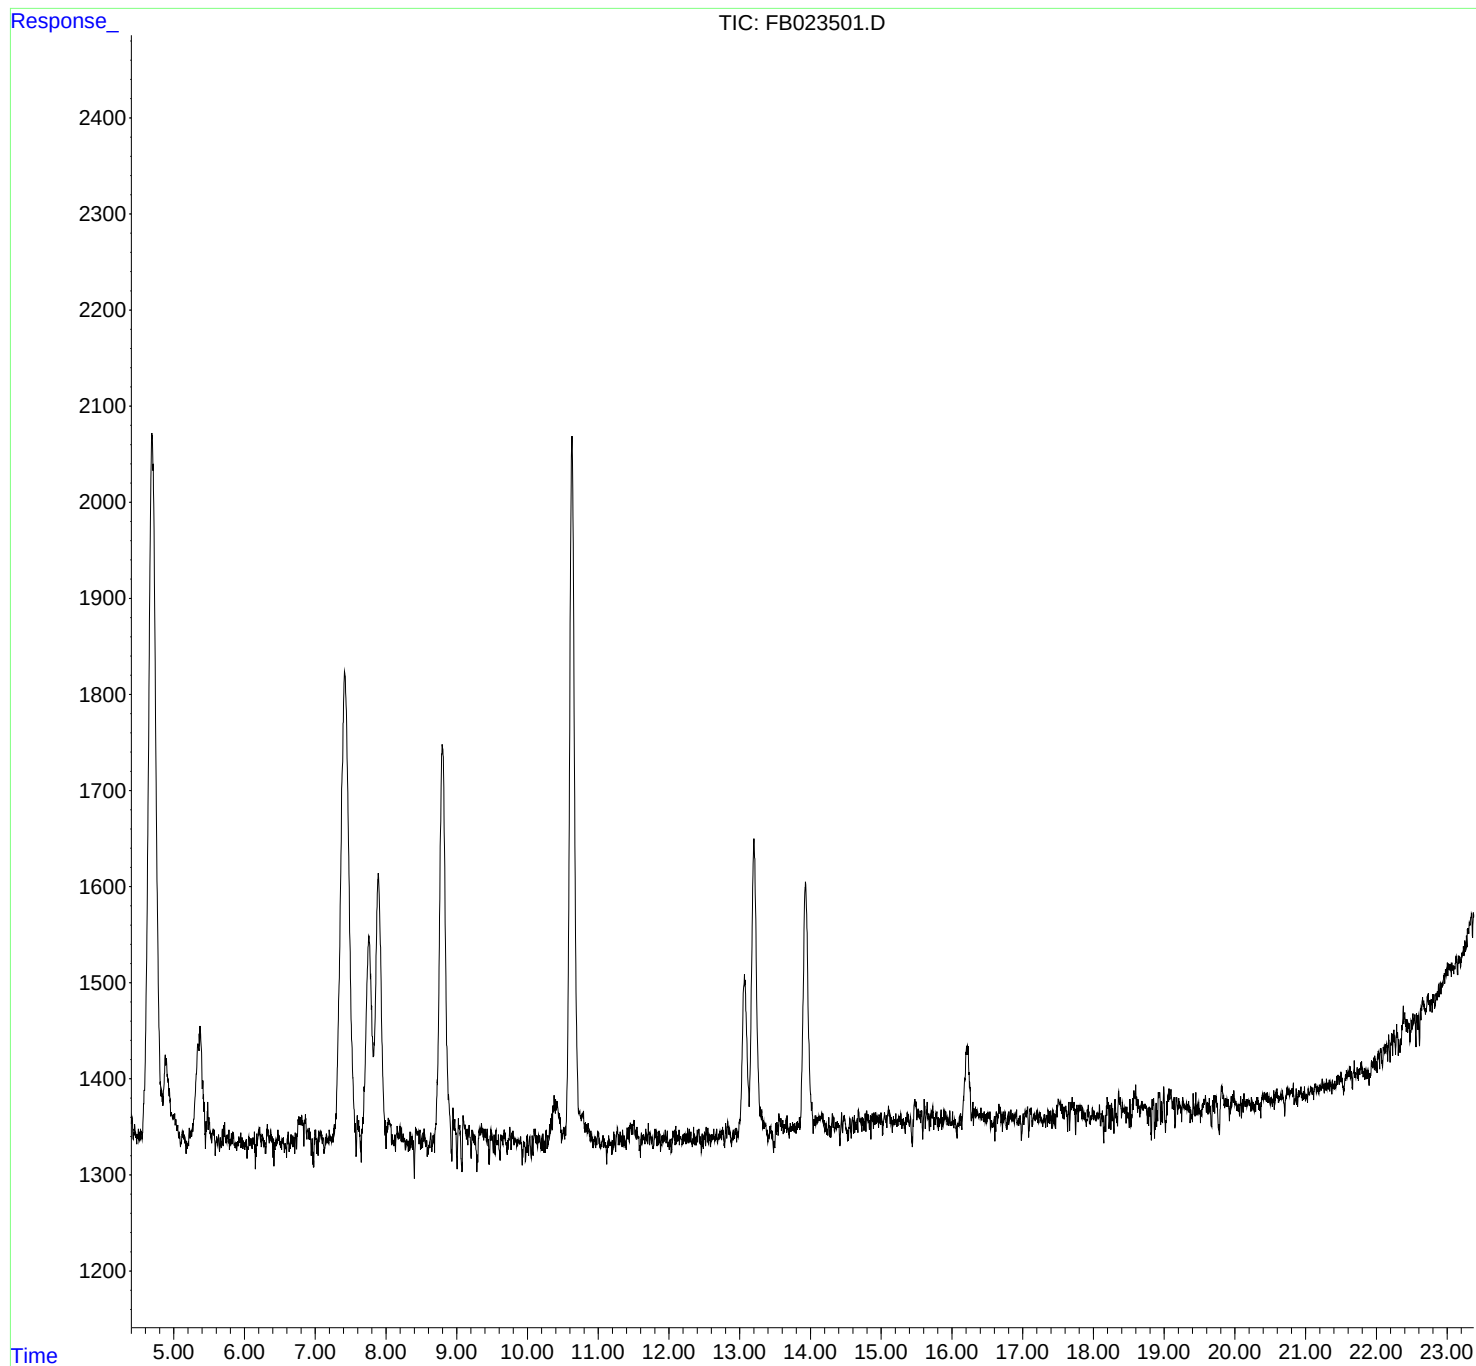

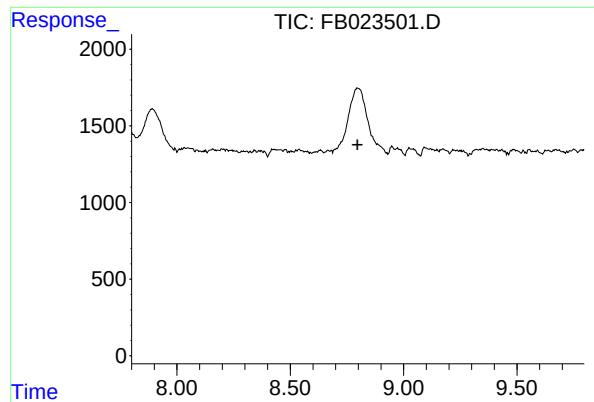

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.797 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS