

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023502.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 14:14
 Operator : DD/AJ
 Sample : L1007-20MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 JC-03-012320-CMS

Integration File: Calibration.e
 Quant Time: Jan 24 21:48:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	477344	20.096 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	941164	29.783 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1044070	30.750 ng/ml
3) t n-Heptane	7.755	342138	10.217 ng/ml
4) t Benzene	7.888	409147	10.019 ng/ml
6) t Toluene	10.626	1188255	30.068 ng/ml
7) t Ethylbenzene	13.067	364106	9.749 ng/ml
8) t m-Xylene	13.200	697729	19.621 ng/ml
9) t O-Xylene	13.927	674502	19.520 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	573321	19.607 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023502.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 14:14
Operator : DD/AJ
Sample : L1007-20MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS

Integration File: Calibration.e
Quant Time: Jan 24 21:48:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

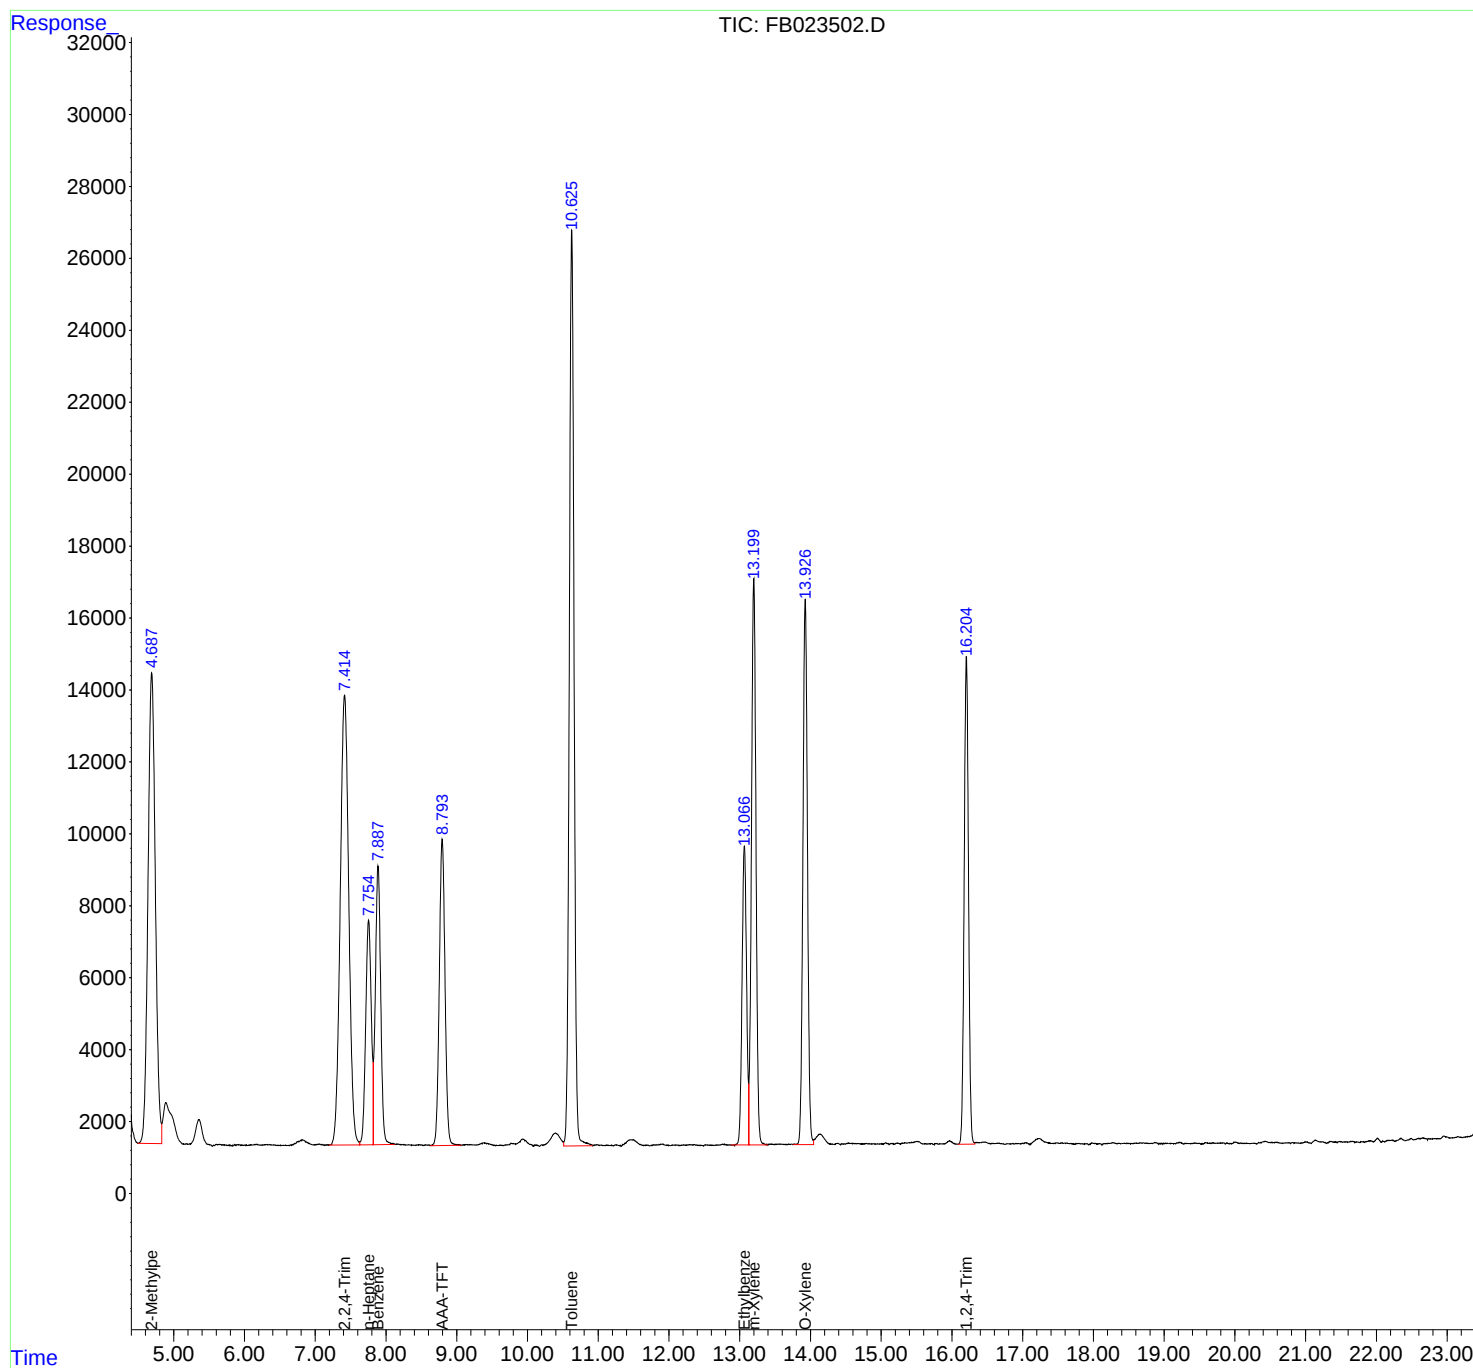


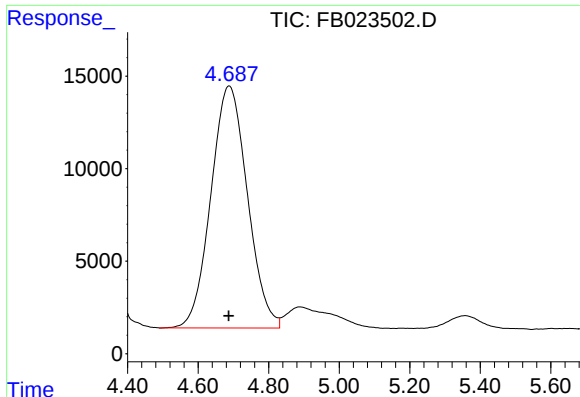

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 941164
Conc: 29.78 ng/ml

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS

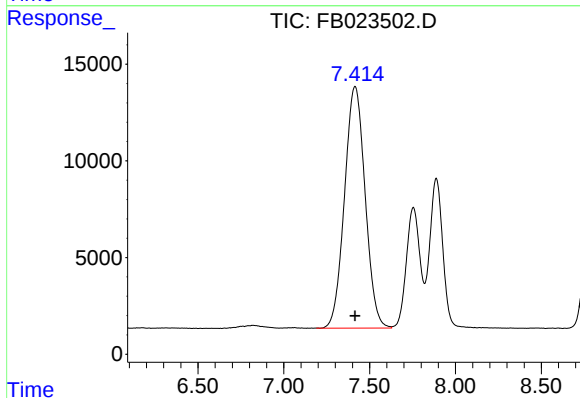


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 1044070
Conc: 30.75 ng/ml

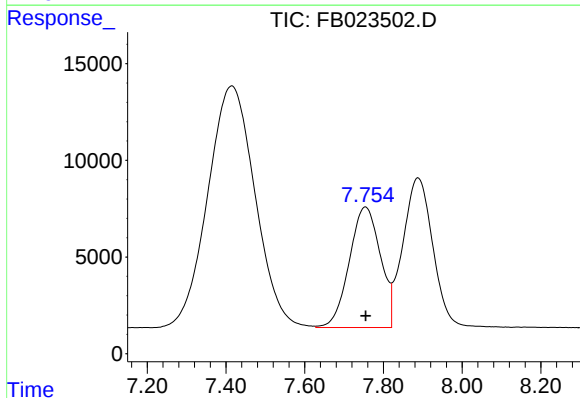


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 342138
Conc: 10.22 ng/ml

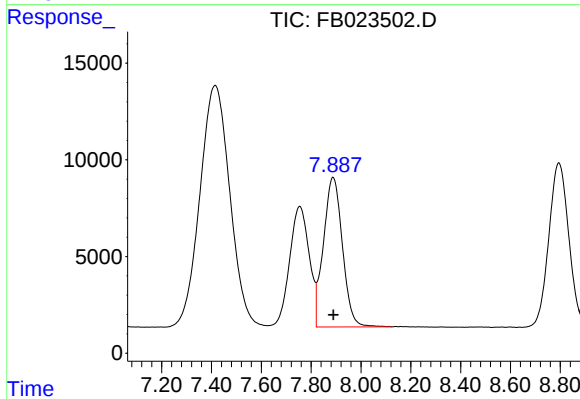

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 409147
Conc: 10.02 ng/ml

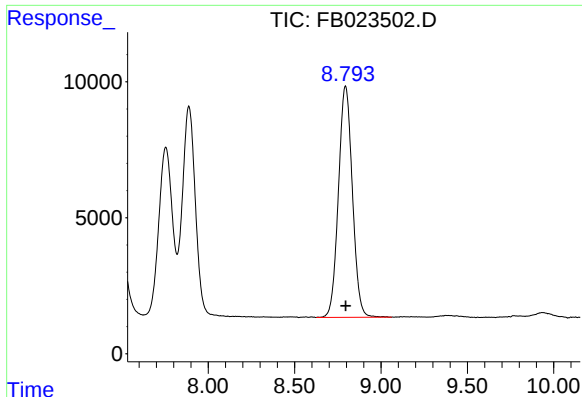

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 477344
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS

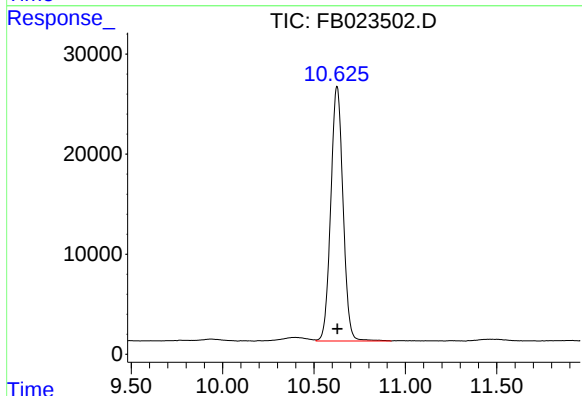


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 1188255
Conc: 30.07 ng/ml

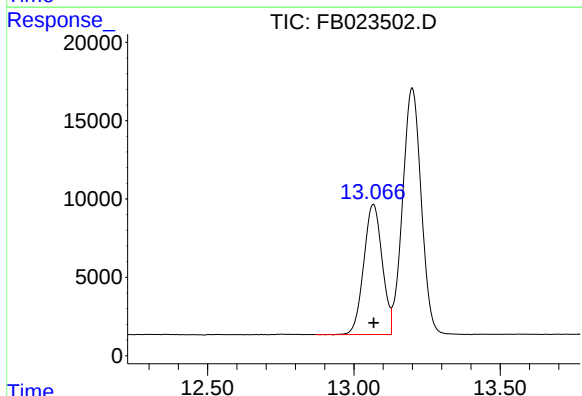


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.002 min
Response: 364106
Conc: 9.75 ng/ml

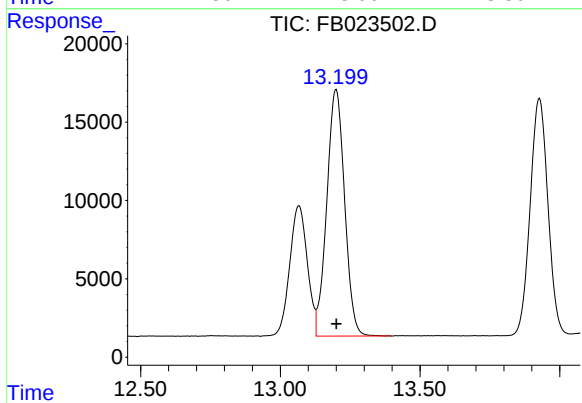

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.001 min
Response: 697729
Conc: 19.62 ng/ml

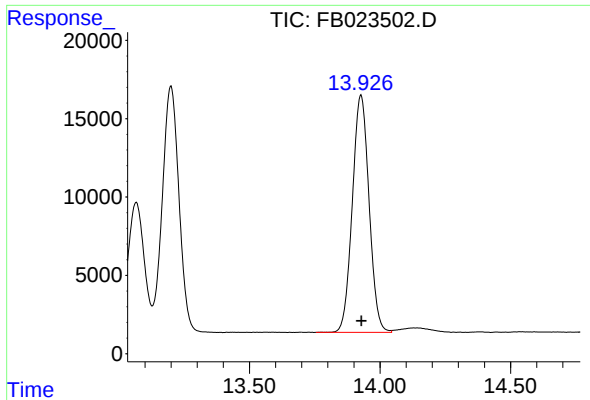

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 674502
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMS

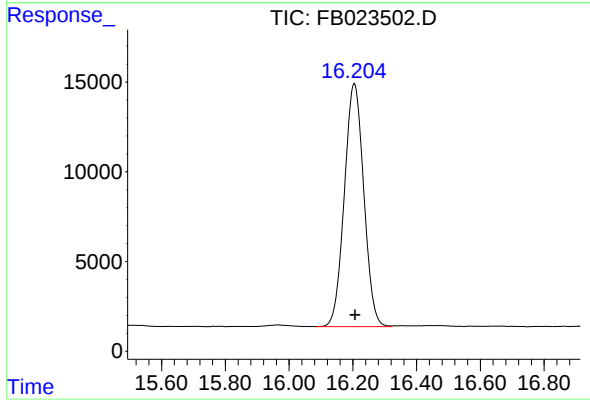

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 573321
Conc: 19.61 ng/ml