

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023507.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 17:00
Operator : DD/AJ
Sample : L1247-13
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-7-6-COMP

Integration File: Calibration.e
Quant Time: Jan 24 21:48:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	436626	18.381 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023507.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 17:00
Operator : DD/AJ
Sample : L1247-13
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-7-6-COMP

Integration File: Calibration.e
Quant Time: Jan 24 21:48:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

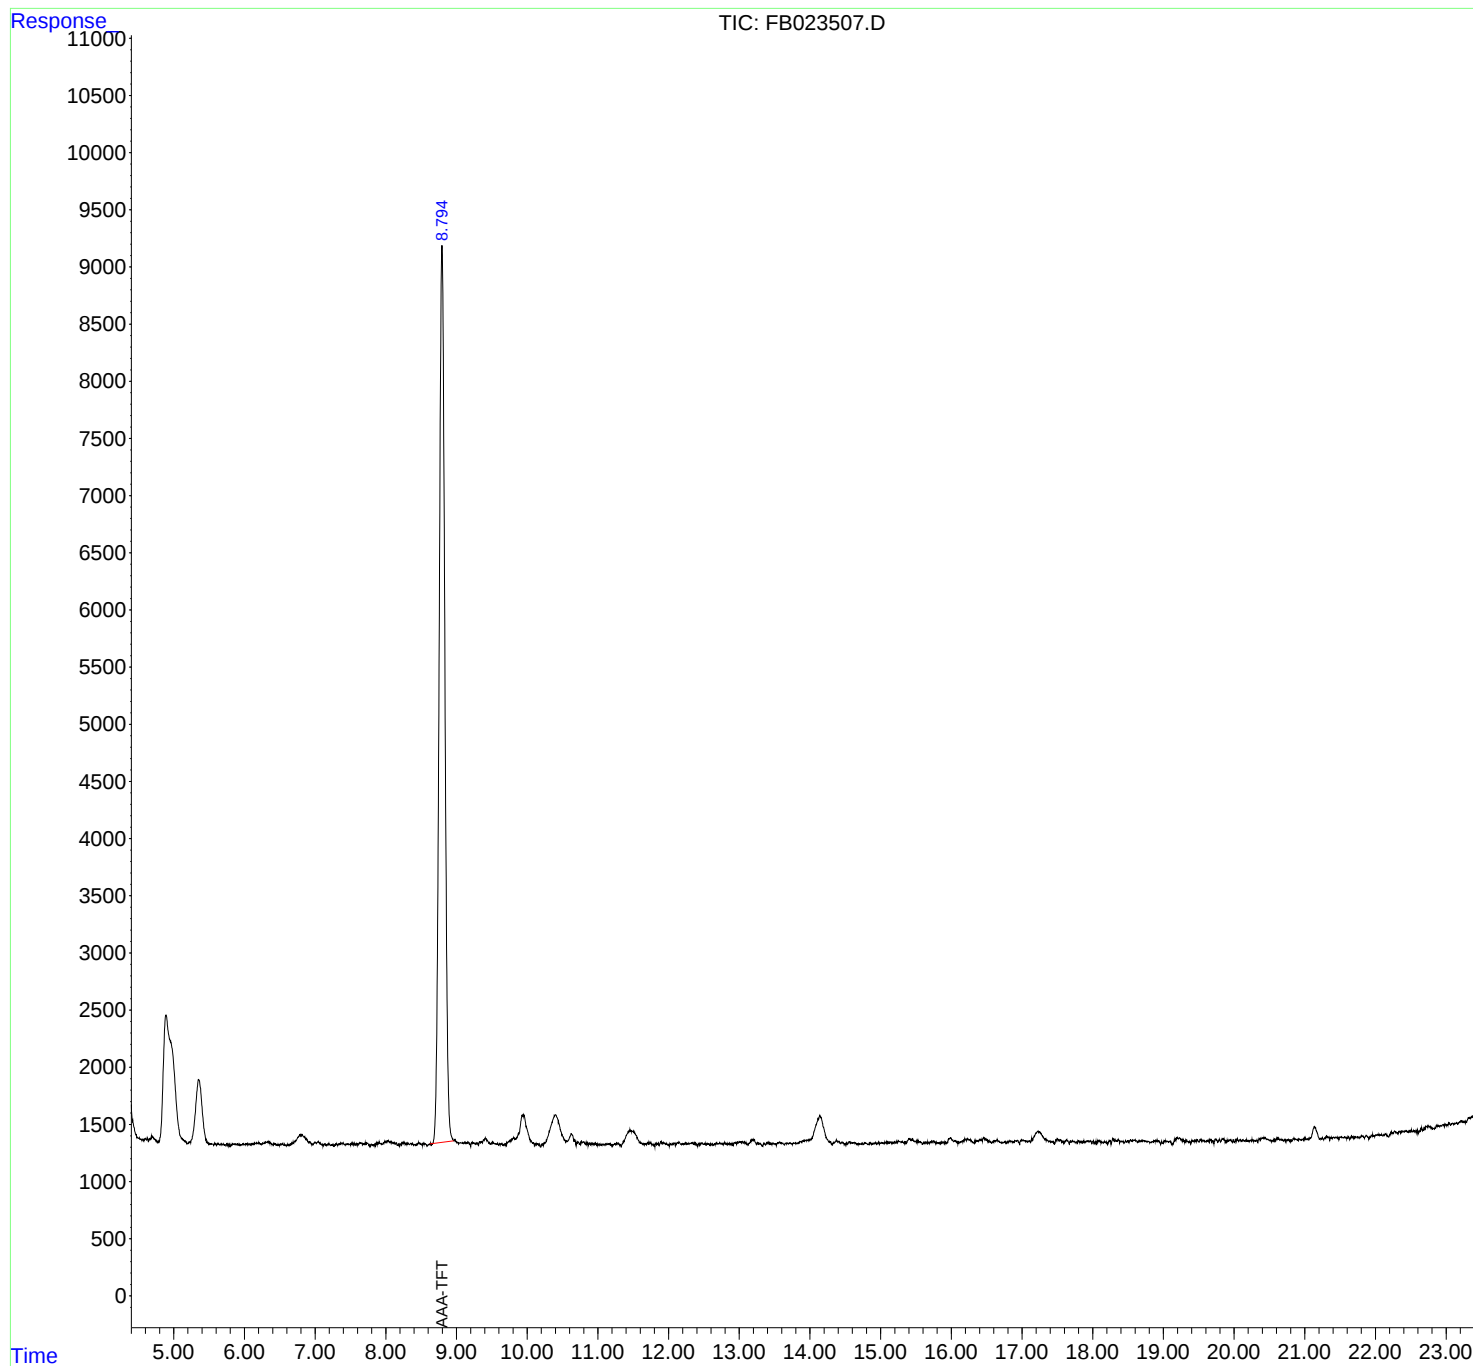

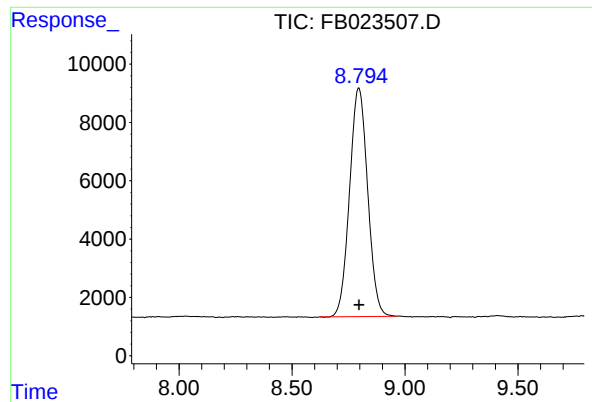

#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 436626
Conc: 18.38 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-7-6-COMP