

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023508.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 17:30
Operator : DD/AJ
Sample : L1247-14
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-7-6-COMP

Integration File: Calibration.e
Quant Time: Jan 24 21:49:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	481169	20.257 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023508.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 17:30
Operator : DD/AJ
Sample : L1247-14
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-7-6-COMP

Integration File: Calibration.e
Quant Time: Jan 24 21:49:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

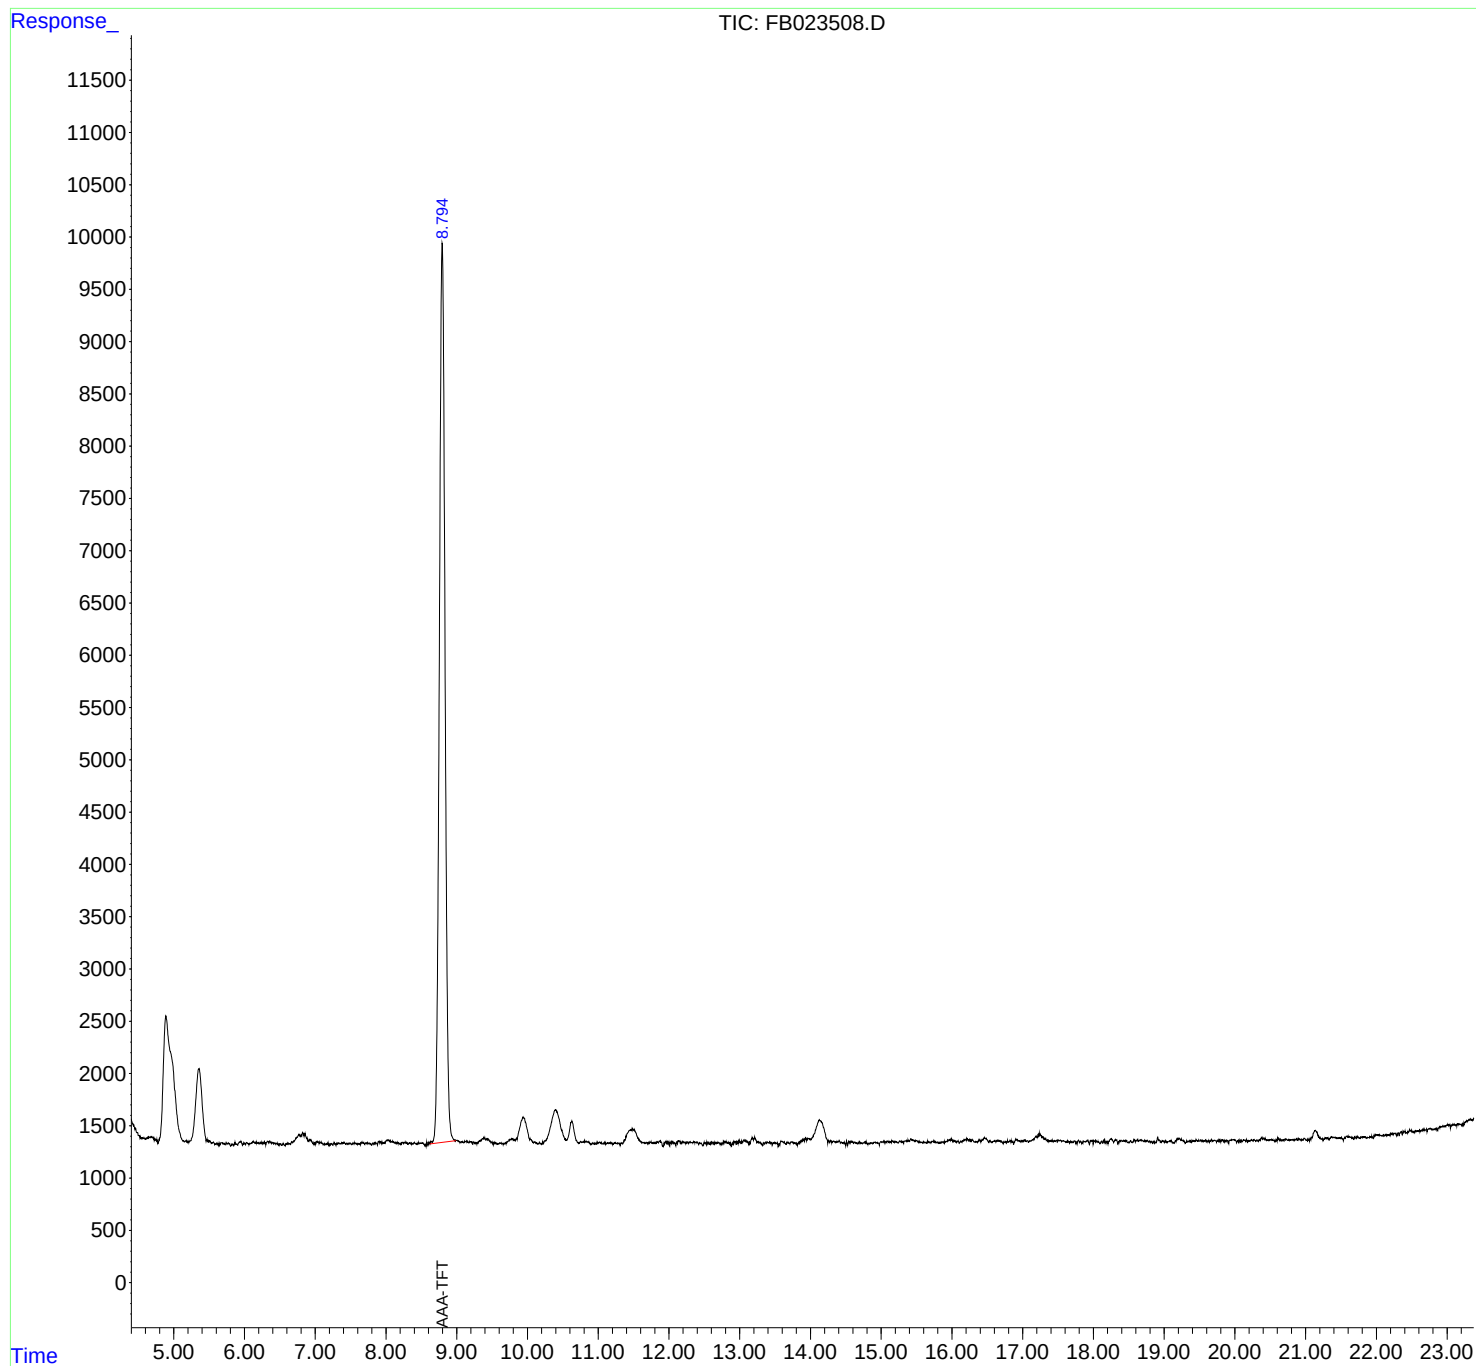

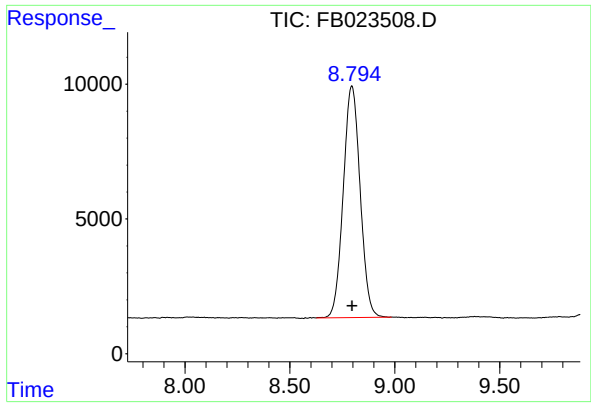

#5 AAA-TFT

R.T.: 8.796 min

Delta R.T.: -0.001 min

Response: 481169

Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-7-6-COMP