

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
 Data File : FB023513.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2020 20:02
 Operator : DD/AJ
 Sample : L1007-20MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 JC-03-012320-CMSD

Integration File: Calibration.e
 Quant Time: Feb 05 08:22:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	523936	22.057 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	958520	30.332 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1063988	31.337 ng/ml
3) t n-Heptane	7.754	347371	10.373 ng/ml
4) t Benzene	7.888	415859	10.183 ng/ml
6) t Toluene	10.626	1216692	30.788 ng/ml
7) t Ethylbenzene	13.066	374215	10.020 ng/ml
8) t m-Xylene	13.199	711308	20.003 ng/ml
9) t O-Xylene	13.927	692071	20.029 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	602674	20.611 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012420\
Data File : FB023513.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2020 20:02
Operator : DD/AJ
Sample : L1007-20MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMSD

Integration File: Calibration.e
Quant Time: Feb 05 08:22:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

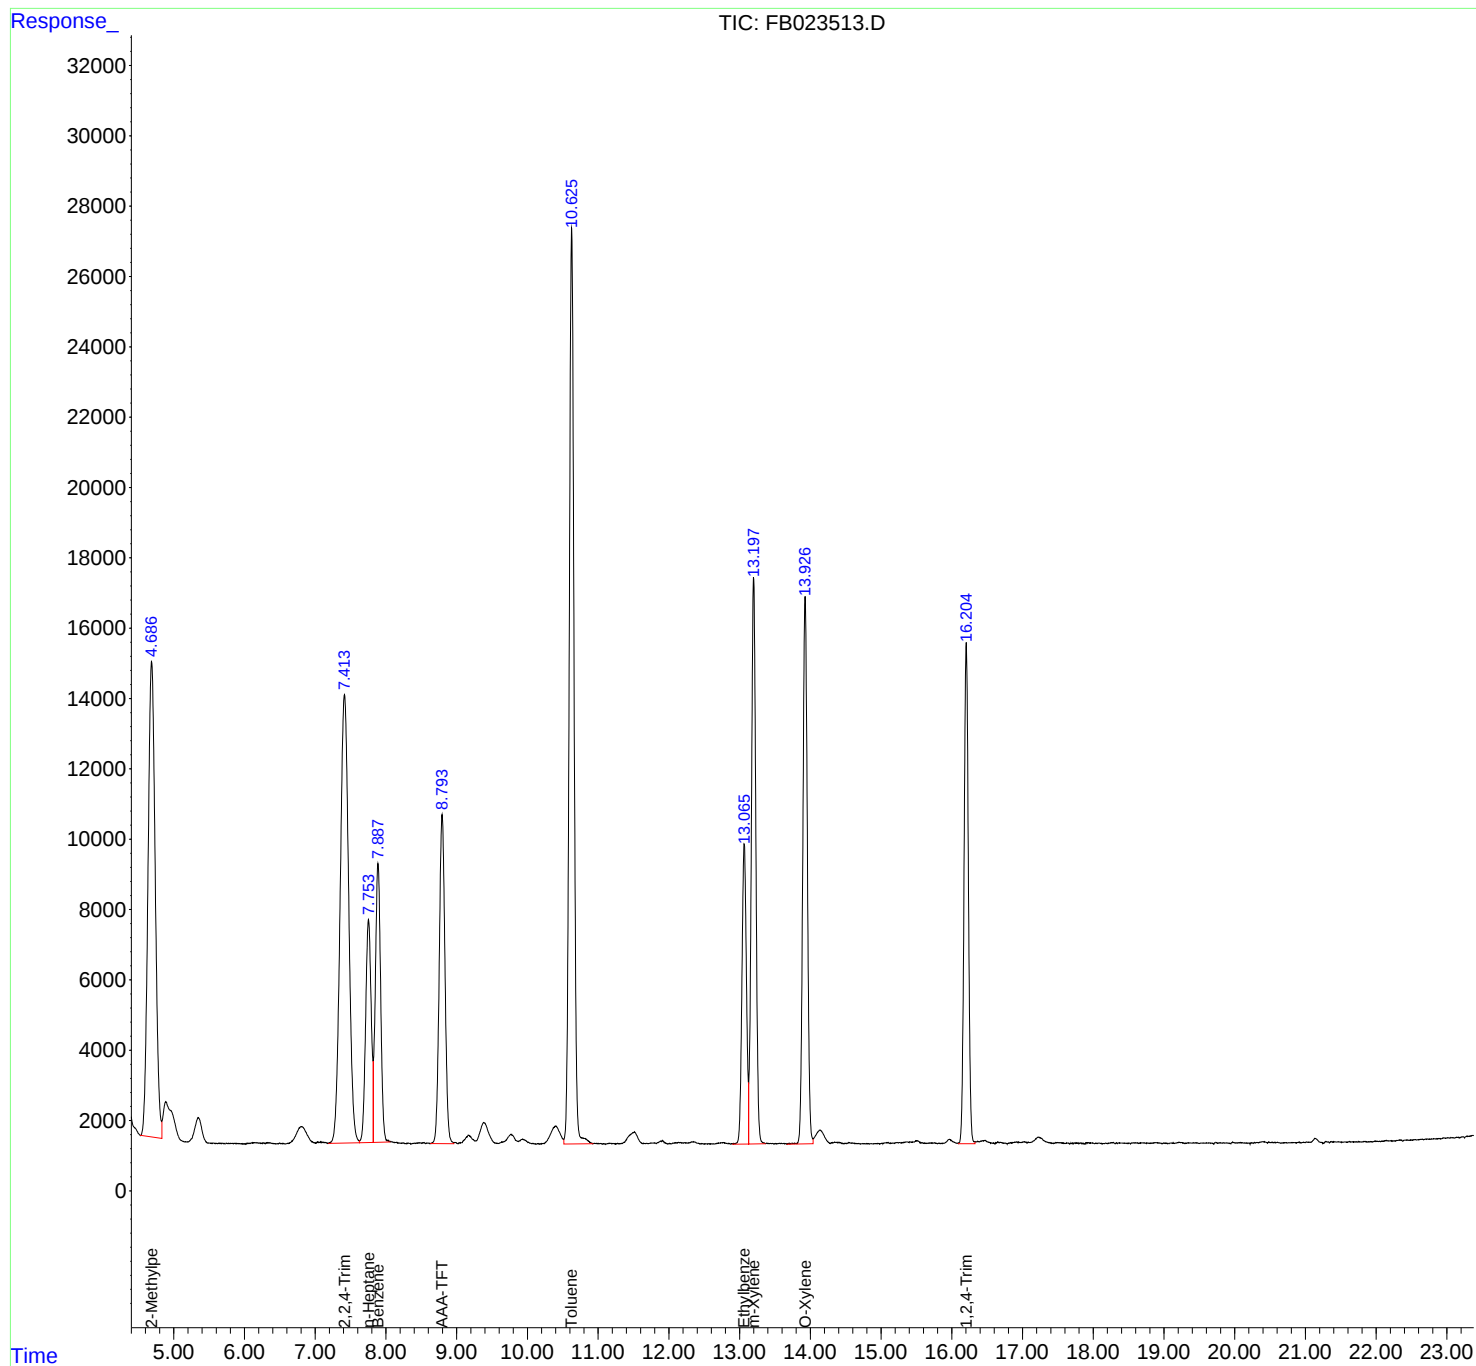


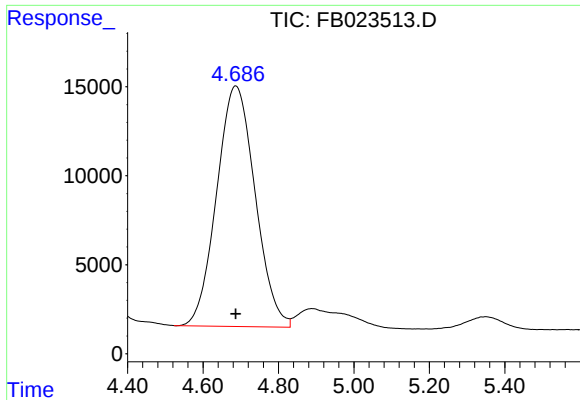

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 958520
Conc: 30.33 ng/ml

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMSD

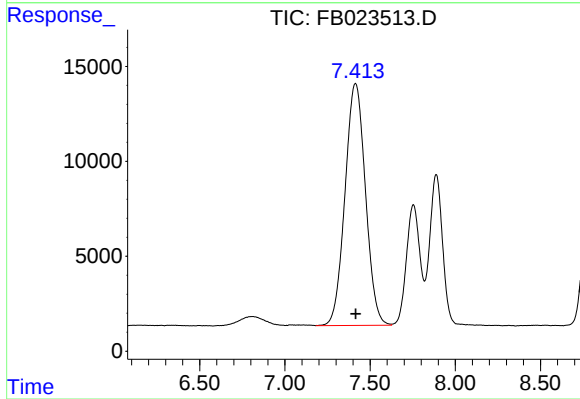


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.000 min
Response: 1063988
Conc: 31.34 ng/ml

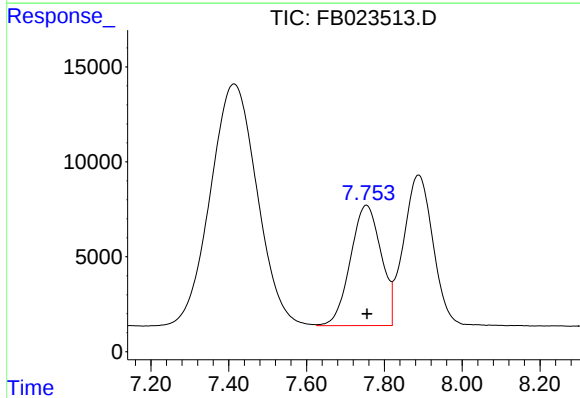


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.001 min
Response: 347371
Conc: 10.37 ng/ml

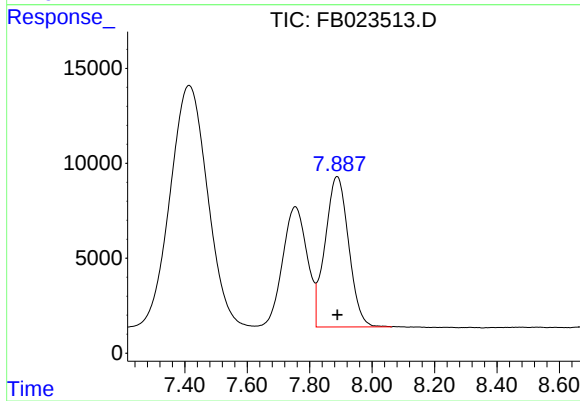

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 415859
Conc: 10.18 ng/ml

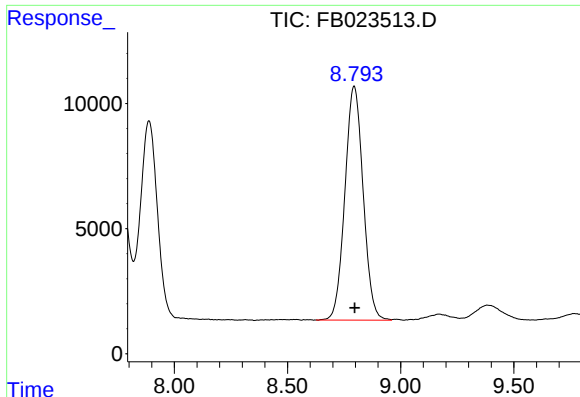

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 523936
Conc: 22.06 ng/ml

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMSD

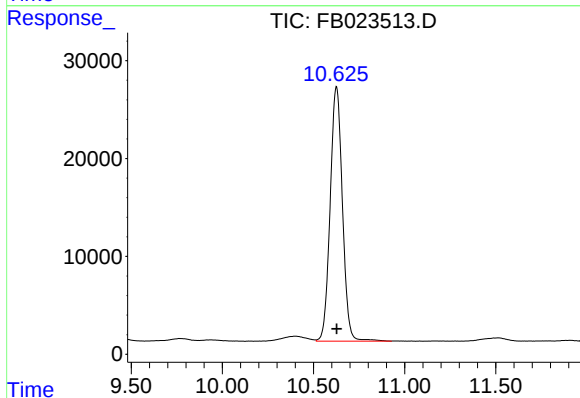


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 1216692
Conc: 30.79 ng/ml

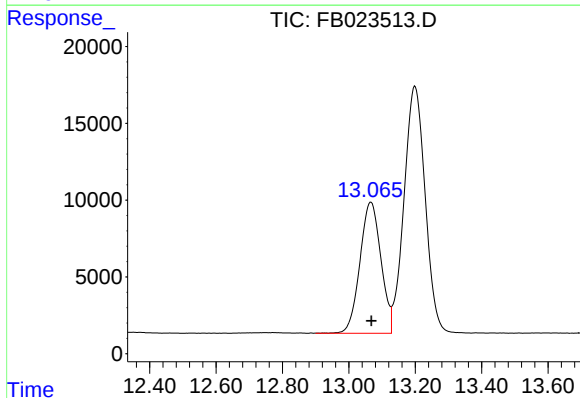


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.002 min
Response: 374215
Conc: 10.02 ng/ml

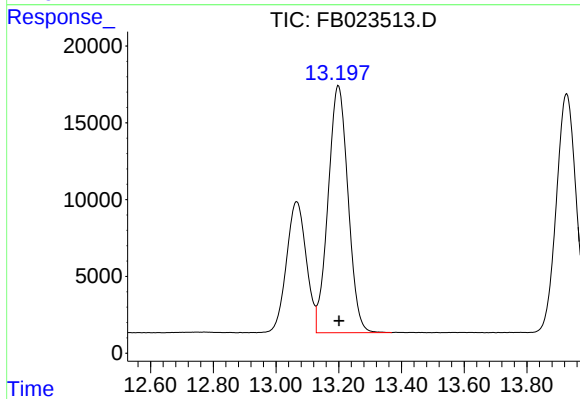

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 711308
Conc: 20.00 ng/ml

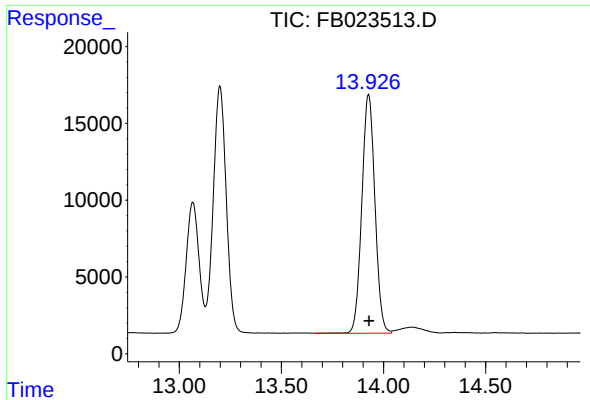

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 692071
Conc: 20.03 ng/ml

Instrument :
FID_B
ClientSampleId :
JC-03-012320-CMSD

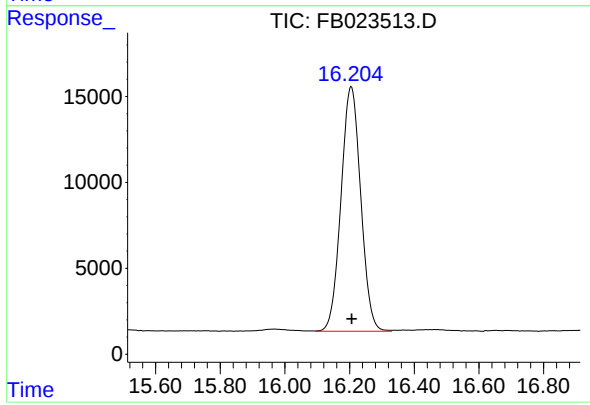

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 602674
Conc: 20.61 ng/ml