

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
 Data File : FB031328.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2025 9:50
 Operator : YP/AJ
 Sample : VBF0124S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 25 02:50:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	443029	18.574 ng/ml
Target Compounds			
6) t Toluene	10.610	478	0.012 ng/ml
8) t m-Xylene	13.182	5796	0.155 ng/ml
9) t O-Xylene	13.919	6065	0.170 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	5527	0.195 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
Data File : FB031328.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2025 9:50
Operator : YP/AJ
Sample : VBF0124S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 25 02:50:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

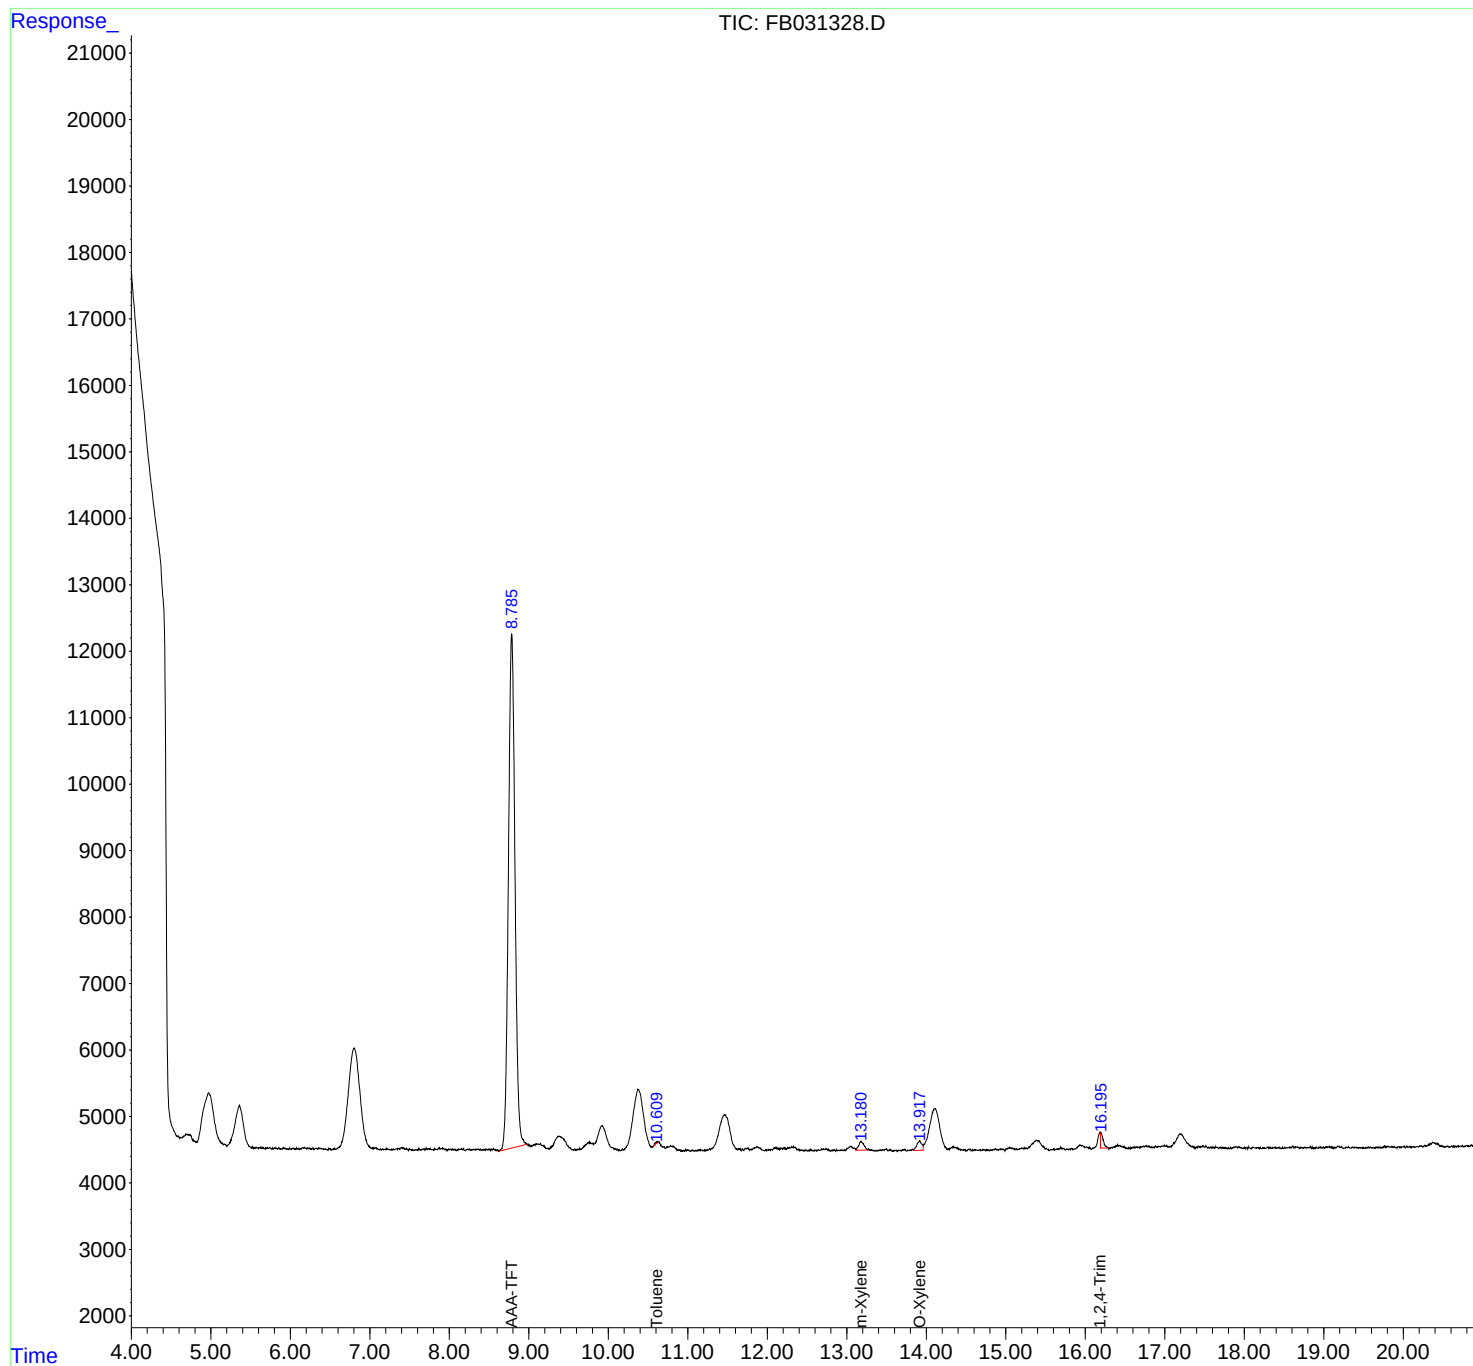


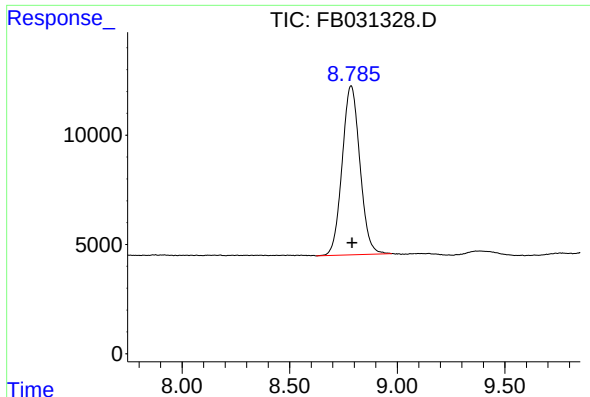

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.004 min
Response: 443029
Conc: 18.57 ng/ml

Instrument :
FID_B
ClientSampleId :

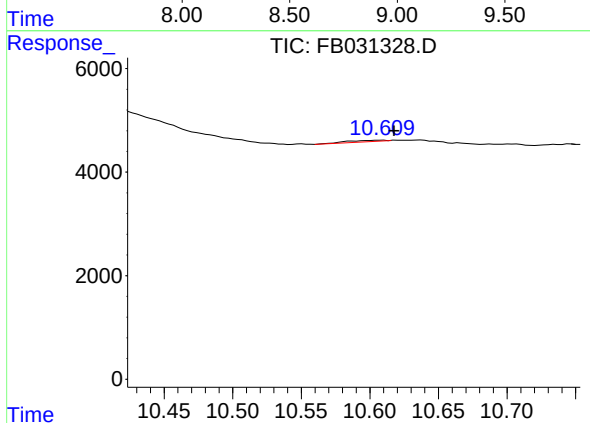


#6 Toluene

R.T.: 10.610 min
Delta R.T.: -0.008 min
Response: 478
Conc: 0.01 ng/ml

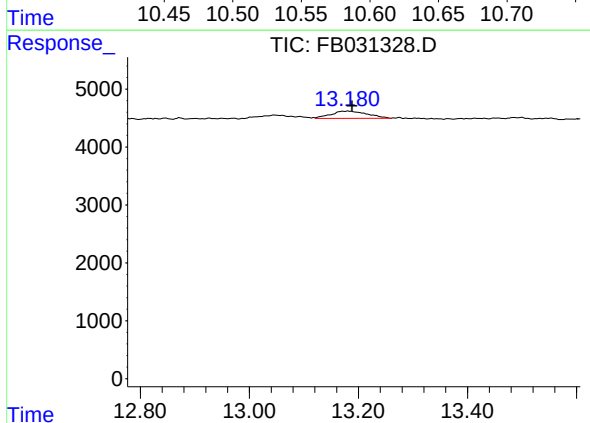


#8 m-Xylene

R.T.: 13.182 min
Delta R.T.: -0.006 min
Response: 5796
Conc: 0.16 ng/ml

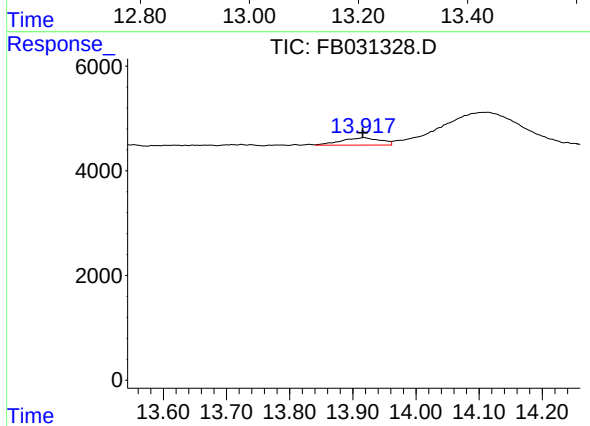

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 6065
Conc: 0.17 ng/ml

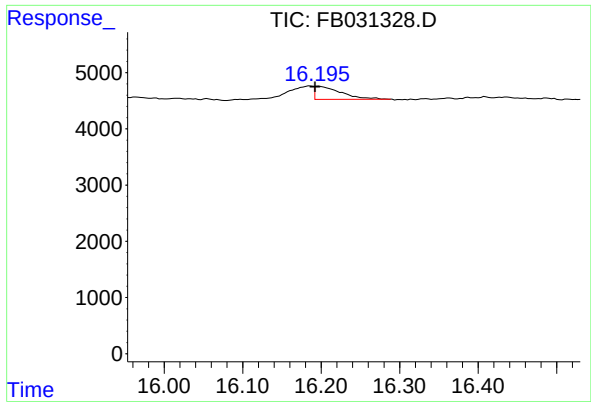

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 5527
Conc: 0.20 ng/ml

Instrument :
FID_B
ClientSampleId :