

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
 Data File : FB031330.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2025 10:43
 Operator : YP/AJ
 Sample : BSF0124S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 25 02:50:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	447743	18.771 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	1025229	30.931 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1178246	31.330 ng/ml
3) t n-Heptane	7.752	372732	10.325 ng/ml
4) t Benzene	7.891	439248	10.313 ng/ml
6) t Toluene	10.618	1250010	32.013 ng/ml
7) t Ethylbenzene	13.054	360152	10.400 ng/ml
8) t m-Xylene	13.188	776395	20.771 ng/ml
9) t O-Xylene	13.916	728884	20.467 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	572289	20.207 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
Data File : FB031330.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2025 10:43
Operator : YP/AJ
Sample : BSF0124S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 25 02:50:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

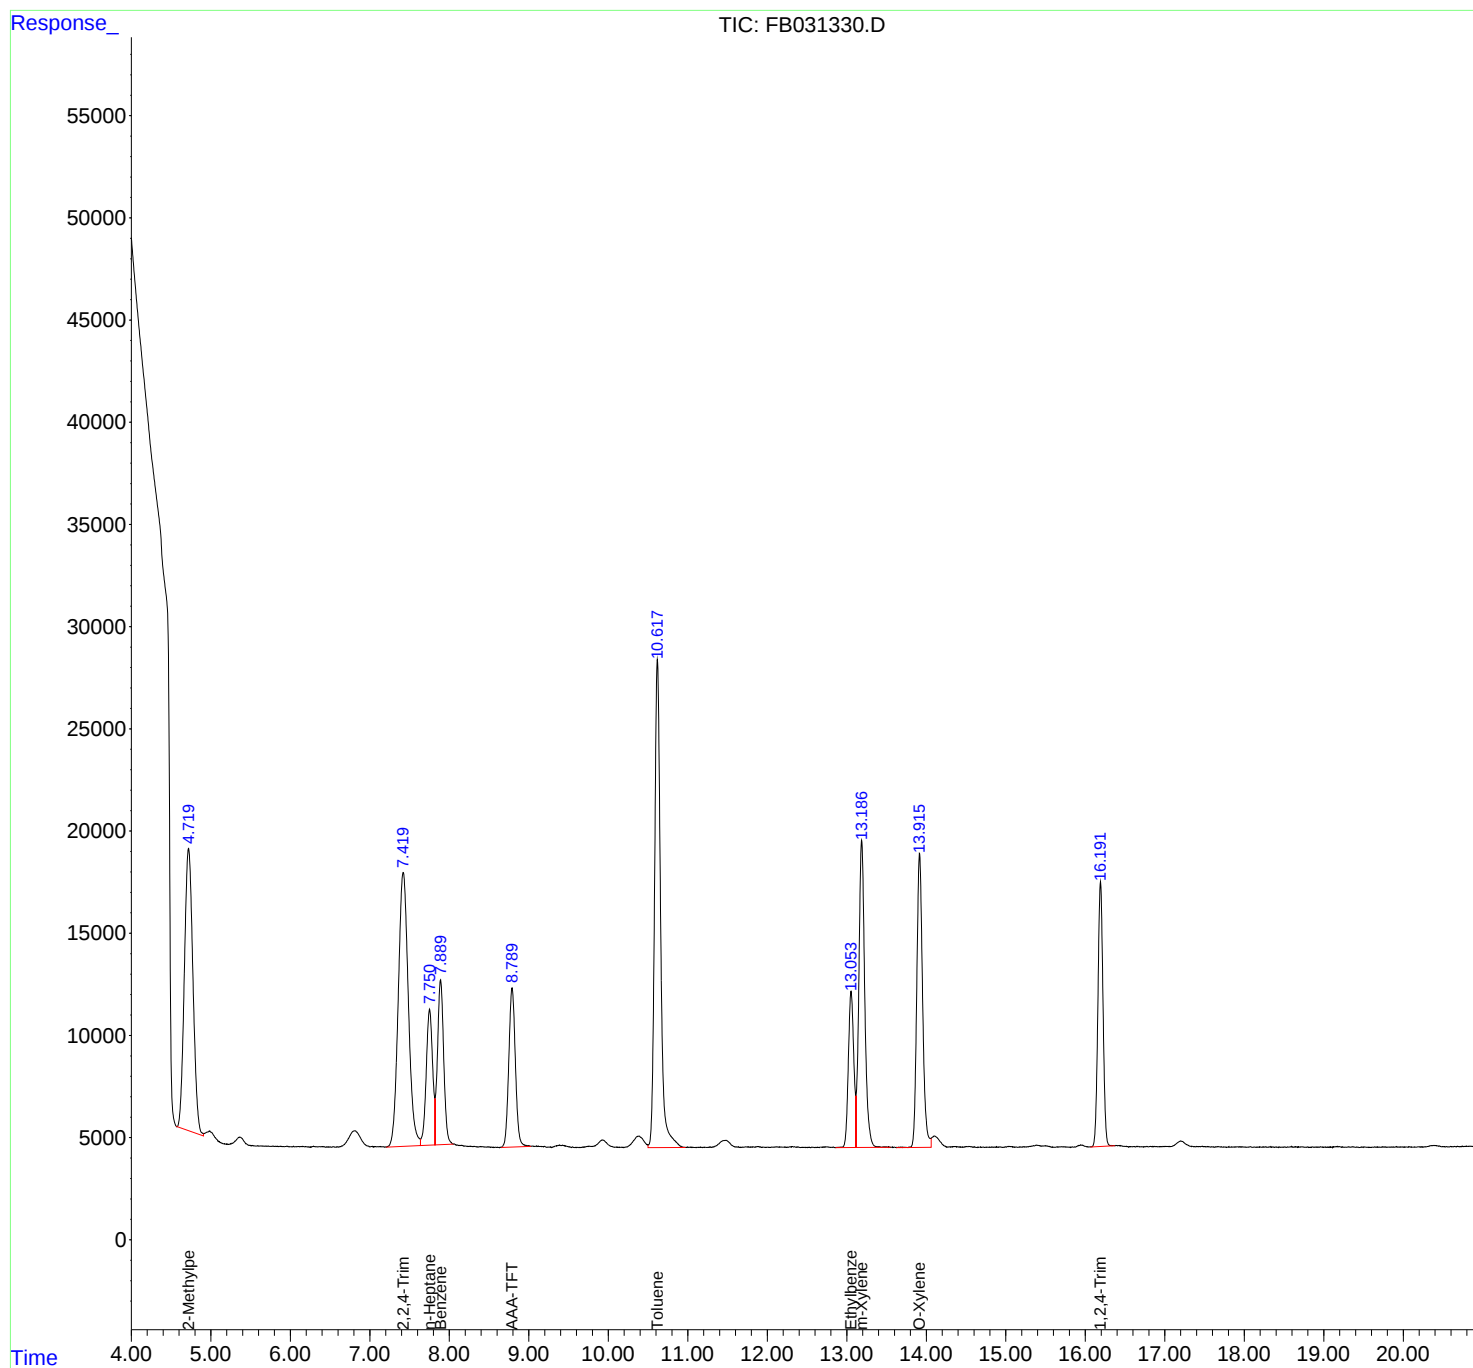


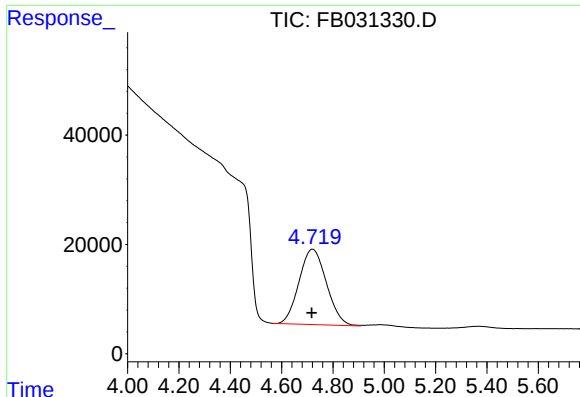

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: 0.003 min
Response: 1025229
Conc: 30.93 ng/ml

Instrument :
FID_B
ClientSampleId :

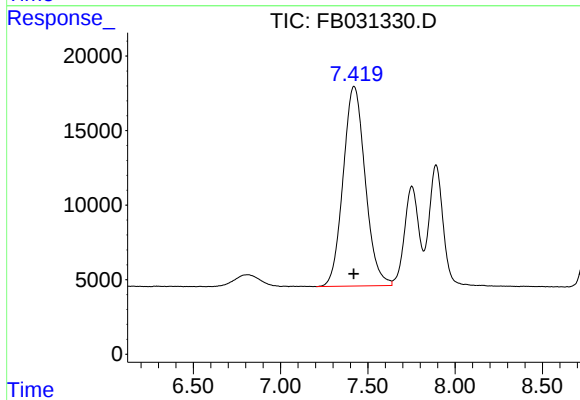


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 1178246
Conc: 31.33 ng/ml

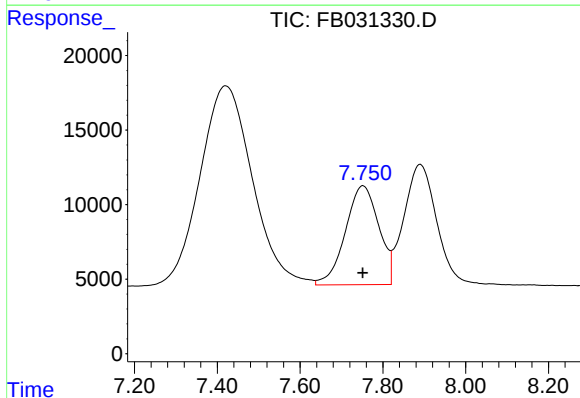


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 372732
Conc: 10.33 ng/ml

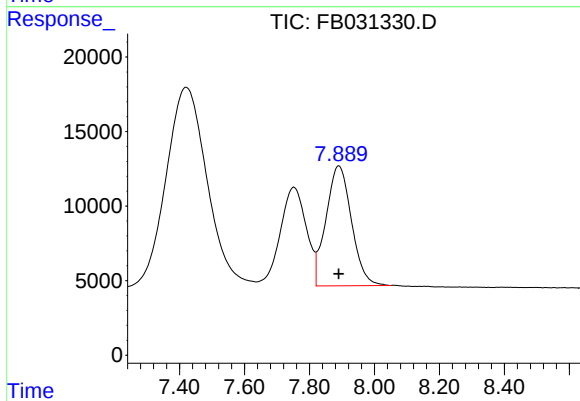

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 439248
Conc: 10.31 ng/ml

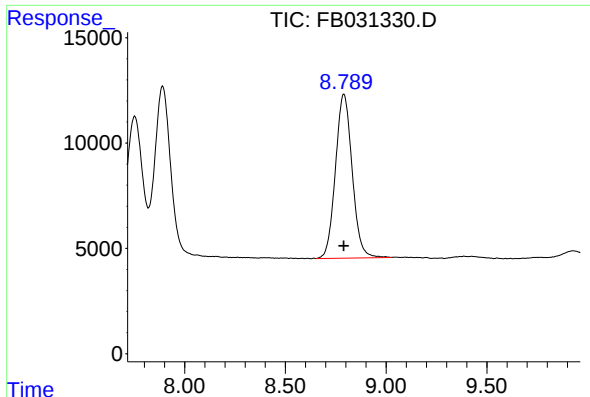

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 447743
Conc: 18.77 ng/ml

Instrument :
FID_B
ClientSampleId :

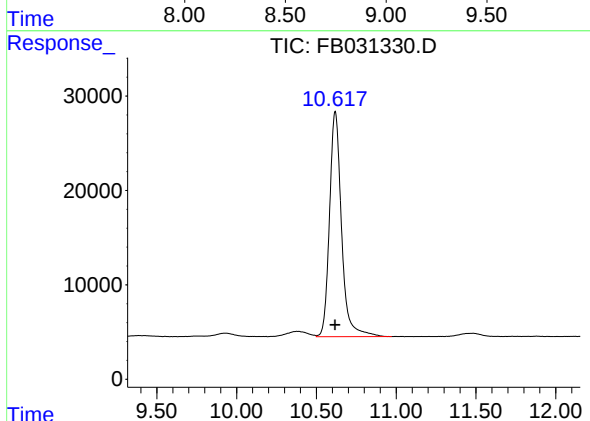


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 1250010
Conc: 32.01 ng/ml

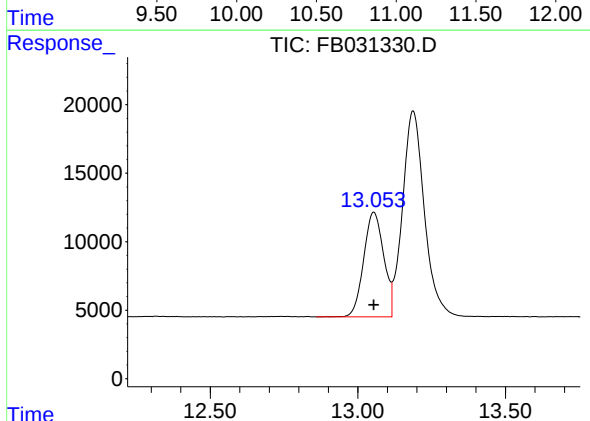


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 360152
Conc: 10.40 ng/ml

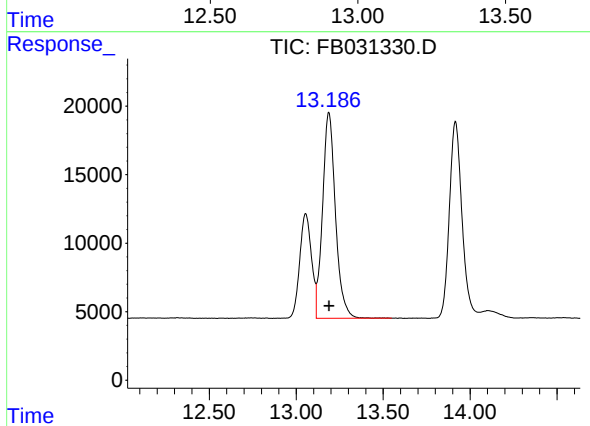

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 776395
Conc: 20.77 ng/ml

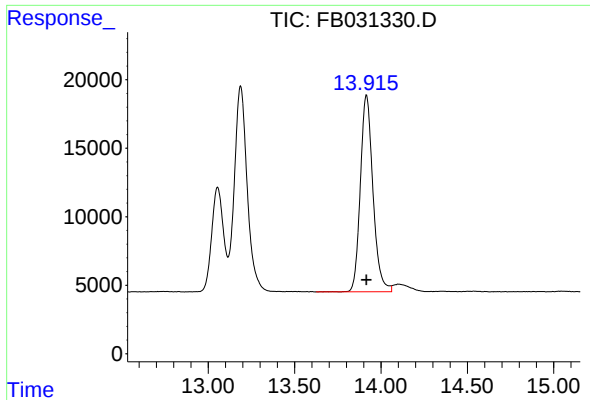

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 728884
Conc: 20.47 ng/ml

Instrument :
FID_B
ClientSampleId :

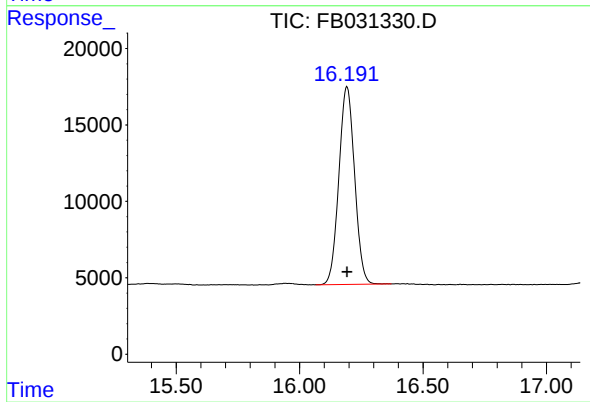

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 572289
Conc: 20.21 ng/ml