

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
 Data File : FB031334.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2025 12:44
 Operator : YP/AJ
 Sample : BSF0124S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 25 02:51:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	506863	21.250 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	1005747	30.343 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1186494	31.549 ng/ml
3) t n-Heptane	7.752	383281	10.617 ng/ml
4) t Benzene	7.891	466080	10.943 ng/ml
6) t Toluene	10.618	1259149	32.247 ng/ml
7) t Ethylbenzene	13.054	362074	10.456 ng/ml
8) t m-Xylene	13.188	781236	20.900 ng/ml
9) t O-Xylene	13.916	735714	20.658 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	574584	20.288 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
Data File : FB031334.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2025 12:44
Operator : YP/AJ
Sample : BSF0124S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 25 02:51:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

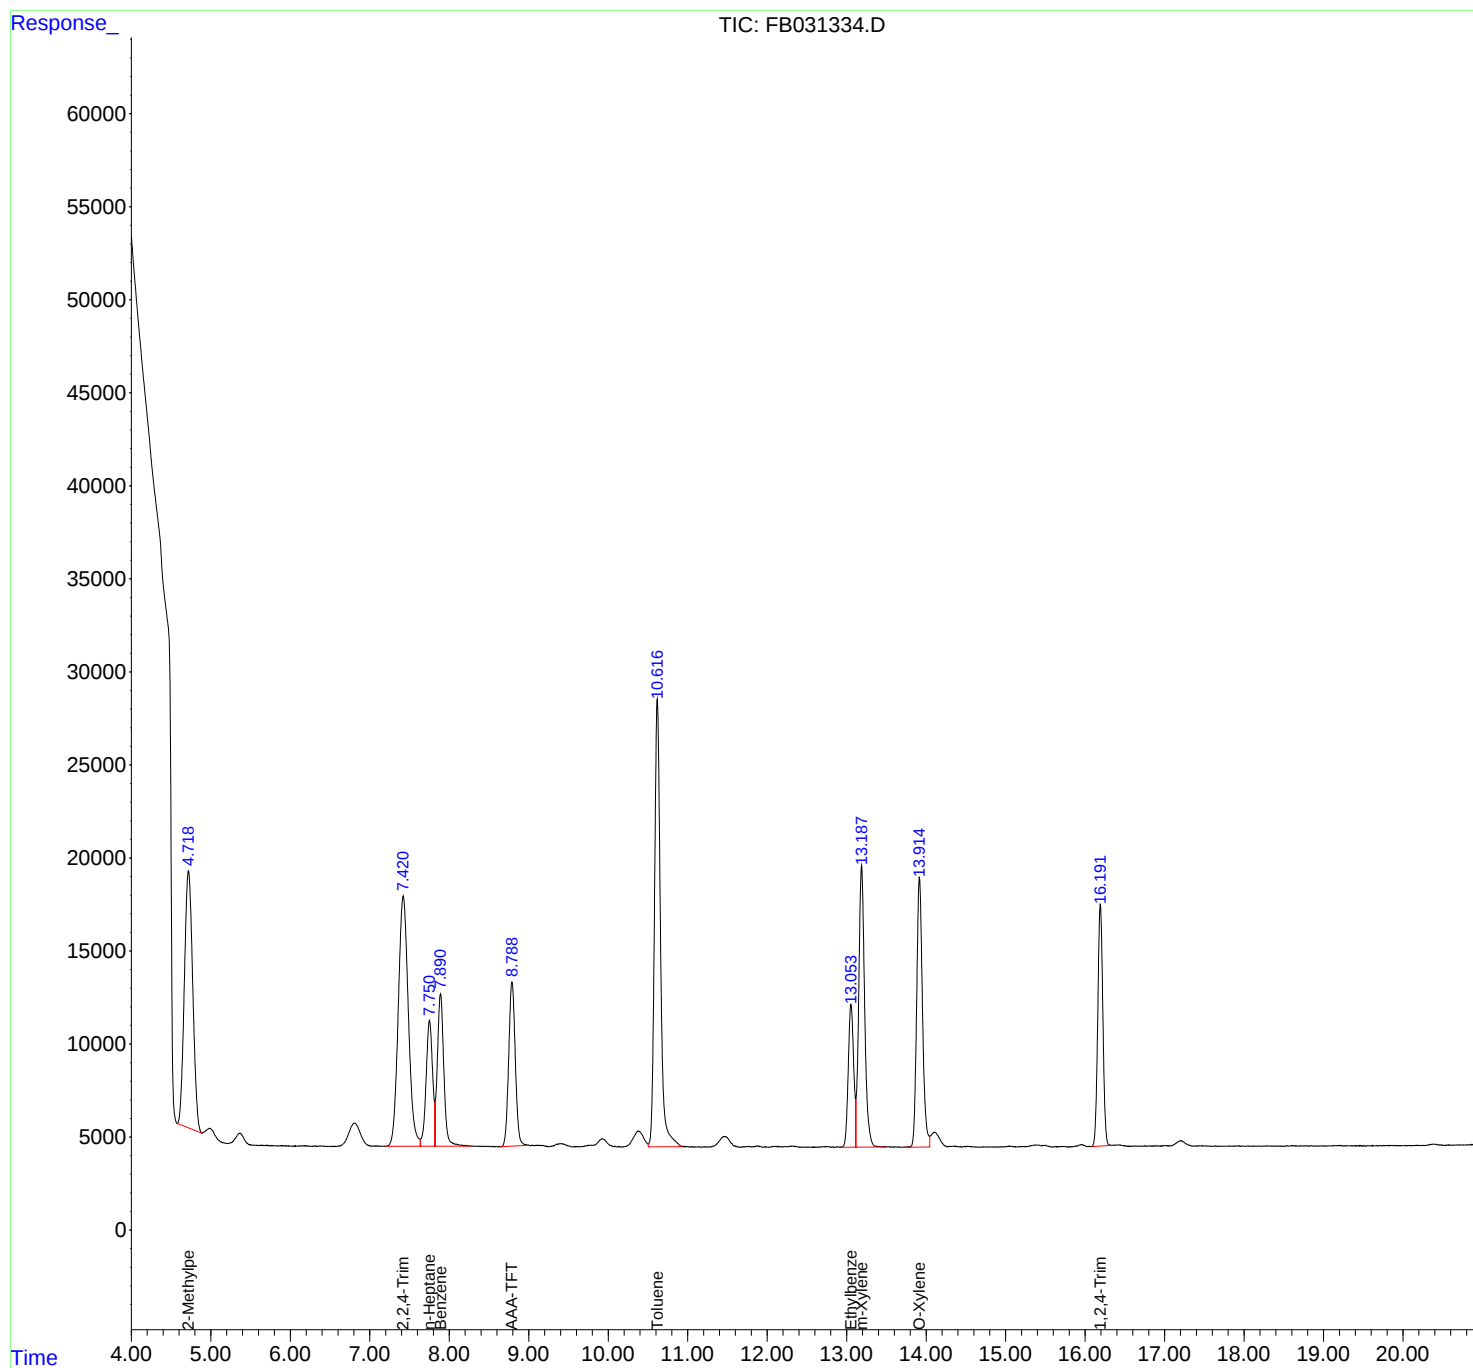


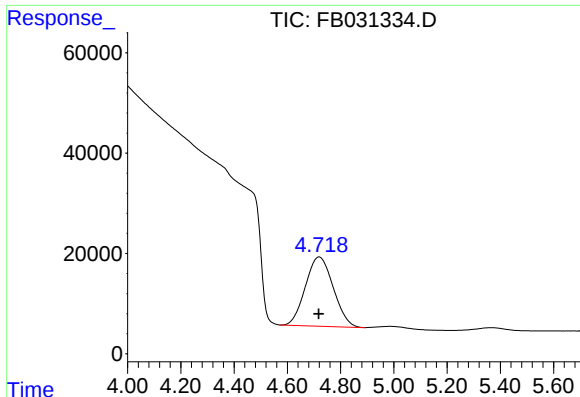

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.001 min
Response: 1005747
Conc: 30.34 ng/ml

Instrument :
FID_B
ClientSampleId :

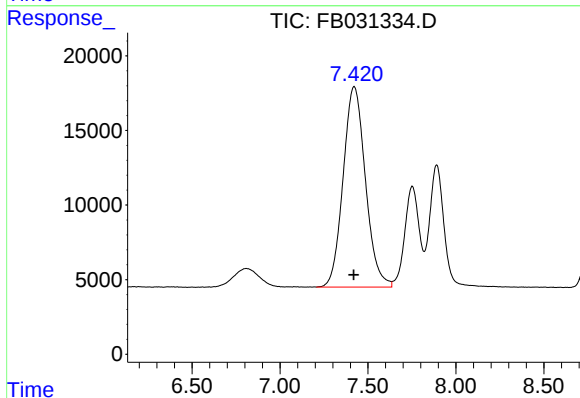


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.002 min
Response: 1186494
Conc: 31.55 ng/ml

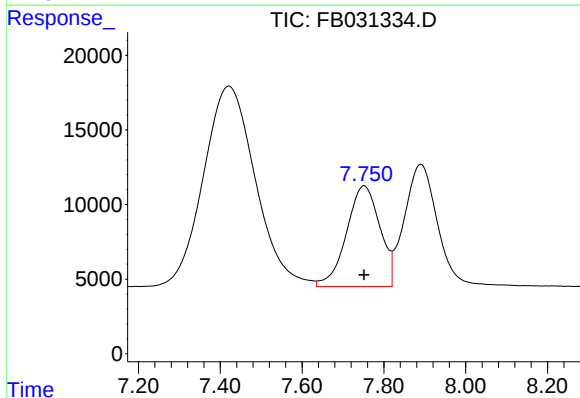


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 383281
Conc: 10.62 ng/ml

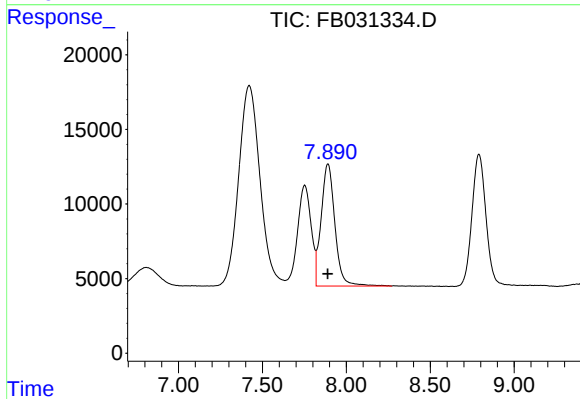

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.001 min
Response: 466080
Conc: 10.94 ng/ml

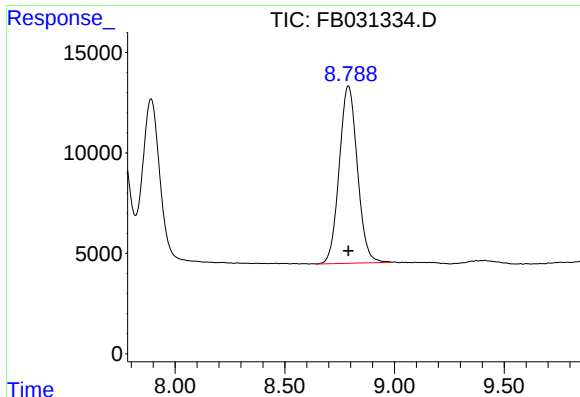

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 506863
Conc: 21.25 ng/ml

Instrument :
FID_B
ClientSampleId :

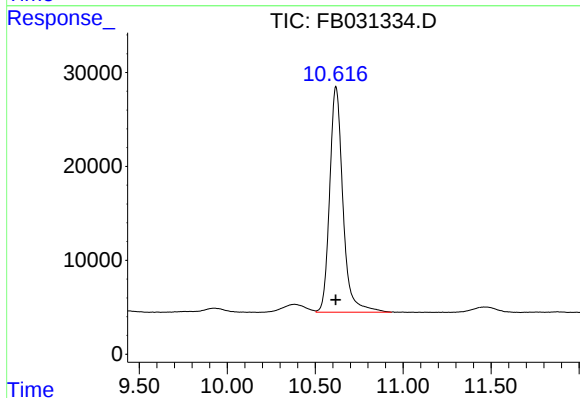


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 1259149
Conc: 32.25 ng/ml

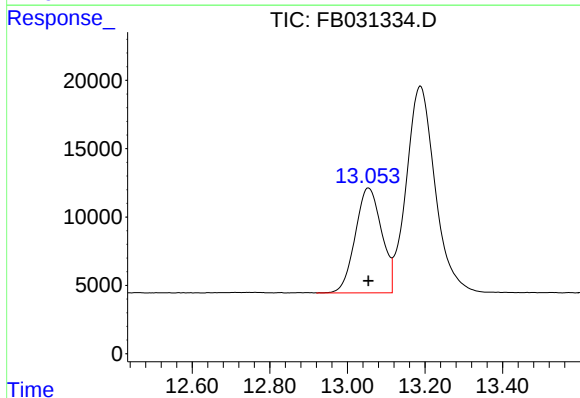


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 362074
Conc: 10.46 ng/ml

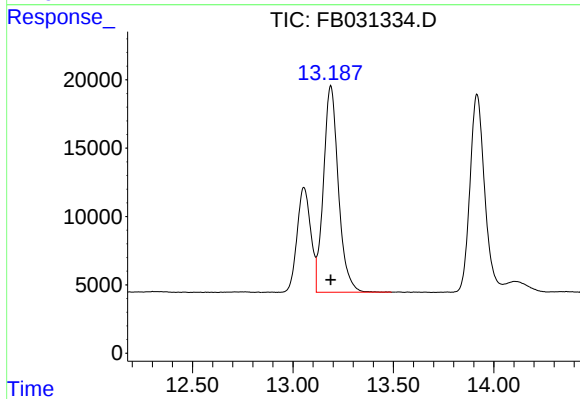

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 781236
Conc: 20.90 ng/ml

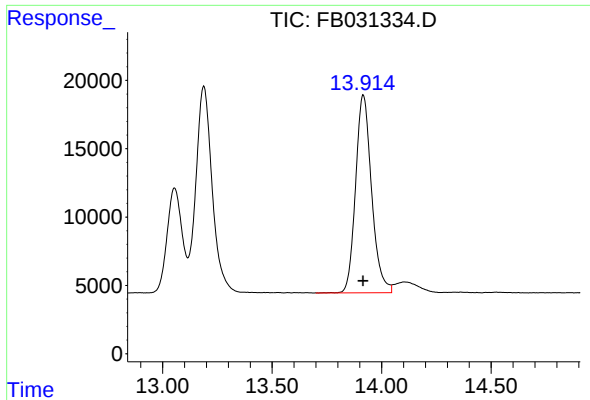

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 735714
Conc: 20.66 ng/ml

Instrument :
FID_B
ClientSampleId :

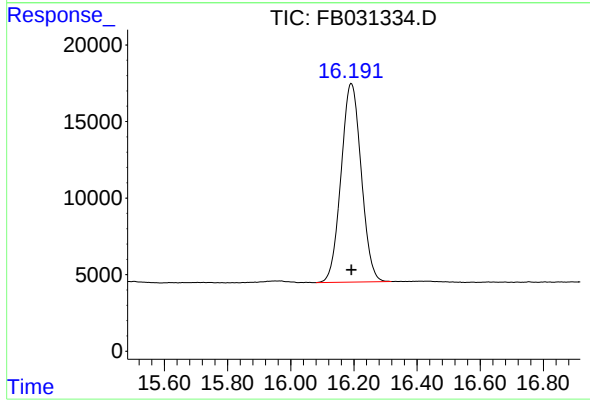

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 574584
Conc: 20.29 ng/ml