

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
 Data File : FB031336.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jan 2025 14:04
 Operator : YP/AJ
 Sample : VBF0124W1
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 25 02:51:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	463344	19.425 ng/ml
Target Compounds			
6) t Toluene	10.612	4063	0.104 ng/ml
8) t m-Xylene	13.198	5596	0.150 ng/ml
9) t O-Xylene	13.926	6531	0.183 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	12795	0.452 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012425\
Data File : FB031336.D
Signal(s) : FID2B.CH
Acq On : 24 Jan 2025 14:04
Operator : YP/AJ
Sample : VBF0124W1
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 25 02:51:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

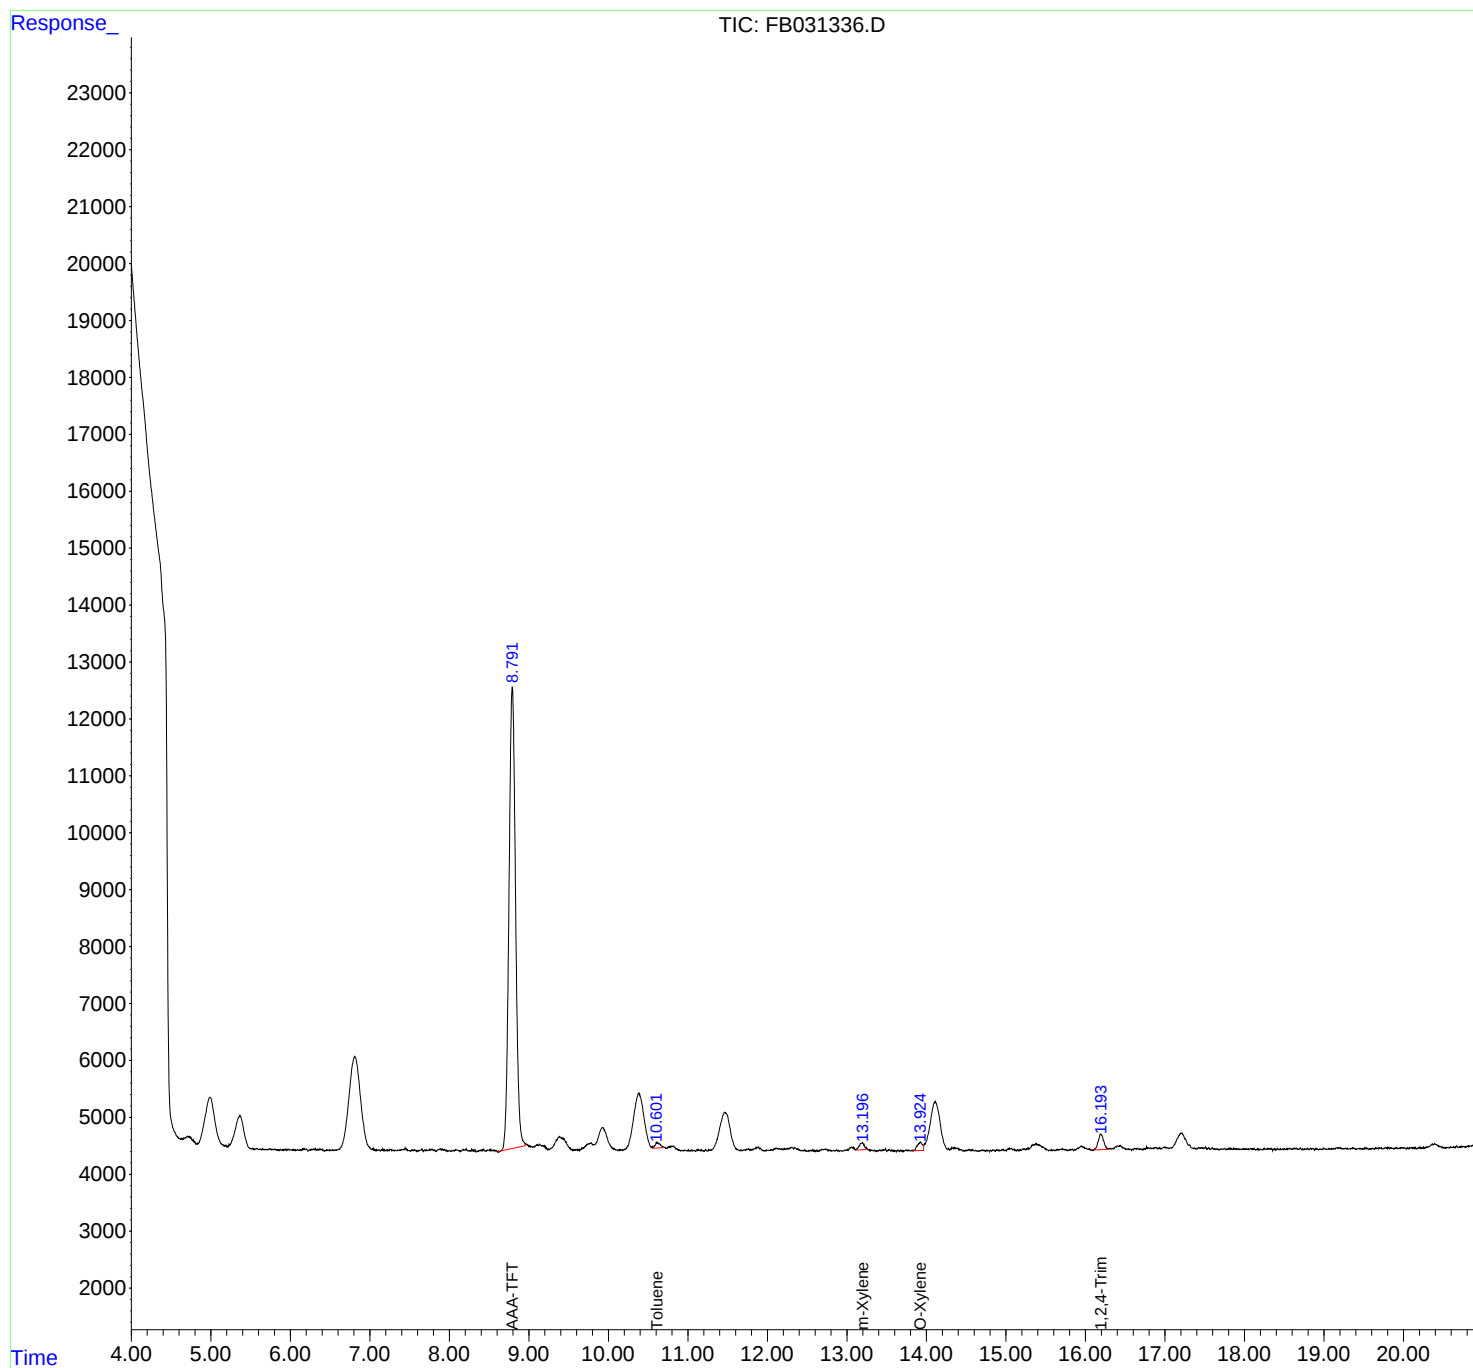


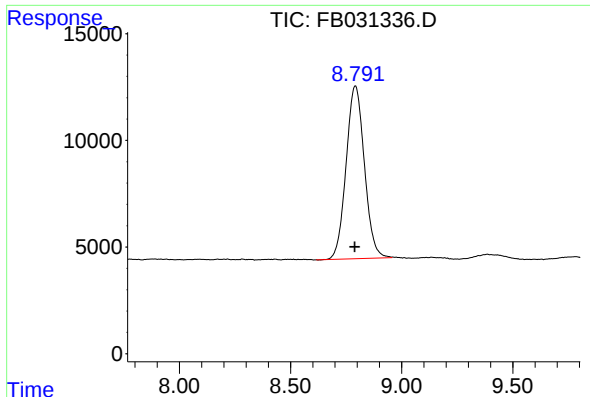

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.003 min
Response: 463344
Conc: 19.43 ng/ml

Instrument :
FID_B
ClientSampleId :

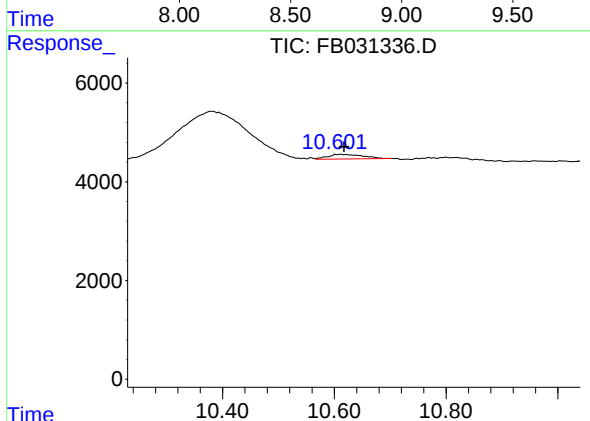


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.005 min
Response: 4063
Conc: 0.10 ng/ml

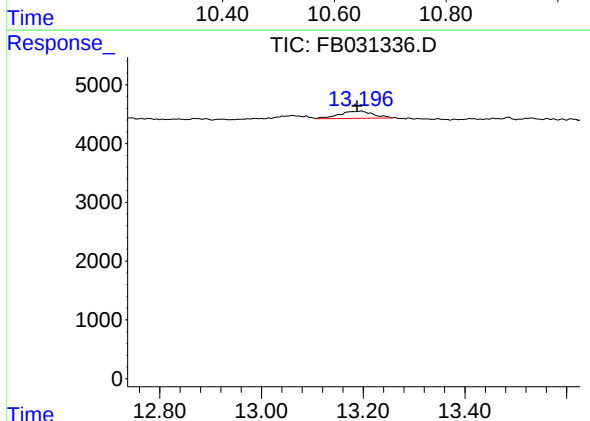


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: 0.010 min
Response: 5596
Conc: 0.15 ng/ml

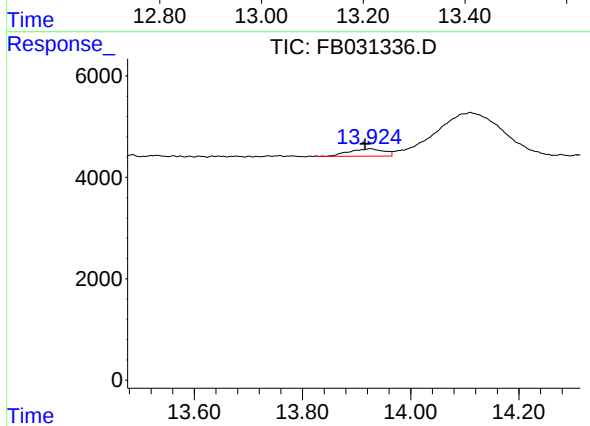

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.010 min
Response: 6531
Conc: 0.18 ng/ml

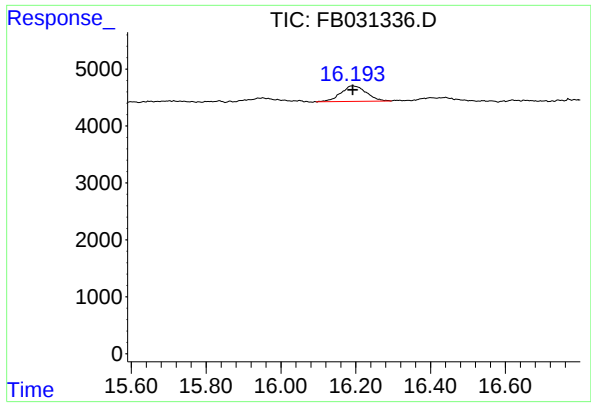

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.001 min
Response: 12795
Conc: 0.45 ng/ml

Instrument :
FID_B
ClientSampleId :