

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG012519\
Data File : FG003591.D
Signal(s) : FID1A.ch
Acq On : 25 Jan 2019 11:14
Operator : AJ\SJ
Sample : K1216-01 25X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 25 12:40:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.418	134141	0.912 ug/ml
12) N-OCTACOSANE	16.703	263892	1.859 ug/ml
13) N-TRIACONTANE	17.552	521846	3.704 ug/ml
14) N-DOTRIACONTANE	18.387	562283	4.157 ug/ml
15) N-TETRATRIACONTANE	19.174	316064	2.455 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG012519\
Data File : FG003591.D
Signal(s) : FID1A.ch
Acq On : 25 Jan 2019 11:14
Operator : AJ\SJ
Sample : K1216-01 25X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 25 12:40:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

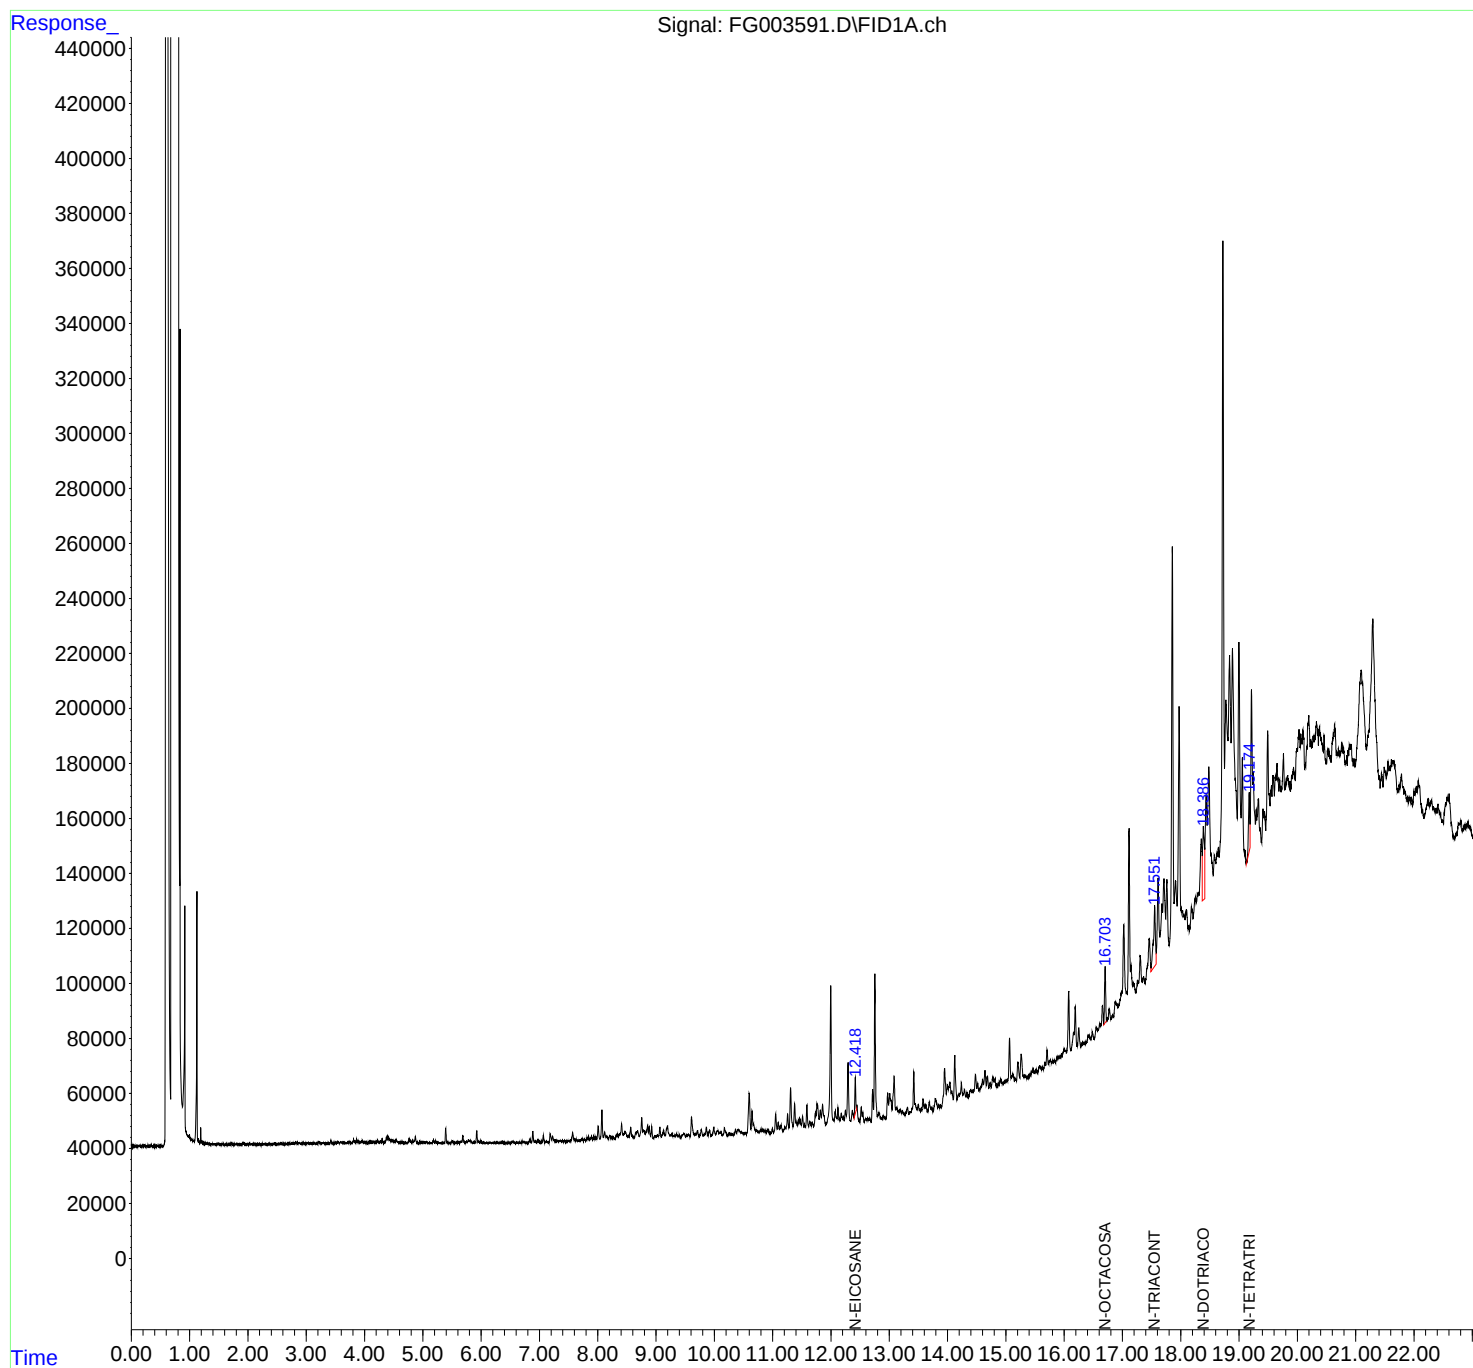

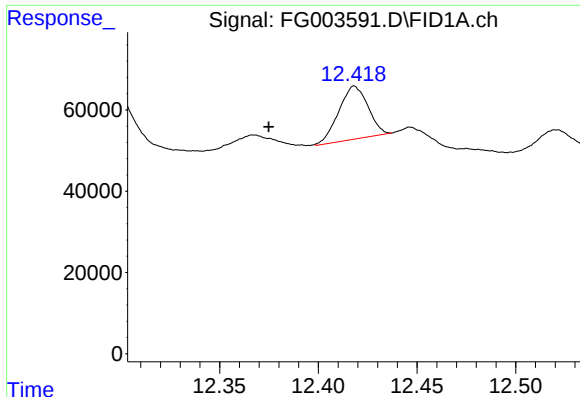


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: 0.044 min
Response: 134141
Conc: 0.91 ug/ml

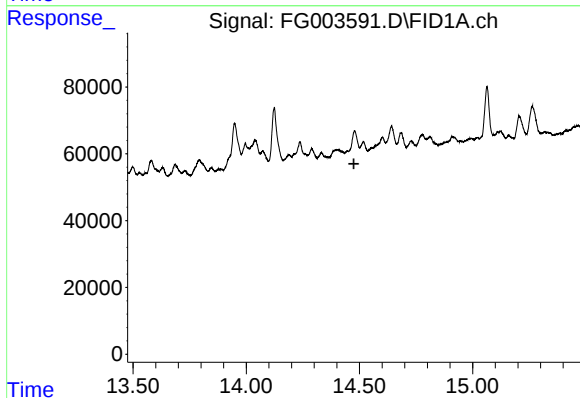


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.476 min
Response: 0
Conc: N.D.

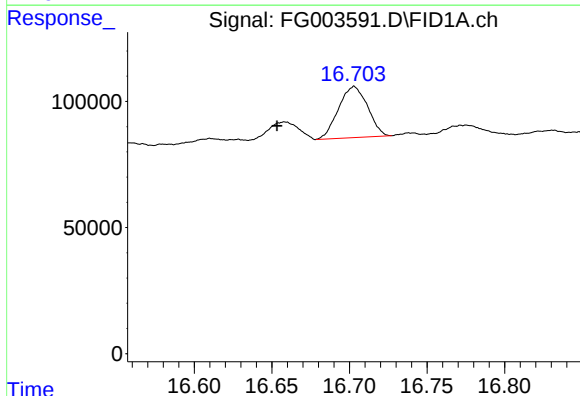


#12 N-OCTACOSANE

R.T.: 16.703 min
Delta R.T.: 0.050 min
Response: 263892
Conc: 1.86 ug/ml

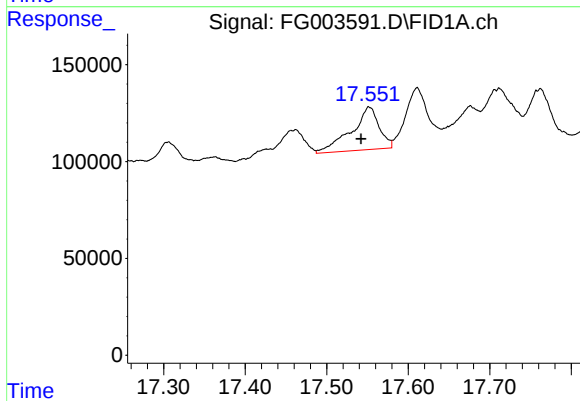


#13 N-TRIACONTANE

R.T.: 17.552 min
Delta R.T.: 0.010 min
Response: 521846
Conc: 3.70 ug/ml

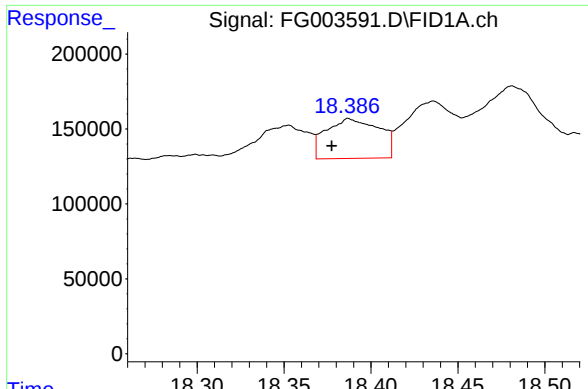

#14 N-DOTRIACONTANE

R.T.: 18.387 min
Delta R.T.: 0.010 min
Response: 562283
Conc: 4.16 ug/ml

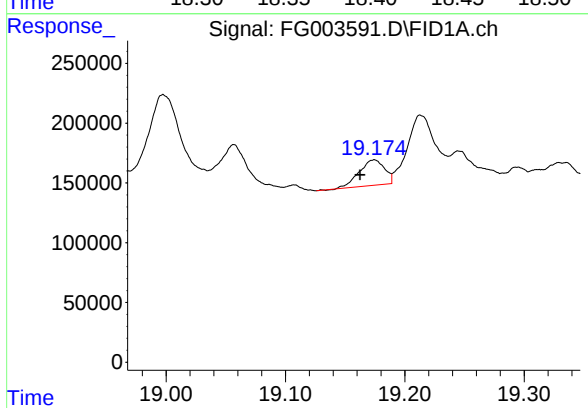

#15 N-TETRATRIACONTANE

R.T.: 19.174 min
Delta R.T.: 0.012 min
Response: 316064
Conc: 2.45 ug/ml