

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012621\
 Data File : FB025413.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jan 2021 12:13
 Operator : DD/AJ
 Sample : M1219-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 26 23:51:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	380903	16.932 ng/ml
Target Compounds			
4) t Benzene	7.898	40204	1.023 ng/ml
6) t Toluene	10.633	118801	3.165 ng/ml
7) t Ethylbenzene	13.075	29192	0.852 ng/ml
8) t m-Xylene	13.204	62791	1.835 ng/ml
9) t O-Xylene	13.937	35294	1.062 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012621\
Data File : FB025413.D
Signal(s) : FID2B.CH
Acq On : 26 Jan 2021 12:13
Operator : DD/AJ
Sample : M1219-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 26 23:51:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

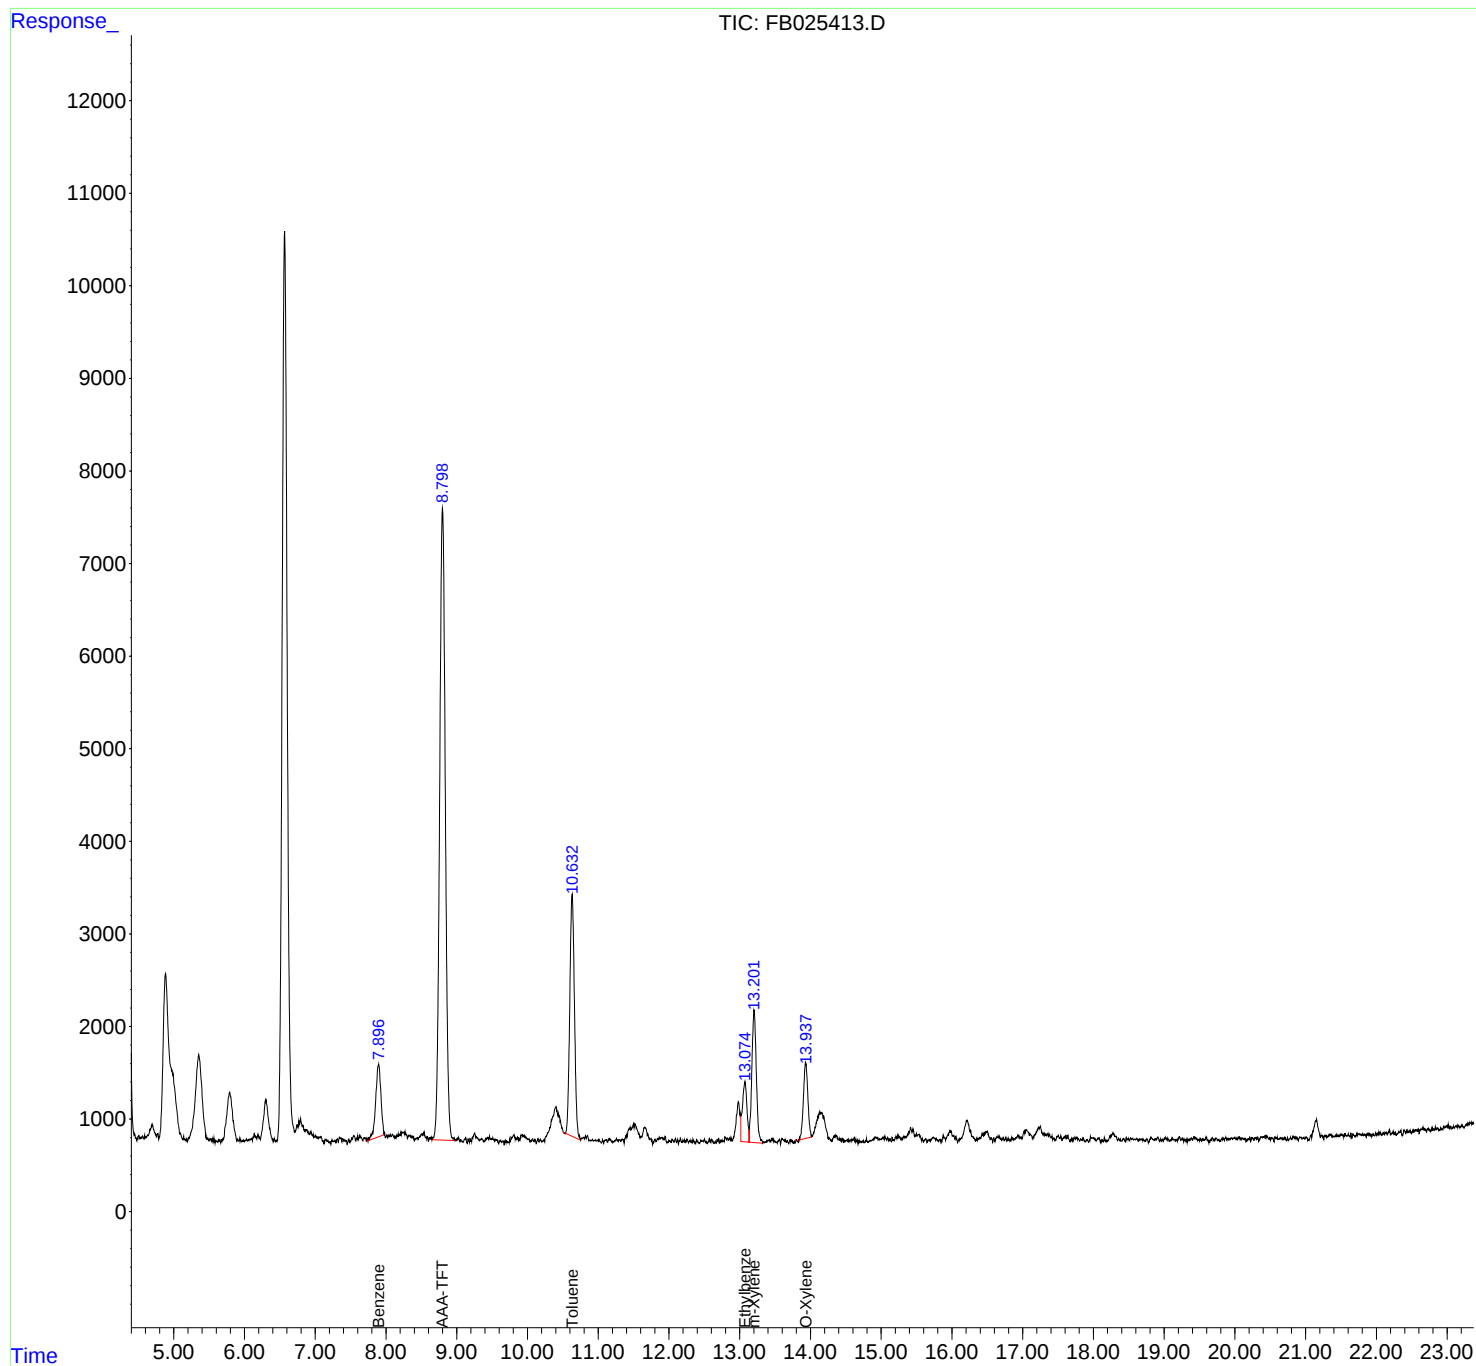


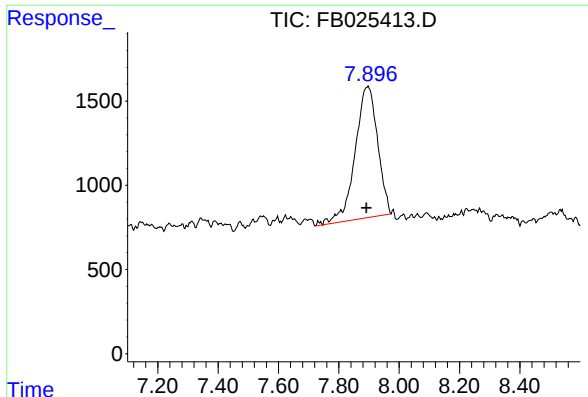

#4 Benzene


R.T.: 7.898 min
Delta R.T.: 0.006 min
Response: 40204
Conc: 1.02 ng/ml

Instrument :
FID_B
ClientSampleId :

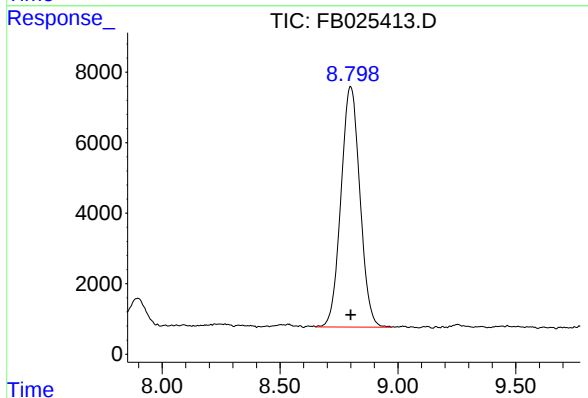


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 380903
Conc: 16.93 ng/ml

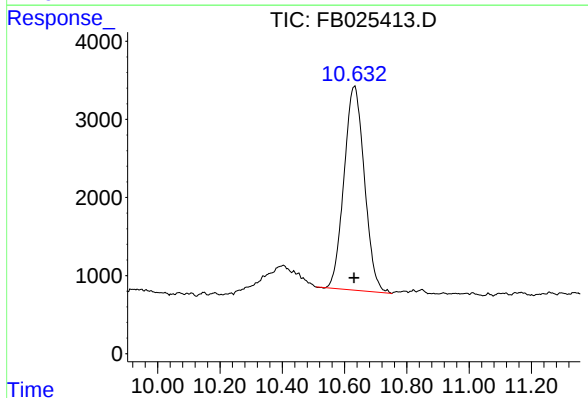


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 118801
Conc: 3.16 ng/ml

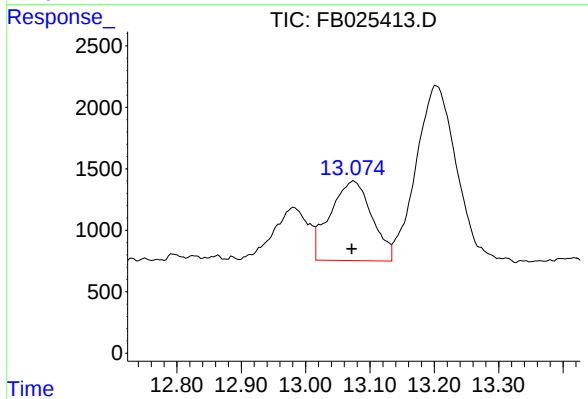

#7 Ethylbenzene


R.T.: 13.075 min
Delta R.T.: 0.004 min
Response: 29192
Conc: 0.85 ng/ml

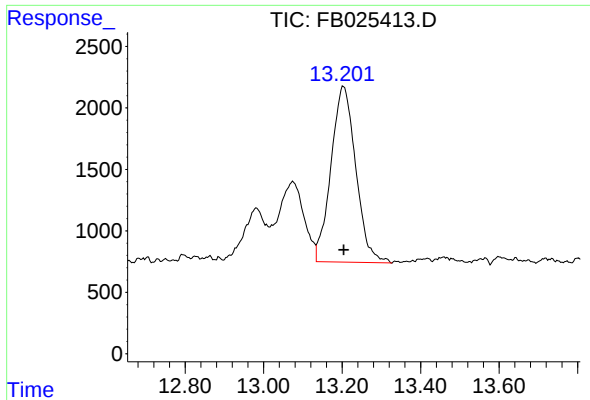

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 62791
Conc: 1.84 ng/ml

Instrument :
FID_B
ClientSampleId :

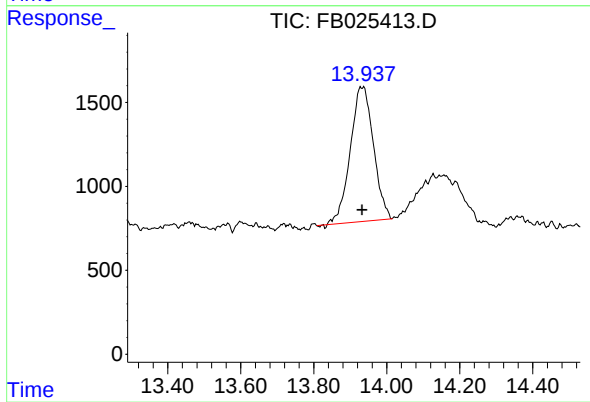

#9 o-Xylene

R.T.: 13.937 min
Delta R.T.: 0.005 min
Response: 35294
Conc: 1.06 ng/ml