

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012621\
 Data File : FB025408.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jan 2021 9:41
 Operator : DD/AJ
 Sample : BSF0126S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0126S1

Integration File: Calibration.e
 Quant Time: Jan 26 23:50:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	457848	20.353 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	903145	28.692 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	949552	29.951 ng/ml
3) t n-Heptane	7.757	310841	9.940 ng/ml
4) t Benzene	7.892	370537	9.425 ng/ml
6) t Toluene	10.630	1063599	28.333 ng/ml
7) t Ethylbenzene	13.070	330245	9.642 ng/ml
8) t m-Xylene	13.203	658338	19.242 ng/ml
9) t O-Xylene	13.931	635026	19.104 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	551320	19.172 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012621\
Data File : FB025408.D
Signal(s) : FID2B.CH
Acq On : 26 Jan 2021 9:41
Operator : DD/AJ
Sample : BSF0126S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0126S1

Integration File: Calibration.e
Quant Time: Jan 26 23:50:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

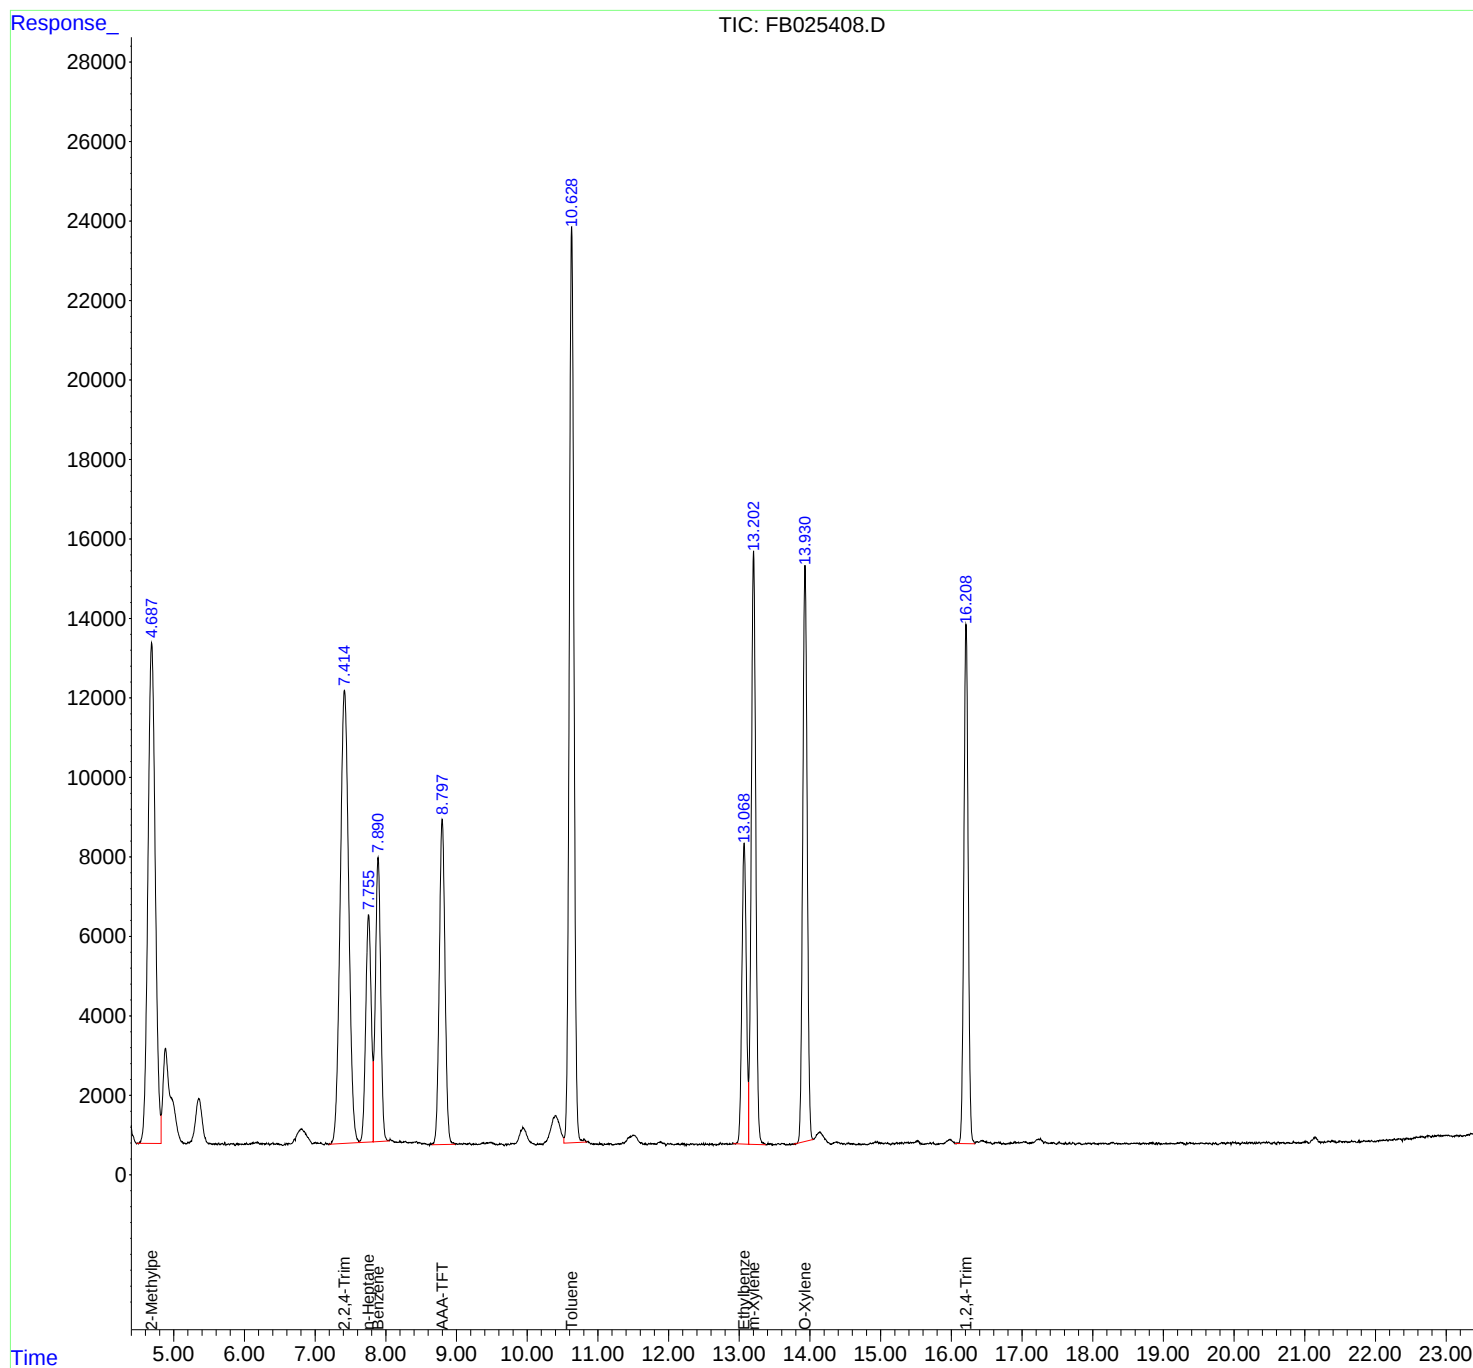


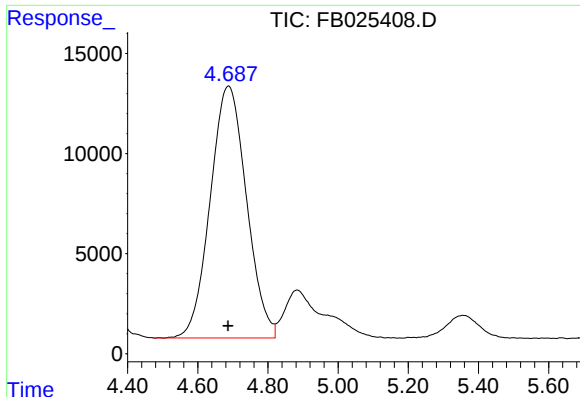

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.003 min
Response: 903145
Conc: 28.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0126S1

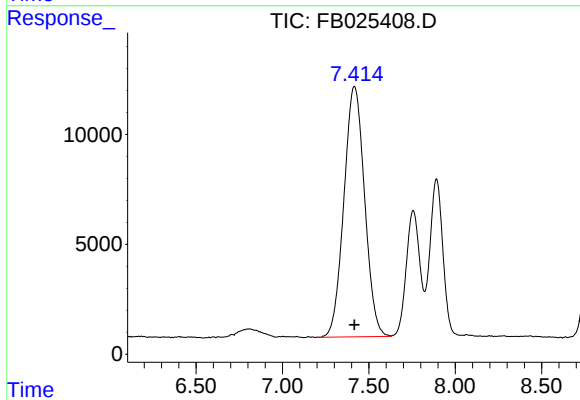


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 949552
Conc: 29.95 ng/ml

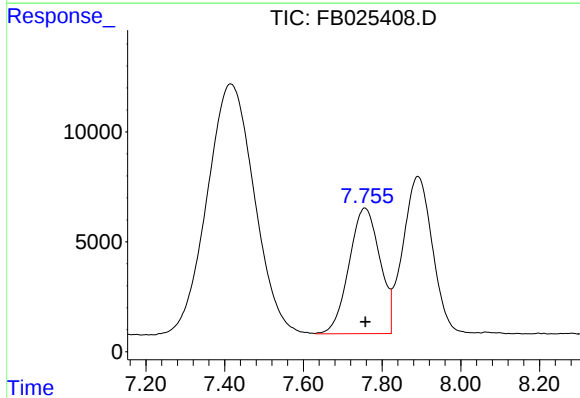


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 310841
Conc: 9.94 ng/ml

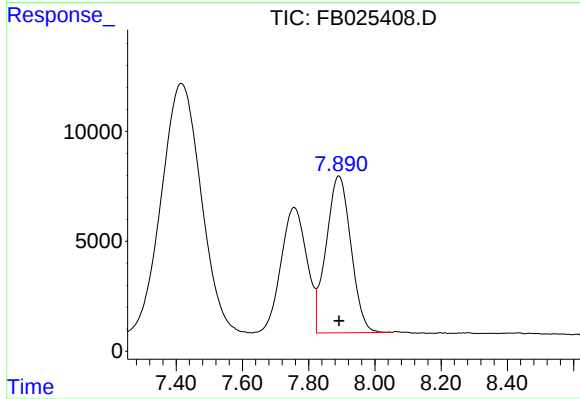

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 370537
Conc: 9.42 ng/ml

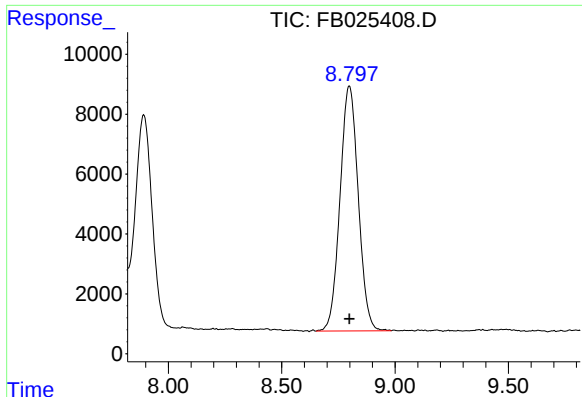

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.001 min
Response: 457848
Conc: 20.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0126S1

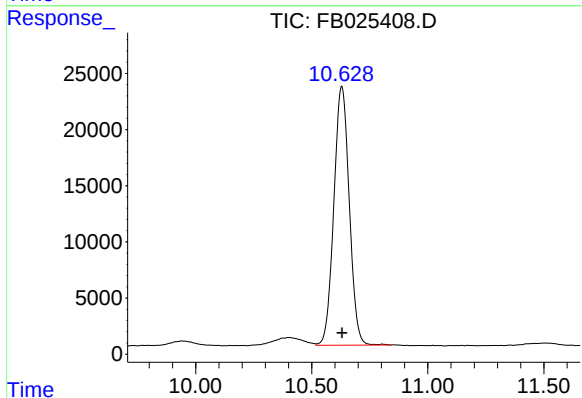


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 1063599
Conc: 28.33 ng/ml

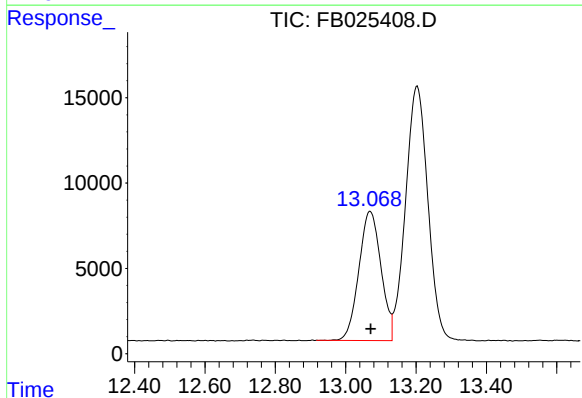


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.002 min
Response: 330245
Conc: 9.64 ng/ml

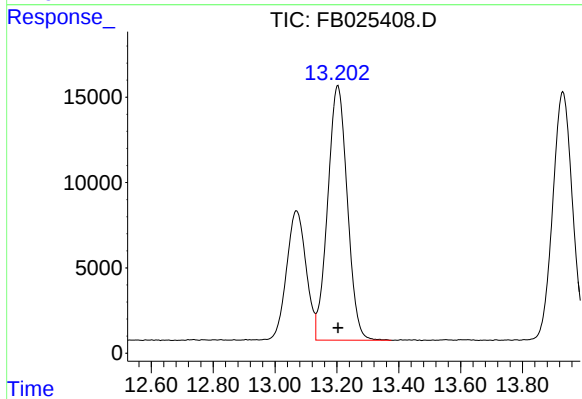

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 658338
Conc: 19.24 ng/ml

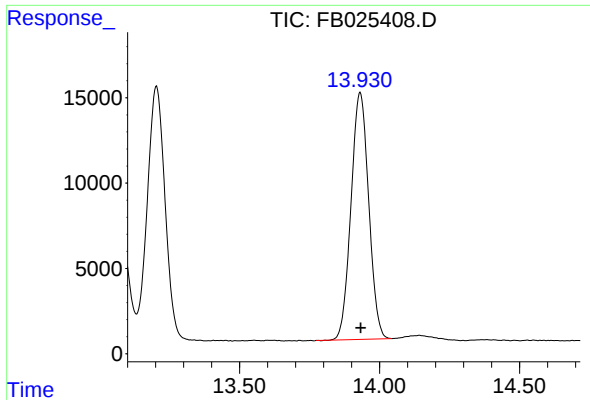

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.001 min
Response: 635026
Conc: 19.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0126S1

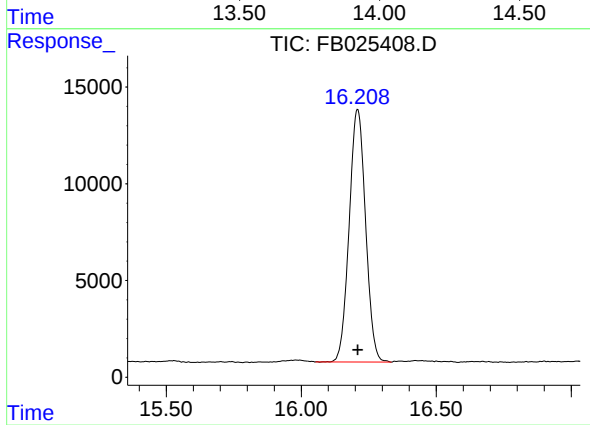

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 551320
Conc: 19.17 ng/ml