

Data Path : P:\HPCHEM1\FID B\Data\FB012718\  
Data File : FB013355.D  
Signal(s) : FID2B.CH  
Acq On : 27 Jan 2018 23:03  
Operator : MJ/SJ  
Sample : J1009-05  
Misc : 4.92g/5.00mL DI Water  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jan 28 08:56:13 2018  
Quant Method : P:\HPCHEM1\FID\_B\Method\FB012218.M  
Quant Title :  
QLast Update : Mon Jan 22 11:28:15 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 9.135  | 131069   | 17.182 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.985 | 9096     | 0.663 ng/ml  |
| 8) t m-Xylene                | 13.560 | 13725    | 0.757 ng/ml  |
| 9) t O-Xylene                | 14.303 | 10468    | 0.549 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.579 | 19446    | 0.986 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID B\Data\FB012718\  
Data File : FB013355.D  
Signal(s) : FID2B.CH  
Acq On : 27 Jan 2018 23:03  
Operator : MJ/SJ  
Sample : J1009-05  
Misc : 4.92g/5.00mL DI Water  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jan 28 08:56:13 2018  
Quant Method : P:\HPCHEM1\FID\_B\Method\FB012218.M  
Quant Title :  
QLast Update : Mon Jan 22 11:28:15 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60m x 0.53mm x 3.00um

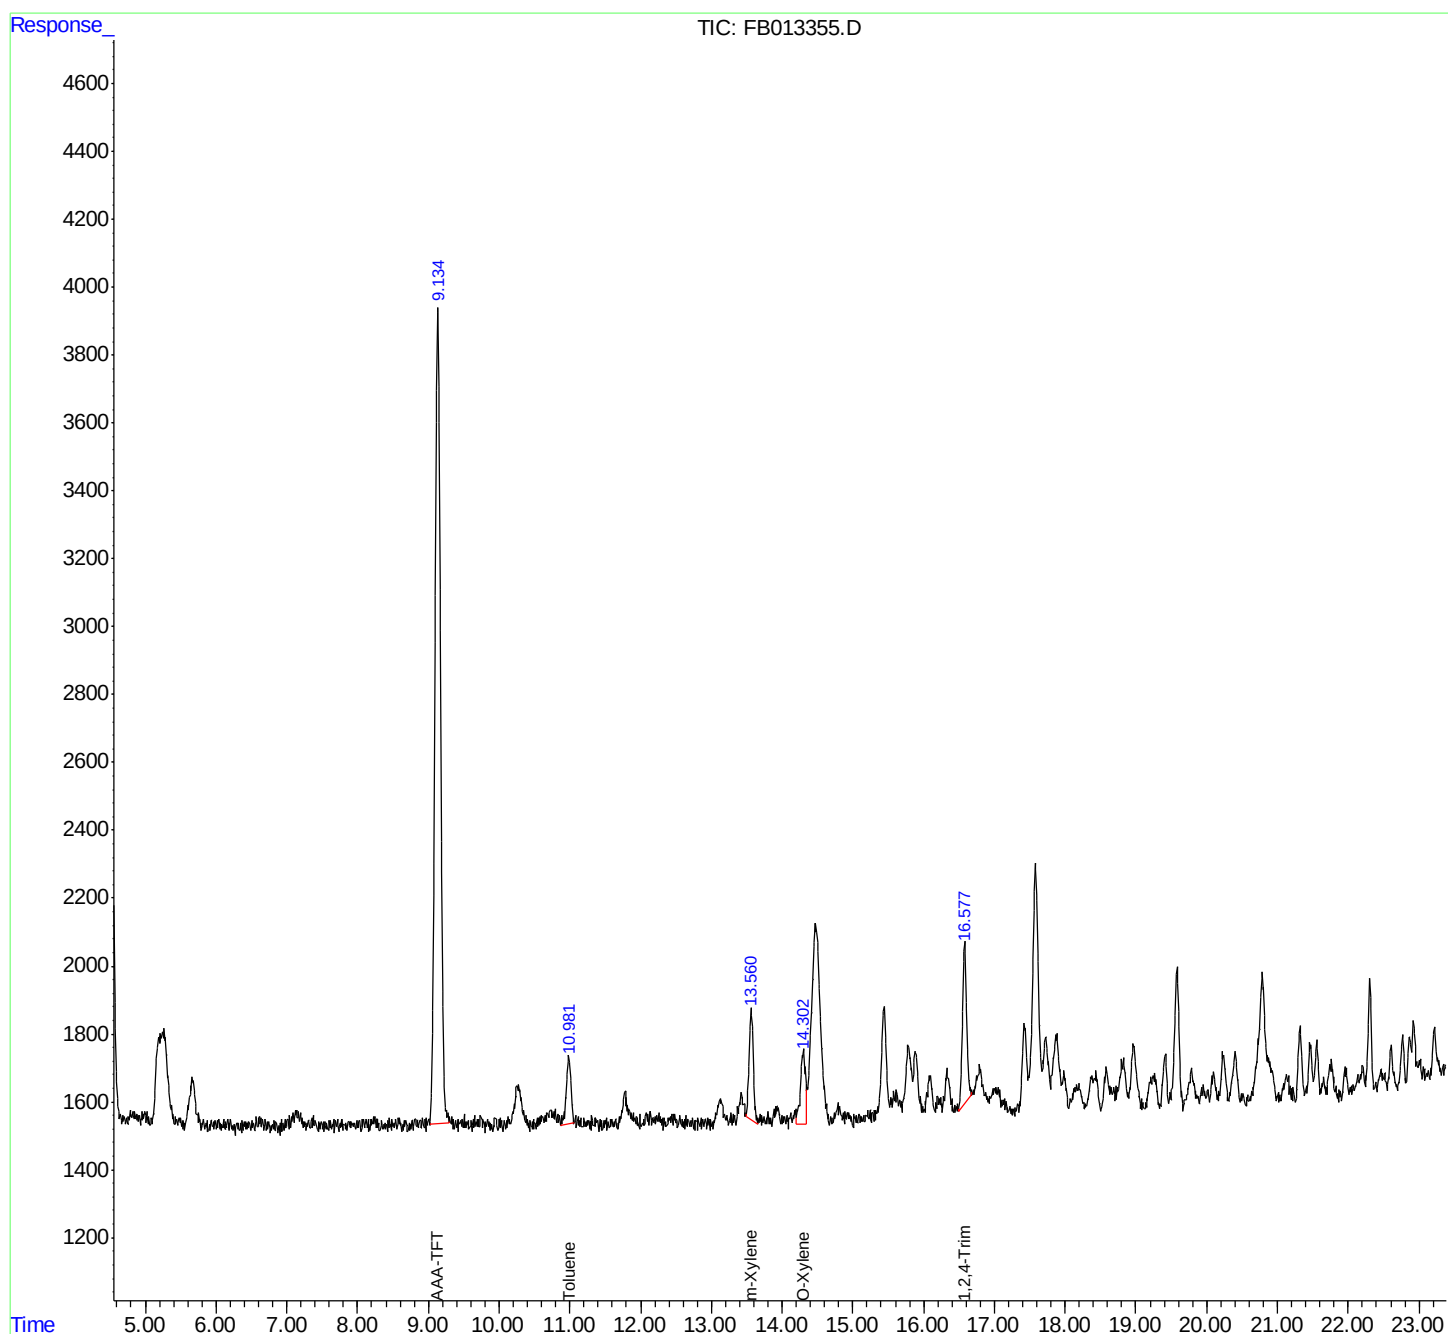


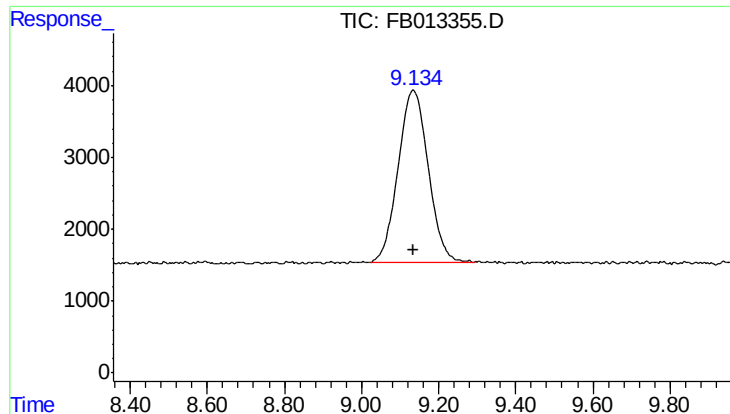

#5 AAA-TFT


R.T.: 9.135 min  
Delta R.T.: 0.001 min  
Response: 131069  
Conc: 17.18 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

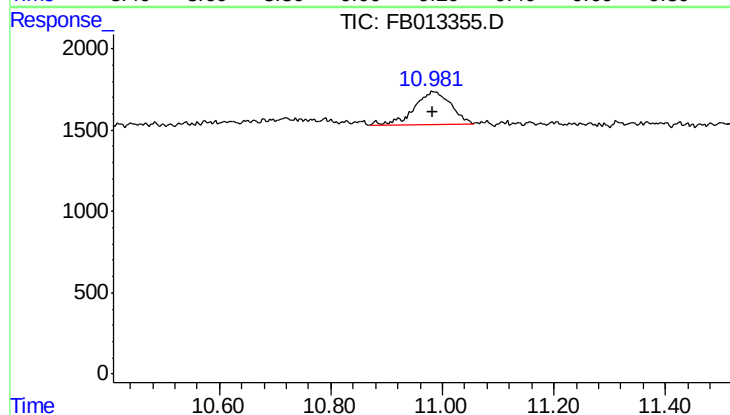


#6 Toluene

R.T.: 10.985 min  
Delta R.T.: 0.001 min  
Response: 9096  
Conc: 0.66 ng/ml

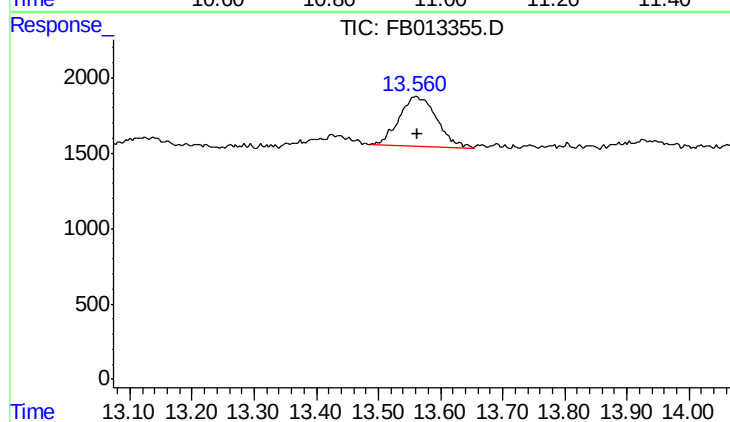


#8 m-Xylene

R.T.: 13.560 min  
Delta R.T.: -0.003 min  
Response: 13725  
Conc: 0.76 ng/ml

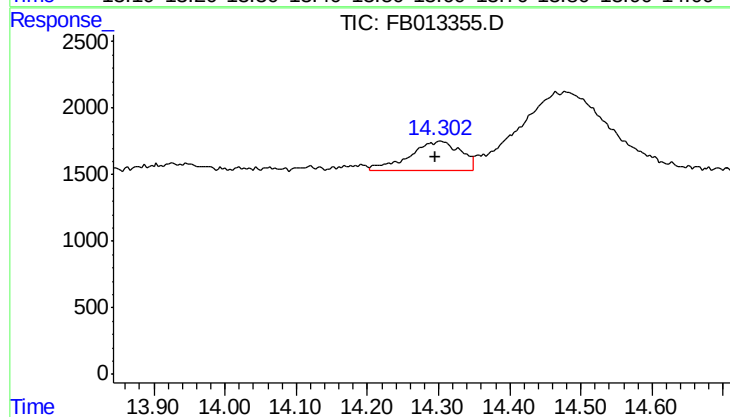

#9 O-Xylene

R.T.: 14.303 min  
Delta R.T.: 0.008 min  
Response: 10468  
Conc: 0.55 ng/ml

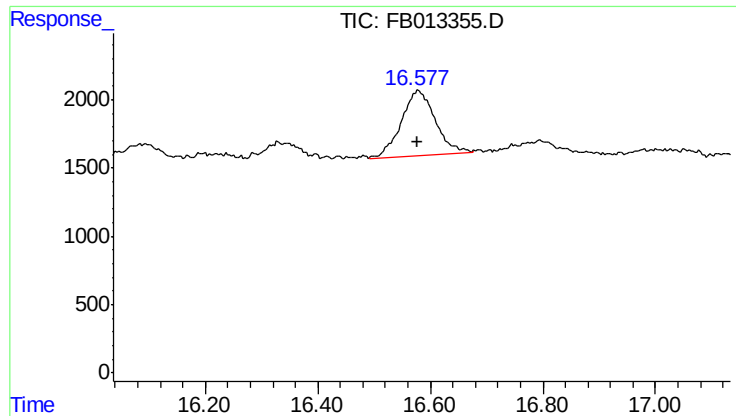

#10 1,2,4-Trimethylbenzene

R.T.: 16.579 min  
Delta R.T.: 0.002 min  
Response: 19446  
Conc: 0.99 ng/ml

Instrument :  
FID\_B  
ClientSampleId :