

Data Path : P:\HPCHEM1\FID B\Data\FB012718\
 Data File : FB013331.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2018 10:23
 Operator : MJ/SJ
 Sample : BSF0127S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0127S1

Integration File: Calibration.e
 Quant Time: Jan 28 08:52:32 2018
 Quant Method : P:\HPCHEM1\FID_B\Method\FB012218.M
 Quant Title :
 QLast Update : Mon Jan 22 11:28:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.132	152036	19.930 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.983	394001	30.684 ng/ml
2) t 2,2,4-Trimethylpentane	7.749	385354	31.420 ng/ml
3) t n-Heptane	8.087	118494	10.213 ng/ml
4) t Benzene	8.228	156568	10.397 ng/ml
6) t Toluene	10.981	425853	31.037 ng/ml
7) t Ethylbenzene	13.429	172486	10.256 ng/ml
8) t m-Xylene	13.562	372947	20.563 ng/ml
9) t O-Xylene	14.293	395567	20.746 ng/ml
10) t 1,2,4-Trimethylbenzene	16.576	416074	21.106 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID B\Data\FB012718\
Data File : FB013331.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2018 10:23
Operator : MJ/SJ
Sample : BSF0127S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleID :
BSF0127S1

Integration File: Calibration.e
Quant Time: Jan 28 08:52:32 2018
Quant Method : P:\HPCHEM1\FID_B\Method\FB012218.M
Quant Title :
QLast Update : Mon Jan 22 11:28:15 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60m x 0.53mm x 3.00um

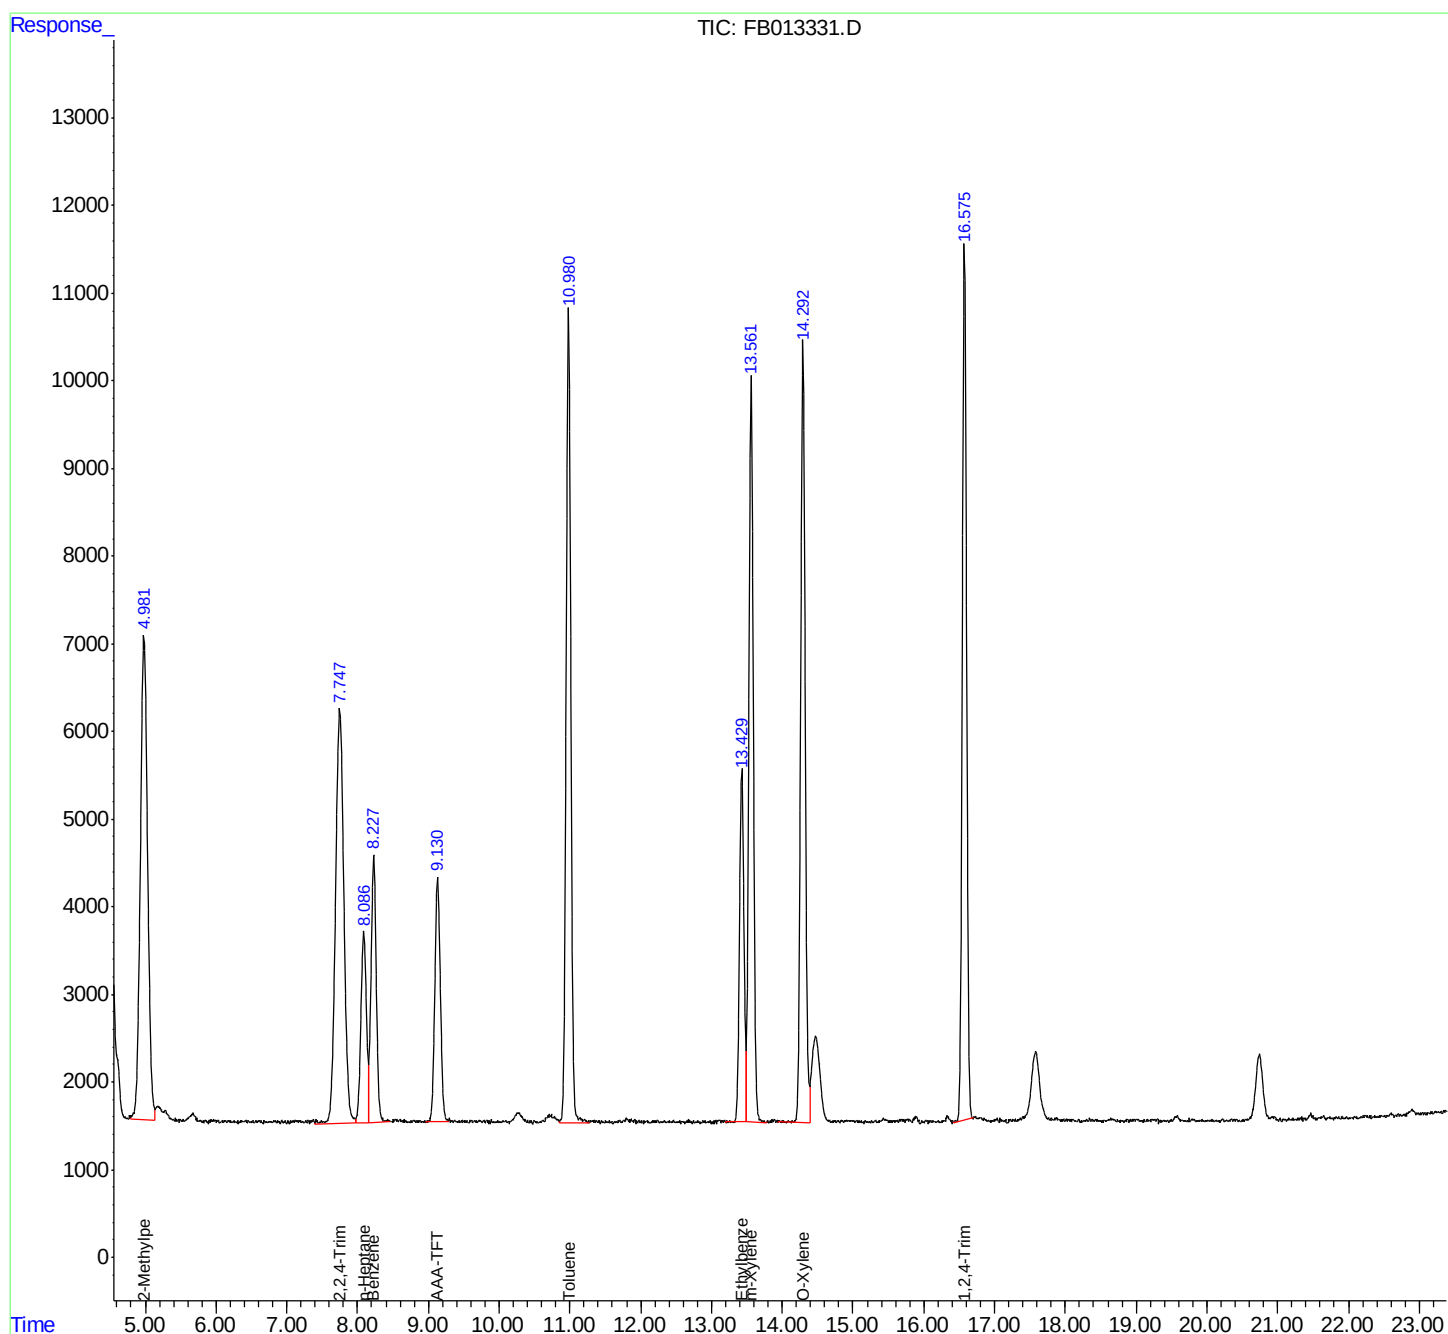


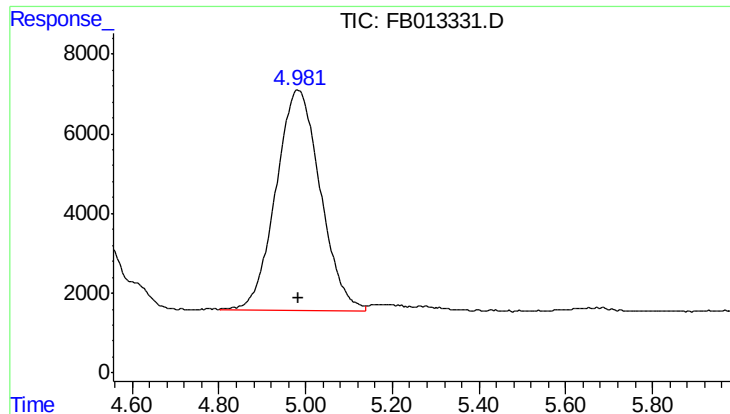

#1 2-Methylpentane


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 394001
Conc: 30.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S1

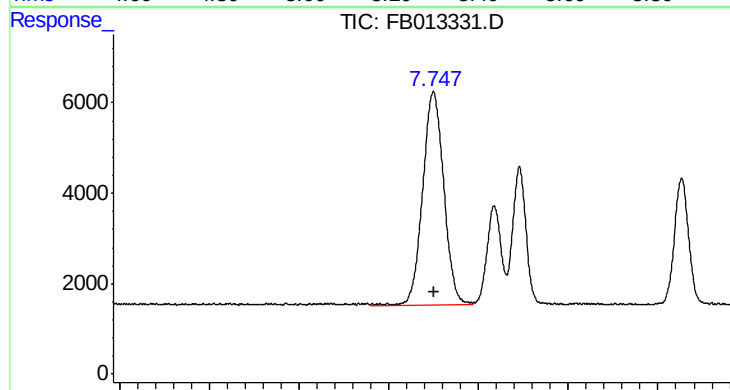


#2 2,2,4-Trimethylpentane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 385354
Conc: 31.42 ng/ml

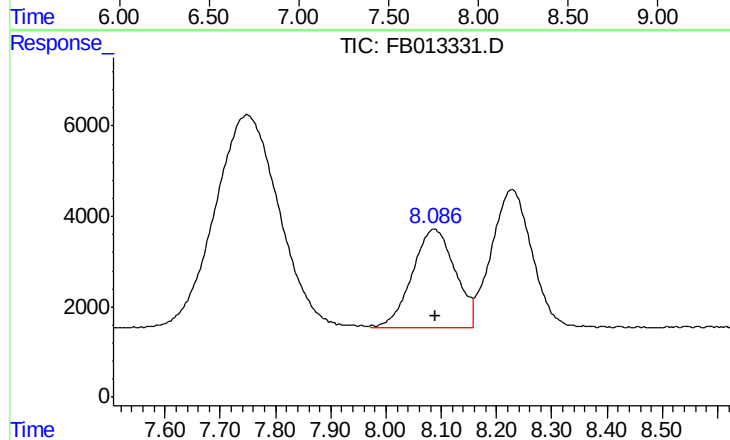


#3 n-Heptane

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 118494
Conc: 10.21 ng/ml

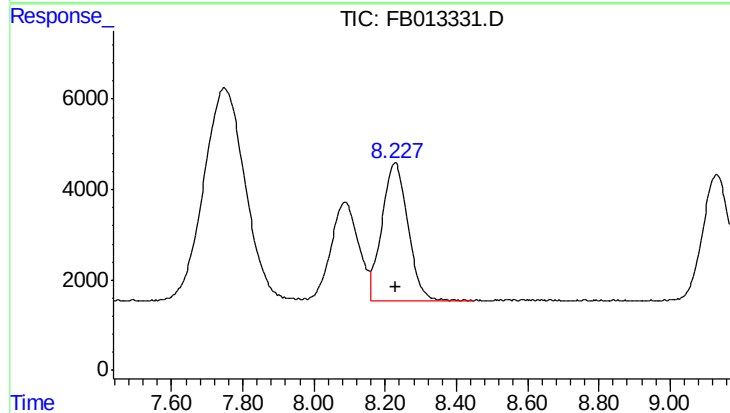

#4 Benzene


R.T.: 8.228 min
Delta R.T.: -0.002 min
Response: 156568
Conc: 10.40 ng/ml

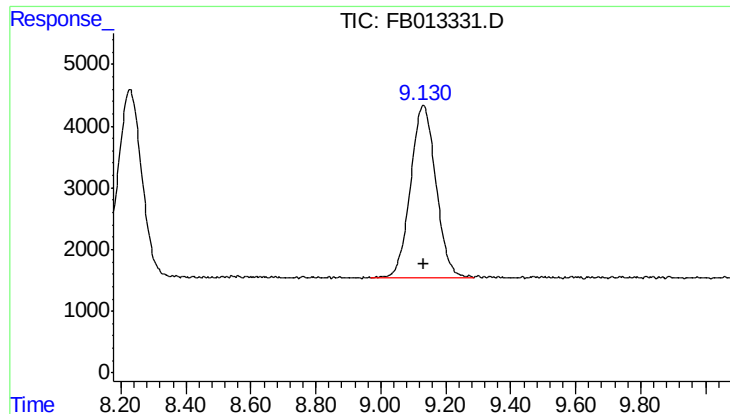

#5 AAA-TFT


R.T.: 9.132 min
Delta R.T.: -0.003 min
Response: 152036
Conc: 19.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S1

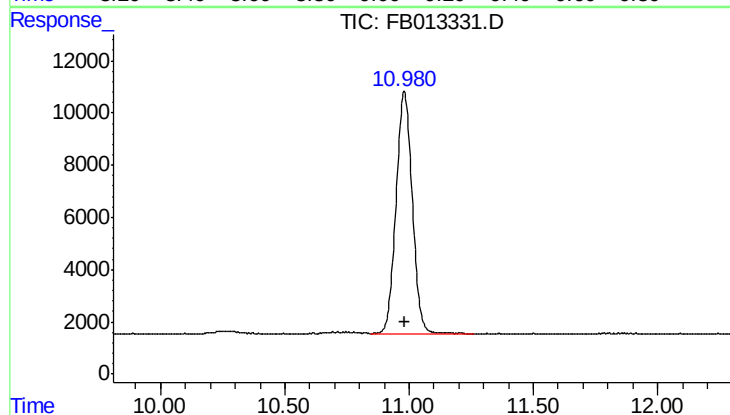


#6 Toluene

R.T.: 10.981 min
Delta R.T.: -0.002 min
Response: 425853
Conc: 31.04 ng/ml

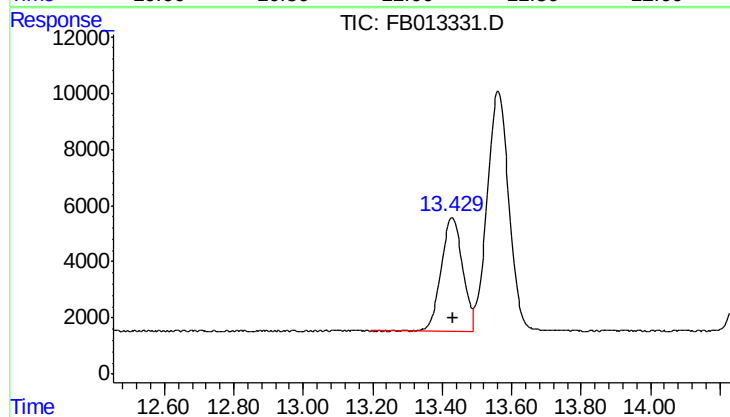


#7 Ethylbenzene

R.T.: 13.429 min
Delta R.T.: -0.002 min
Response: 172486
Conc: 10.26 ng/ml

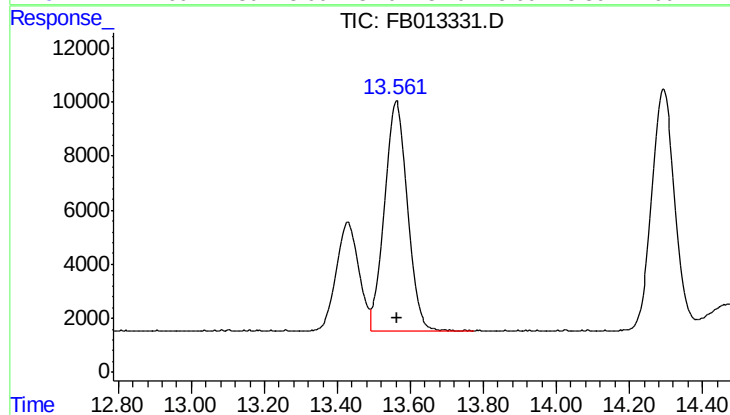

#8 m-Xylene


R.T.: 13.562 min
Delta R.T.: -0.002 min
Response: 372947
Conc: 20.56 ng/ml

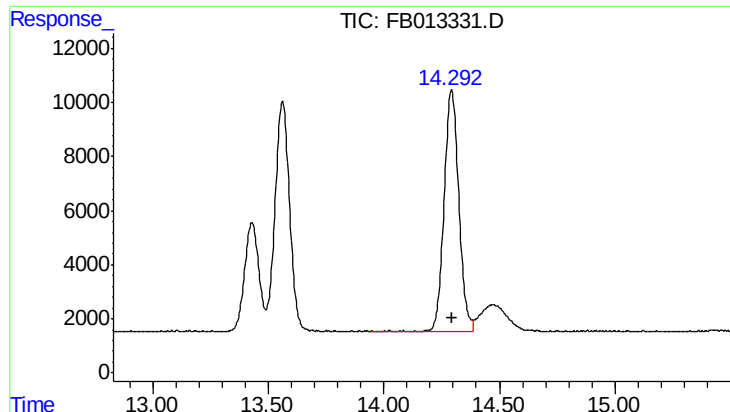

#9 O-Xylene

R.T.: 14.293 min
Delta R.T.: -0.002 min
Response: 395567
Conc: 20.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S1

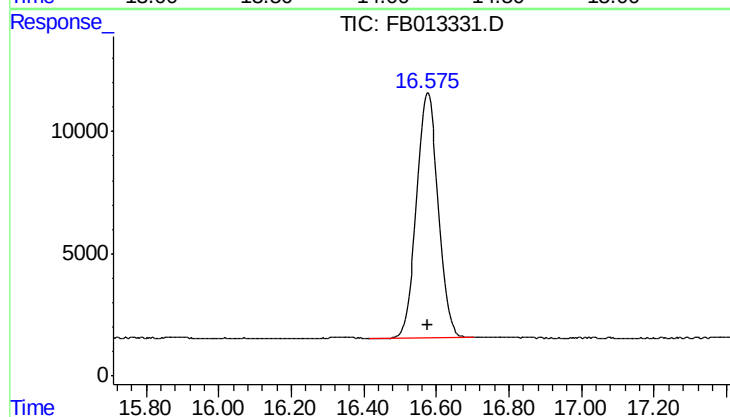

#10 1,2,4-Trimethylbenzene

R.T.: 16.576 min
Delta R.T.: 0.000 min
Response: 416074
Conc: 21.11 ng/ml