

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012720\
 Data File : FB023542.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2020 20:17
 Operator : DD/AJ
 Sample : L1161-09
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 28 01:22:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	50464	2.124 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	57170	1.809 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	56363	1.660 ng/ml
3) t n-Heptane	7.760	17533	0.524 ng/ml
4) t Benzene	7.893	21115	0.517 ng/ml
6) t Toluene	10.630	67467	1.707 ng/ml
7) t Ethylbenzene	13.073	21710	0.581 ng/ml
8) t m-Xylene	13.203	42652	1.199 ng/ml
9) t O-Xylene	13.931	43082	1.247 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	35044	1.198 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012720\
Data File : FB023542.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2020 20:17
Operator : DD/AJ
Sample : L1161-09
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 28 01:22:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

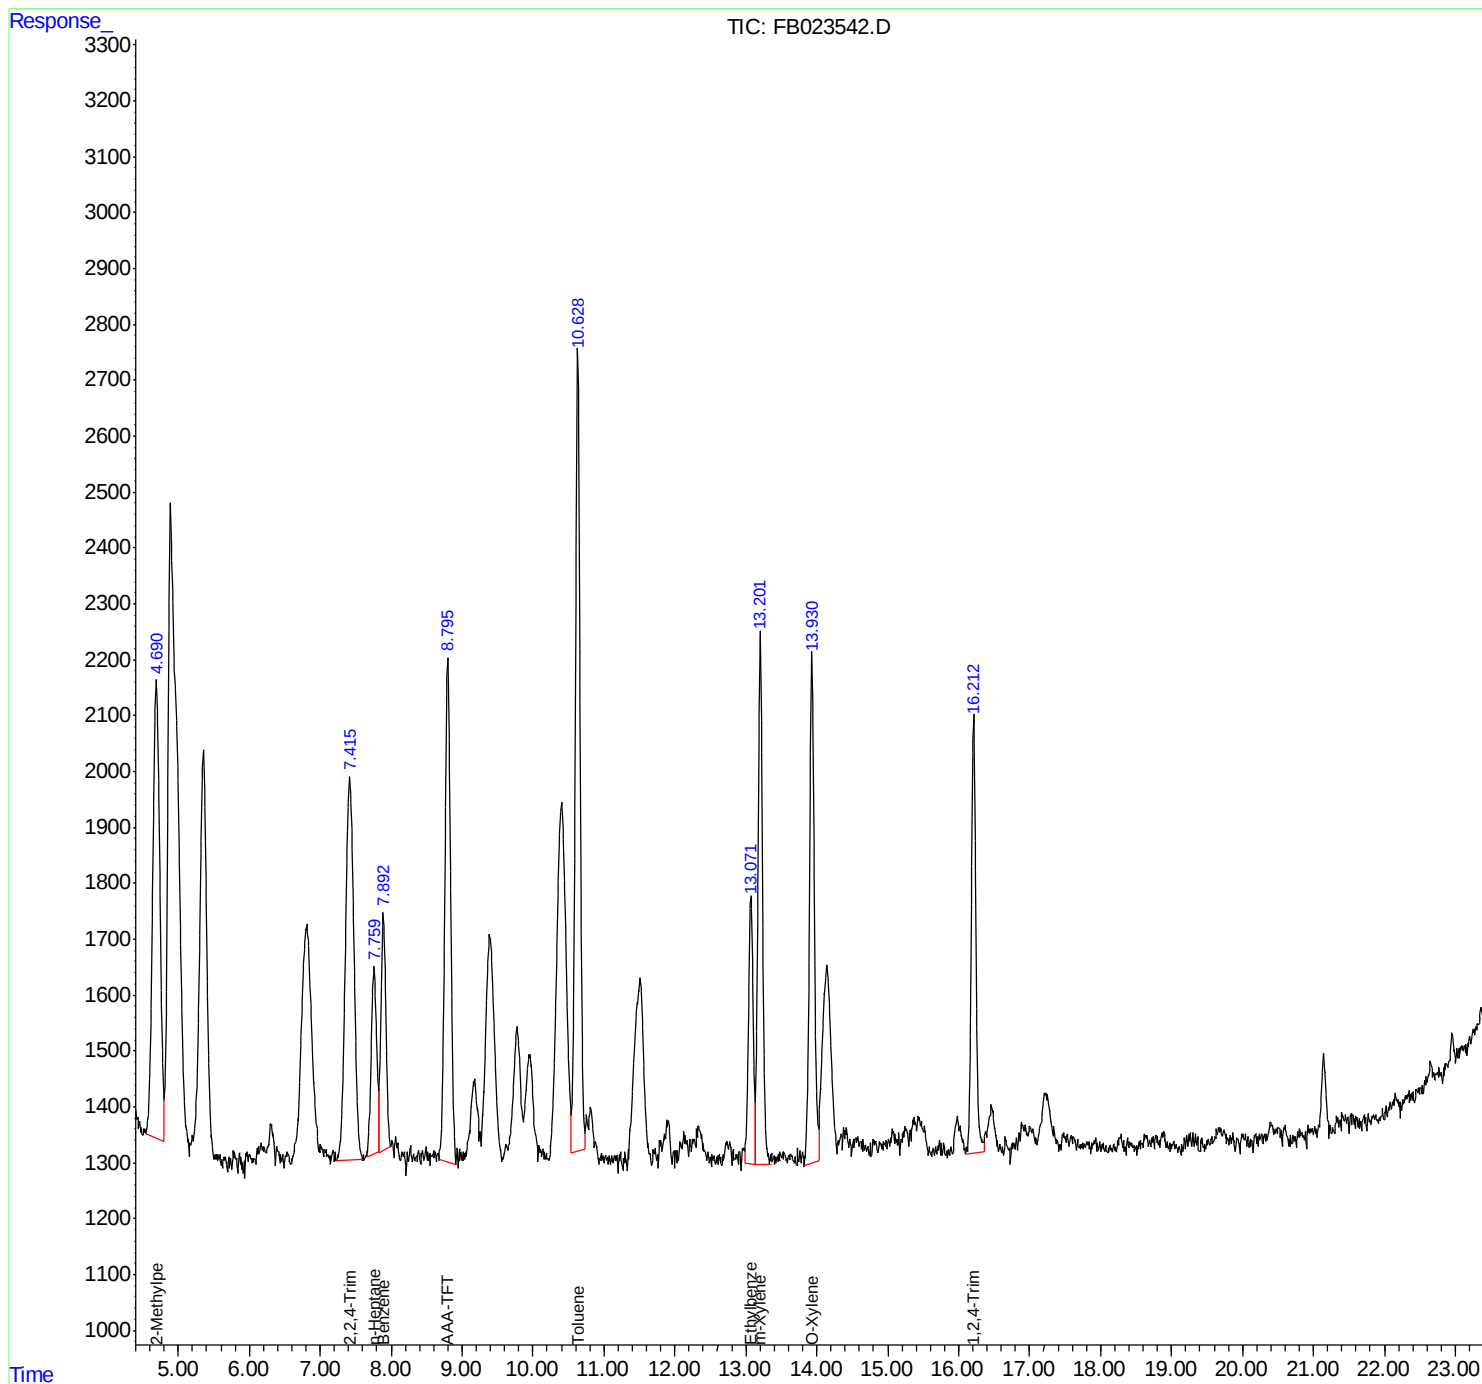

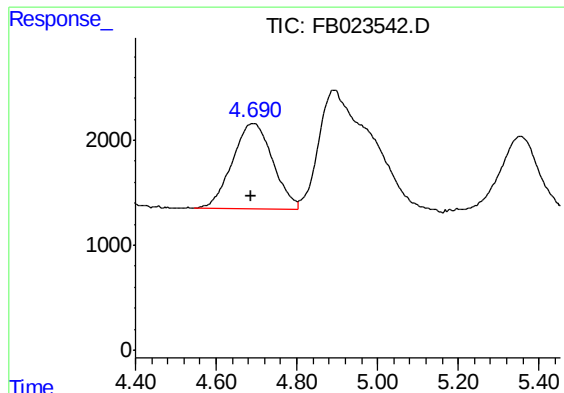


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.004 min
Response: 57170
Conc: 1.81 ng/ml

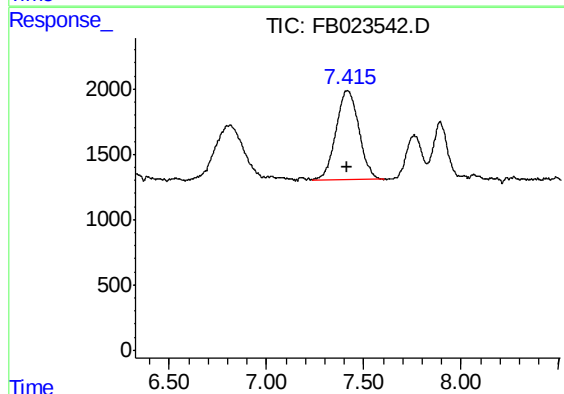


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 56363
Conc: 1.66 ng/ml

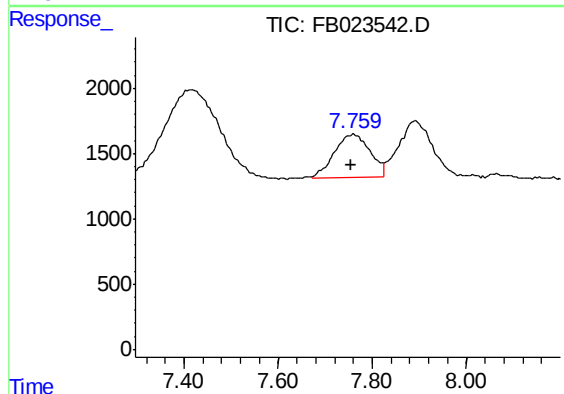


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.005 min
Response: 17533
Conc: 0.52 ng/ml

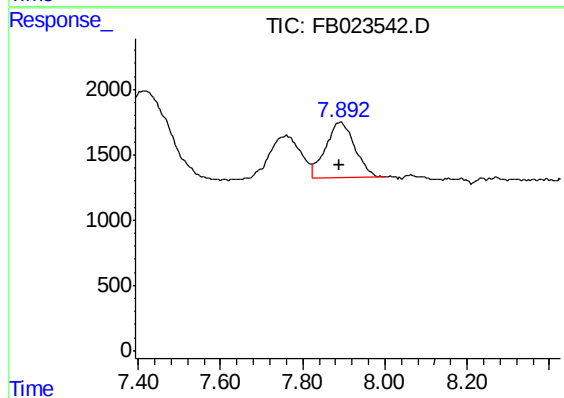


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.003 min
Response: 21115
Conc: 0.52 ng/ml

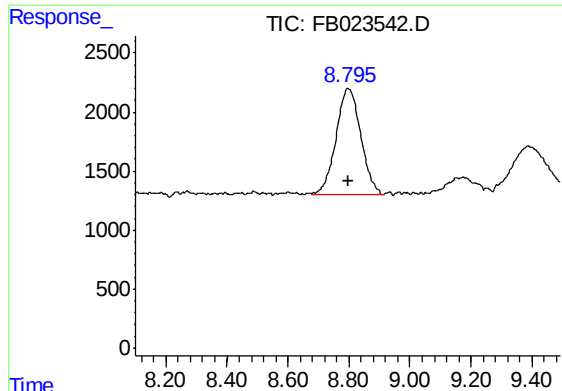


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 50464
Conc: 2.12 ng/ml

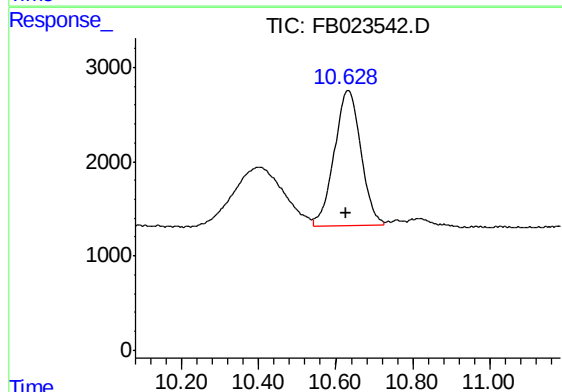


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.002 min
Response: 67467
Conc: 1.71 ng/ml

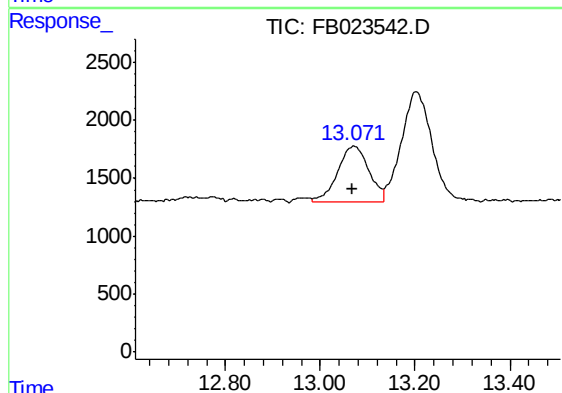


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.005 min
Response: 21710
Conc: 0.58 ng/ml

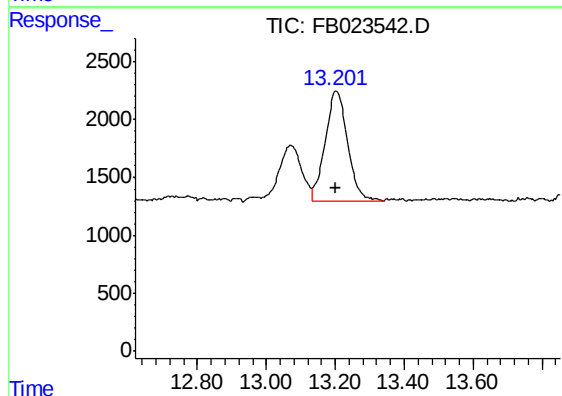


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.002 min
Response: 42652
Conc: 1.20 ng/ml

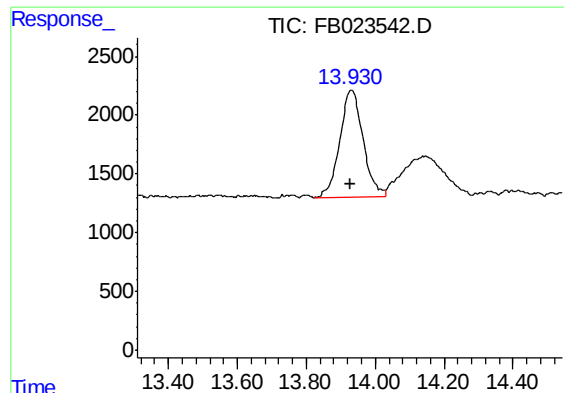

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.003 min
Response: 43082
Conc: 1.25 ng/ml

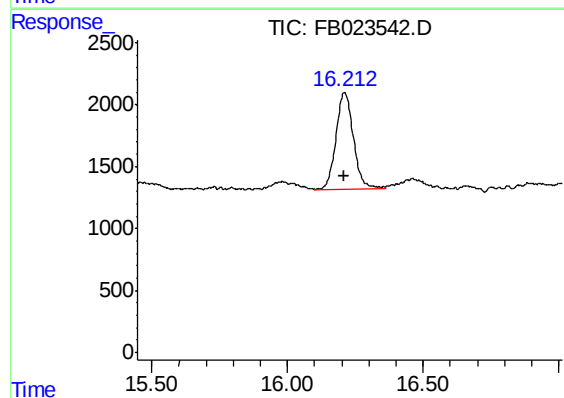

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.005 min
Response: 35044
Conc: 1.20 ng/ml