

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012720\
 Data File : FB023524.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2020 9:58
 Operator : DD/AJ
 Sample : BSF0127S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 28 01:19:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	508221	21.395 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	955197	30.227 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	1075296	31.670 ng/ml
3) t	n-Heptane	7.757	347788	10.386 ng/ml
4) t	Benzene	7.891	413781	10.132 ng/ml
6) t	Toluene	10.629	1222306	30.930 ng/ml
7) t	Ethylbenzene	13.070	382888	10.252 ng/ml
8) t	m-Xylene	13.202	733769	20.634 ng/ml
9) t	O-Xylene	13.931	709252	20.526 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	607148	20.764 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012720\
Data File : FB023524.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2020 9:58
Operator : DD/AJ
Sample : BSF0127S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 28 01:19:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

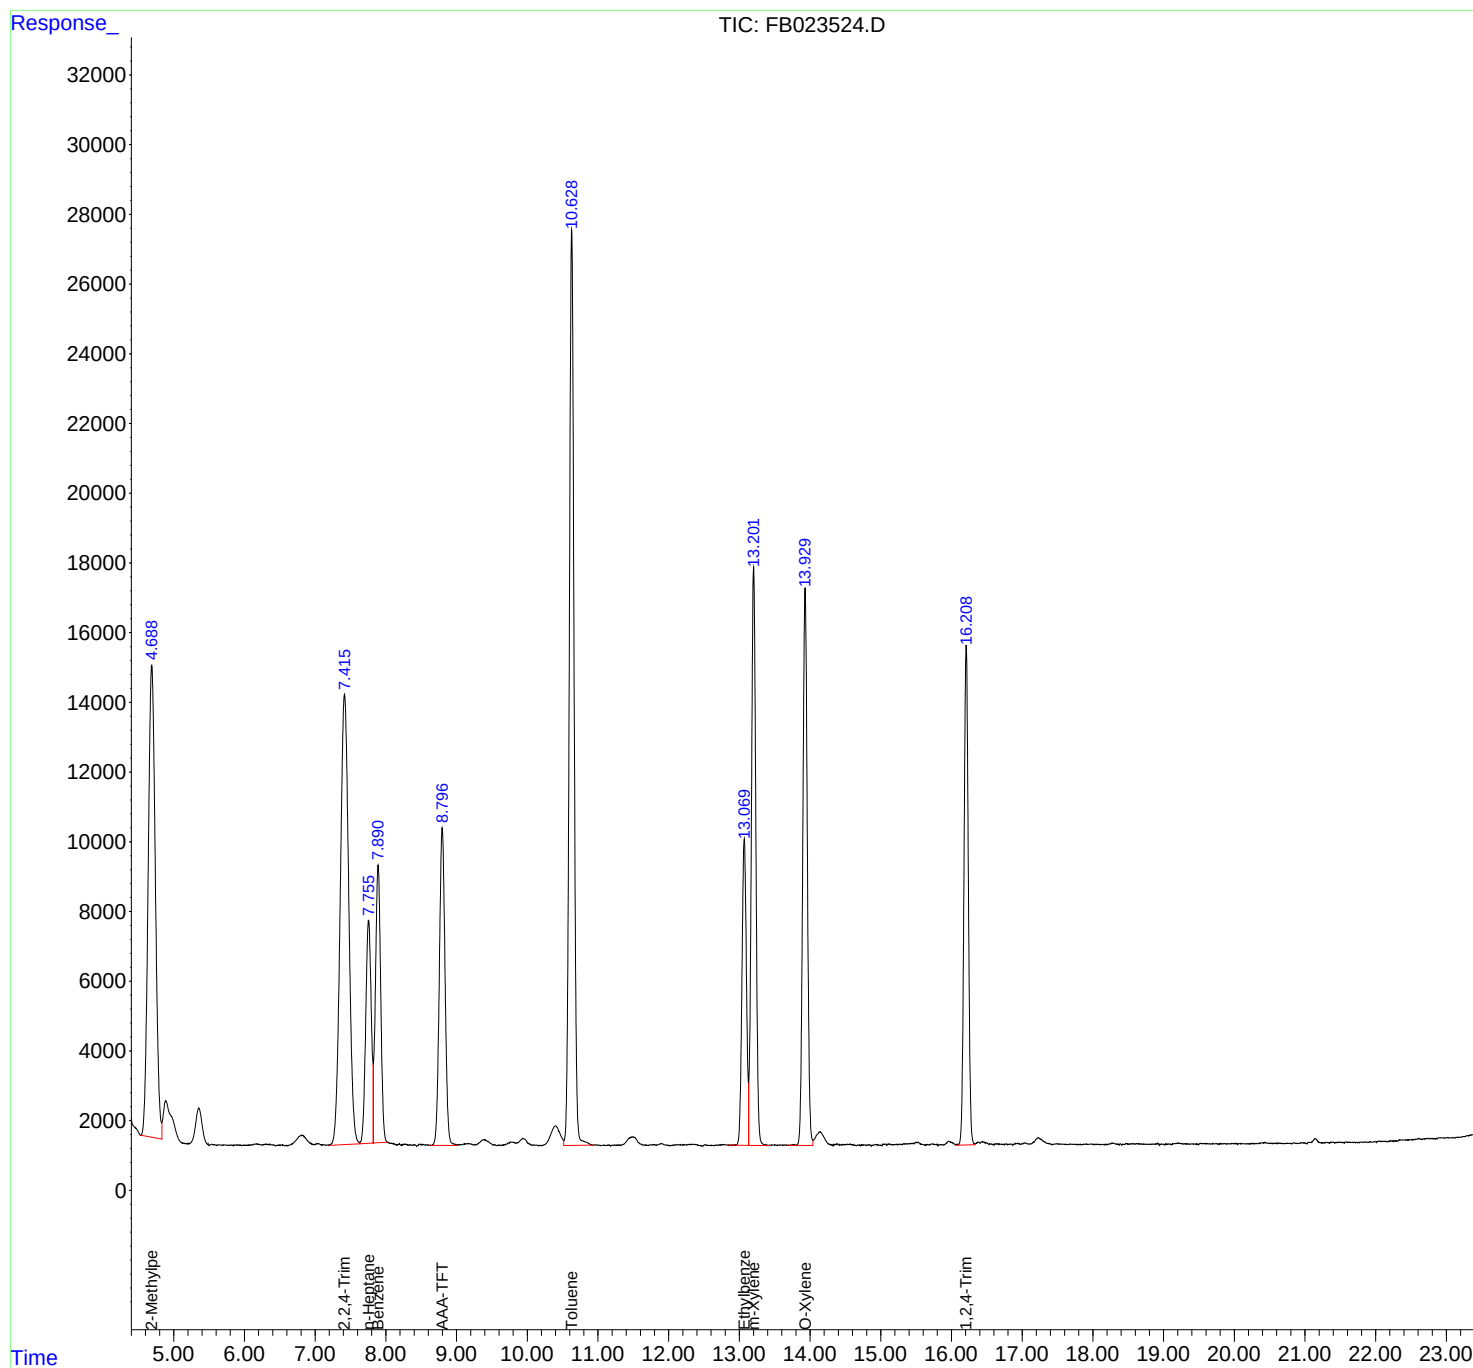

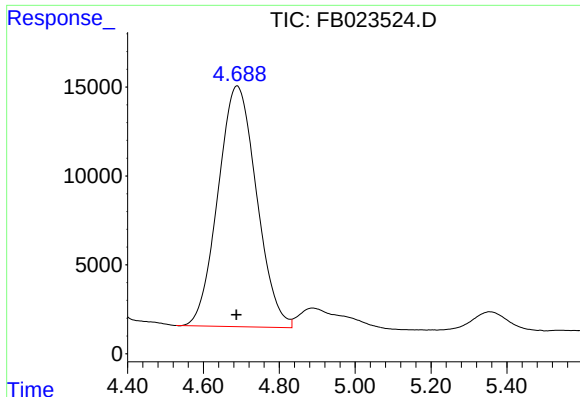


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 955197
Conc: 30.23 ng/ml

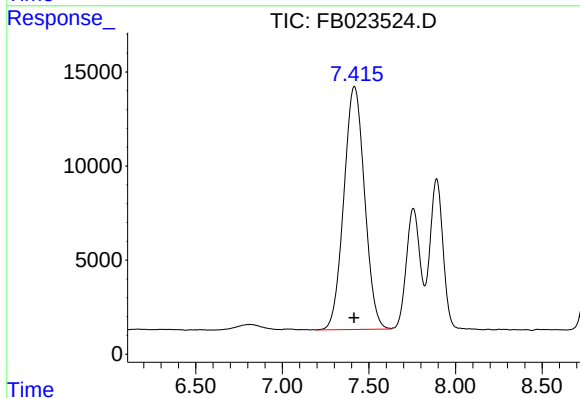


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 1075296
Conc: 31.67 ng/ml

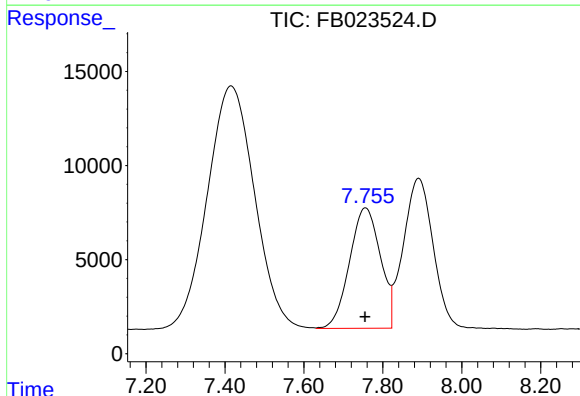


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.001 min
Response: 347788
Conc: 10.39 ng/ml

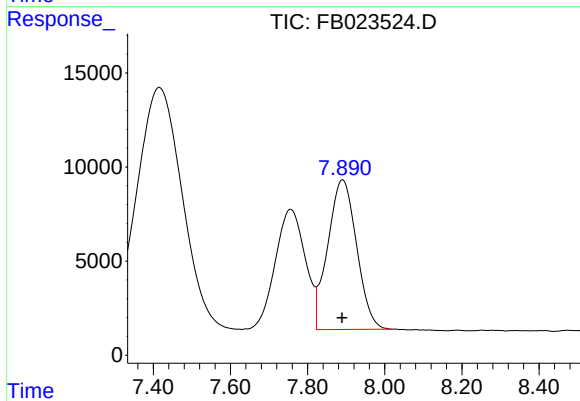


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.002 min
Response: 413781
Conc: 10.13 ng/ml

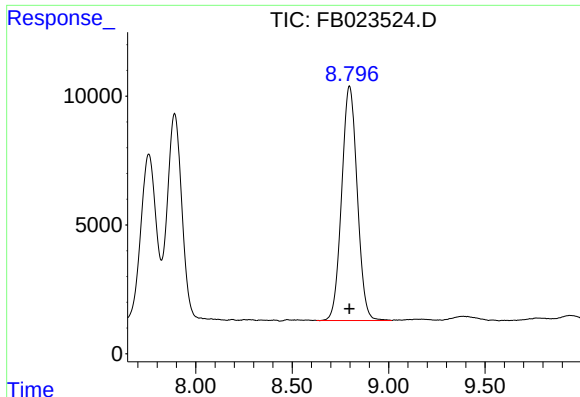


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 508221
Conc: 21.40 ng/ml

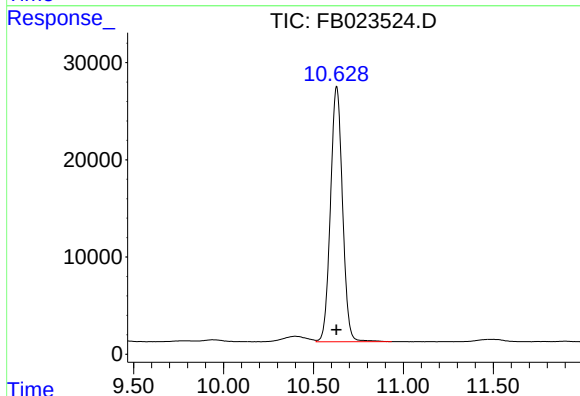


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.002 min
Response: 1222306
Conc: 30.93 ng/ml

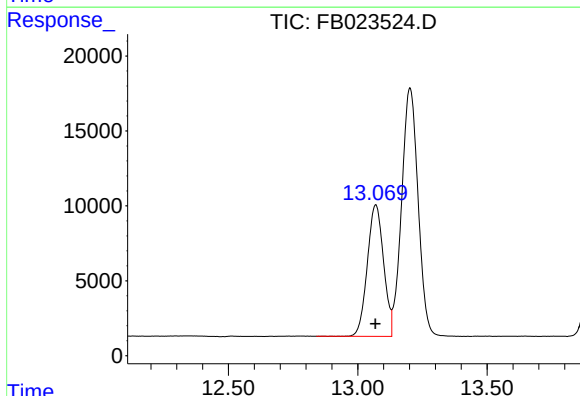


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.002 min
Response: 382888
Conc: 10.25 ng/ml

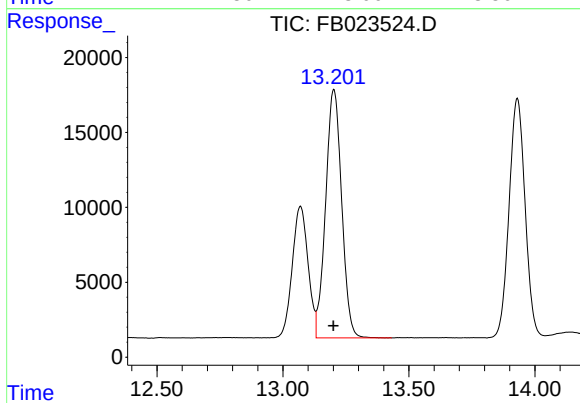


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.002 min
Response: 733769
Conc: 20.63 ng/ml

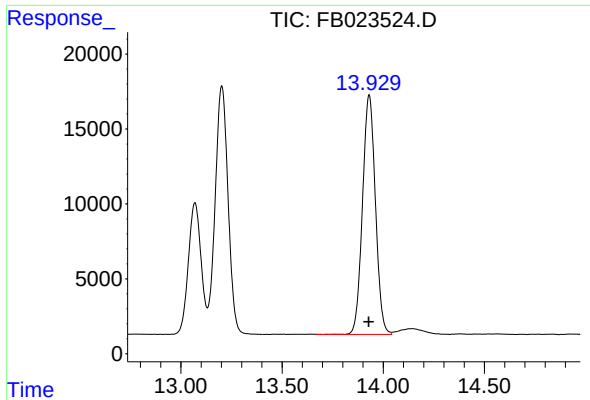

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.002 min
Response: 709252
Conc: 20.53 ng/ml

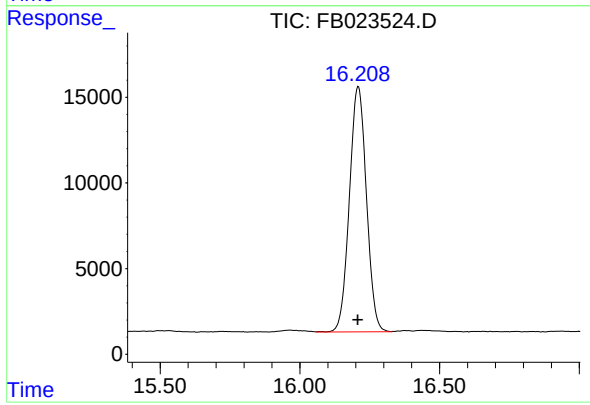

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.002 min
Response: 607148
Conc: 20.76 ng/ml