

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012721\
Data File : FB025419.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2021 11:57
Operator : DD/AJ
Sample : M1213-01
Misc : 3.88g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 28 00:22:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	483500	21.493 ng/ml
Target Compounds			
6) t Toluene	10.628	20437	0.544 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012721\
Data File : FB025419.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2021 11:57
Operator : DD/AJ
Sample : M1213-01
Misc : 3.88g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 28 00:22:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

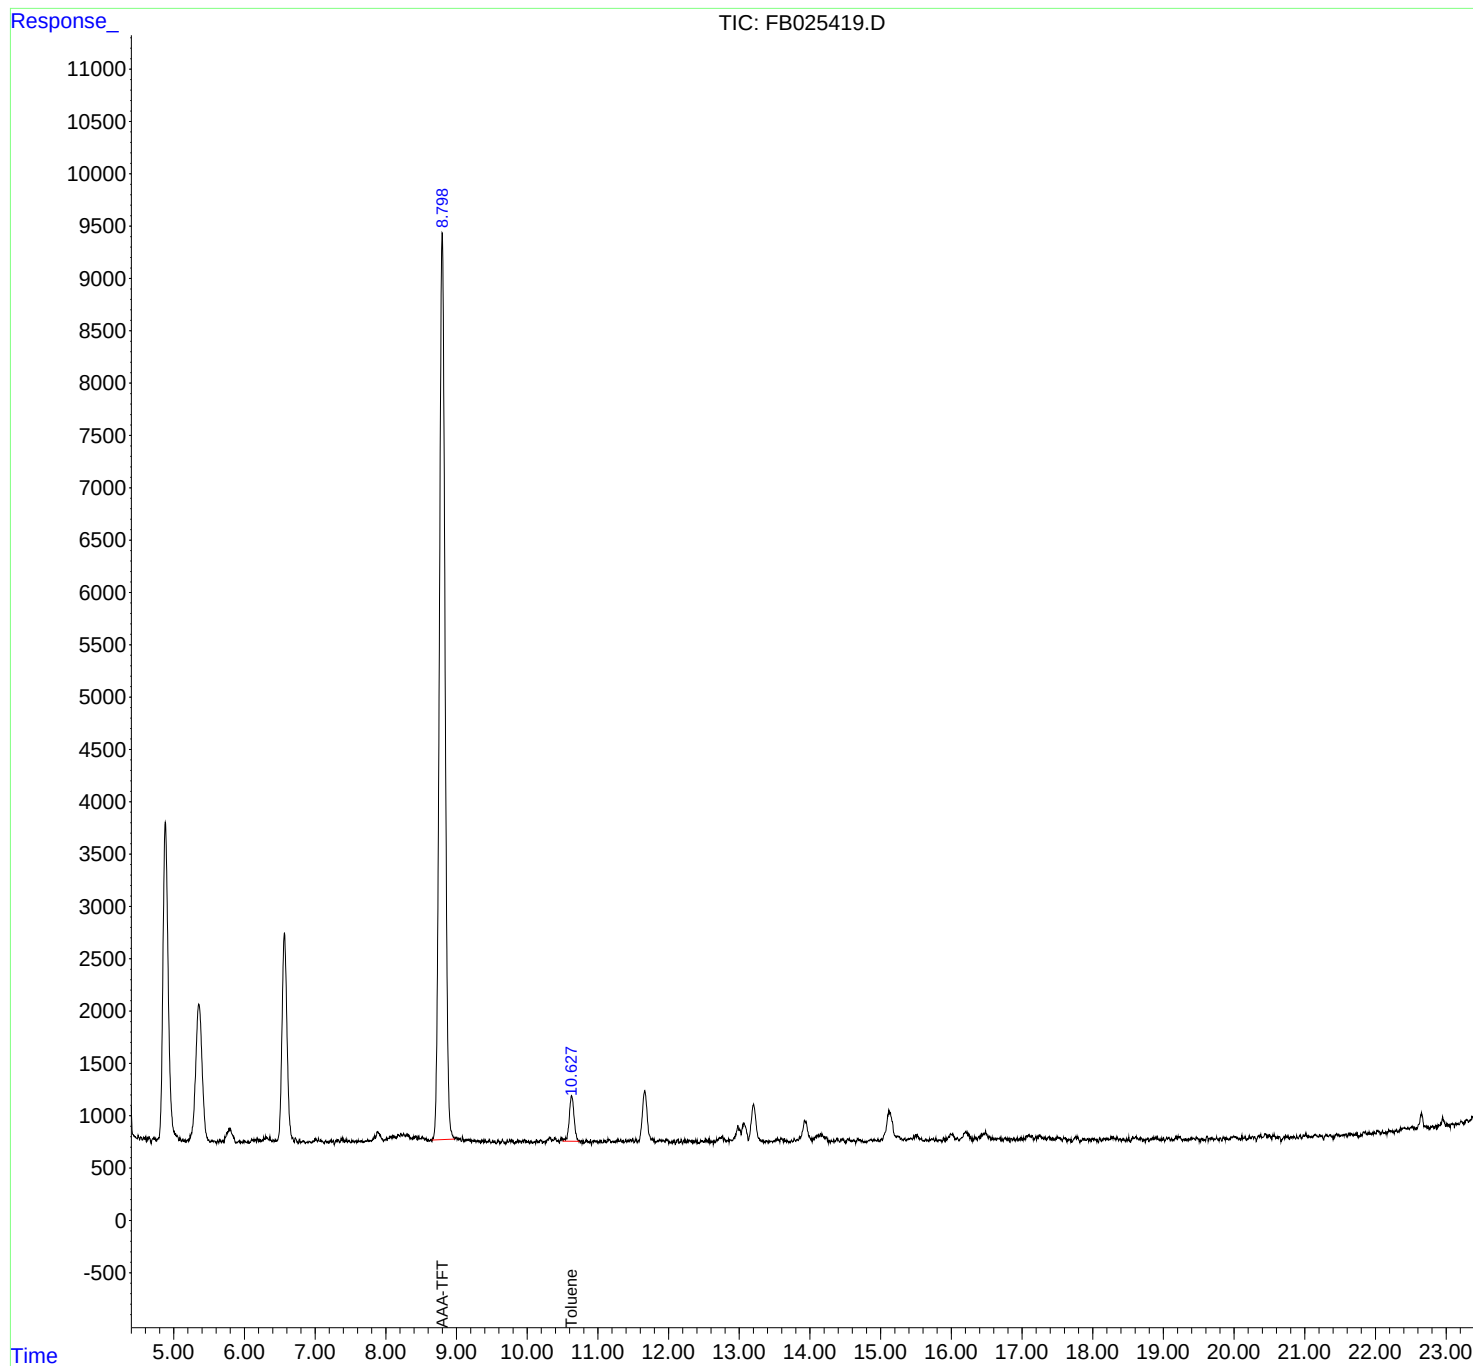


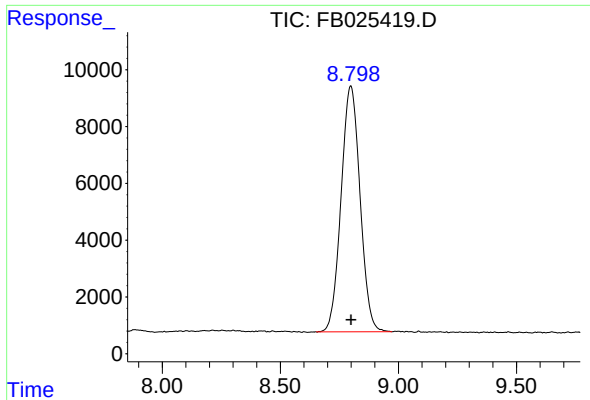

#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 483500
Conc: 21.49 ng/ml

Instrument :
FID_B
ClientSampleId :

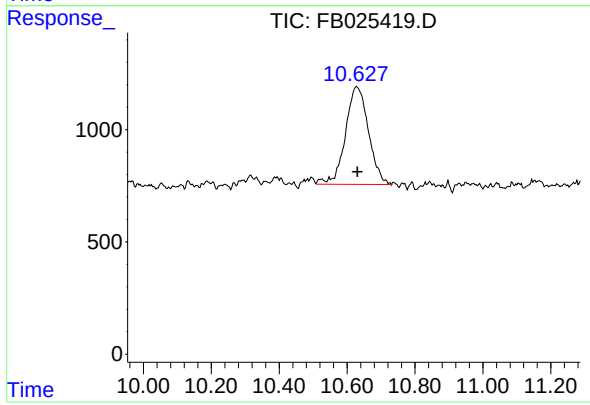

#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 20437
Conc: 0.54 ng/ml