

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012721\
 Data File : FB025417.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2021 10:12
 Operator : DD/AJ
 Sample : BSF0127S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0127S1

Integration File: Calibration.e
 Quant Time: Jan 28 00:21:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	448212	19.925 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	921552	29.277 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	970509	30.612 ng/ml
3) t n-Heptane	7.759	318565	10.187 ng/ml
4) t Benzene	7.894	380700	9.683 ng/ml
6) t Toluene	10.631	1086827	28.952 ng/ml
7) t Ethylbenzene	13.071	337123	9.842 ng/ml
8) t m-Xylene	13.204	667622	19.514 ng/ml
9) t O-Xylene	13.932	644274	19.382 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	563875	19.608 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012721\
Data File : FB025417.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2021 10:12
Operator : DD/AJ
Sample : BSF0127S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0127S1

Integration File: Calibration.e
Quant Time: Jan 28 00:21:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

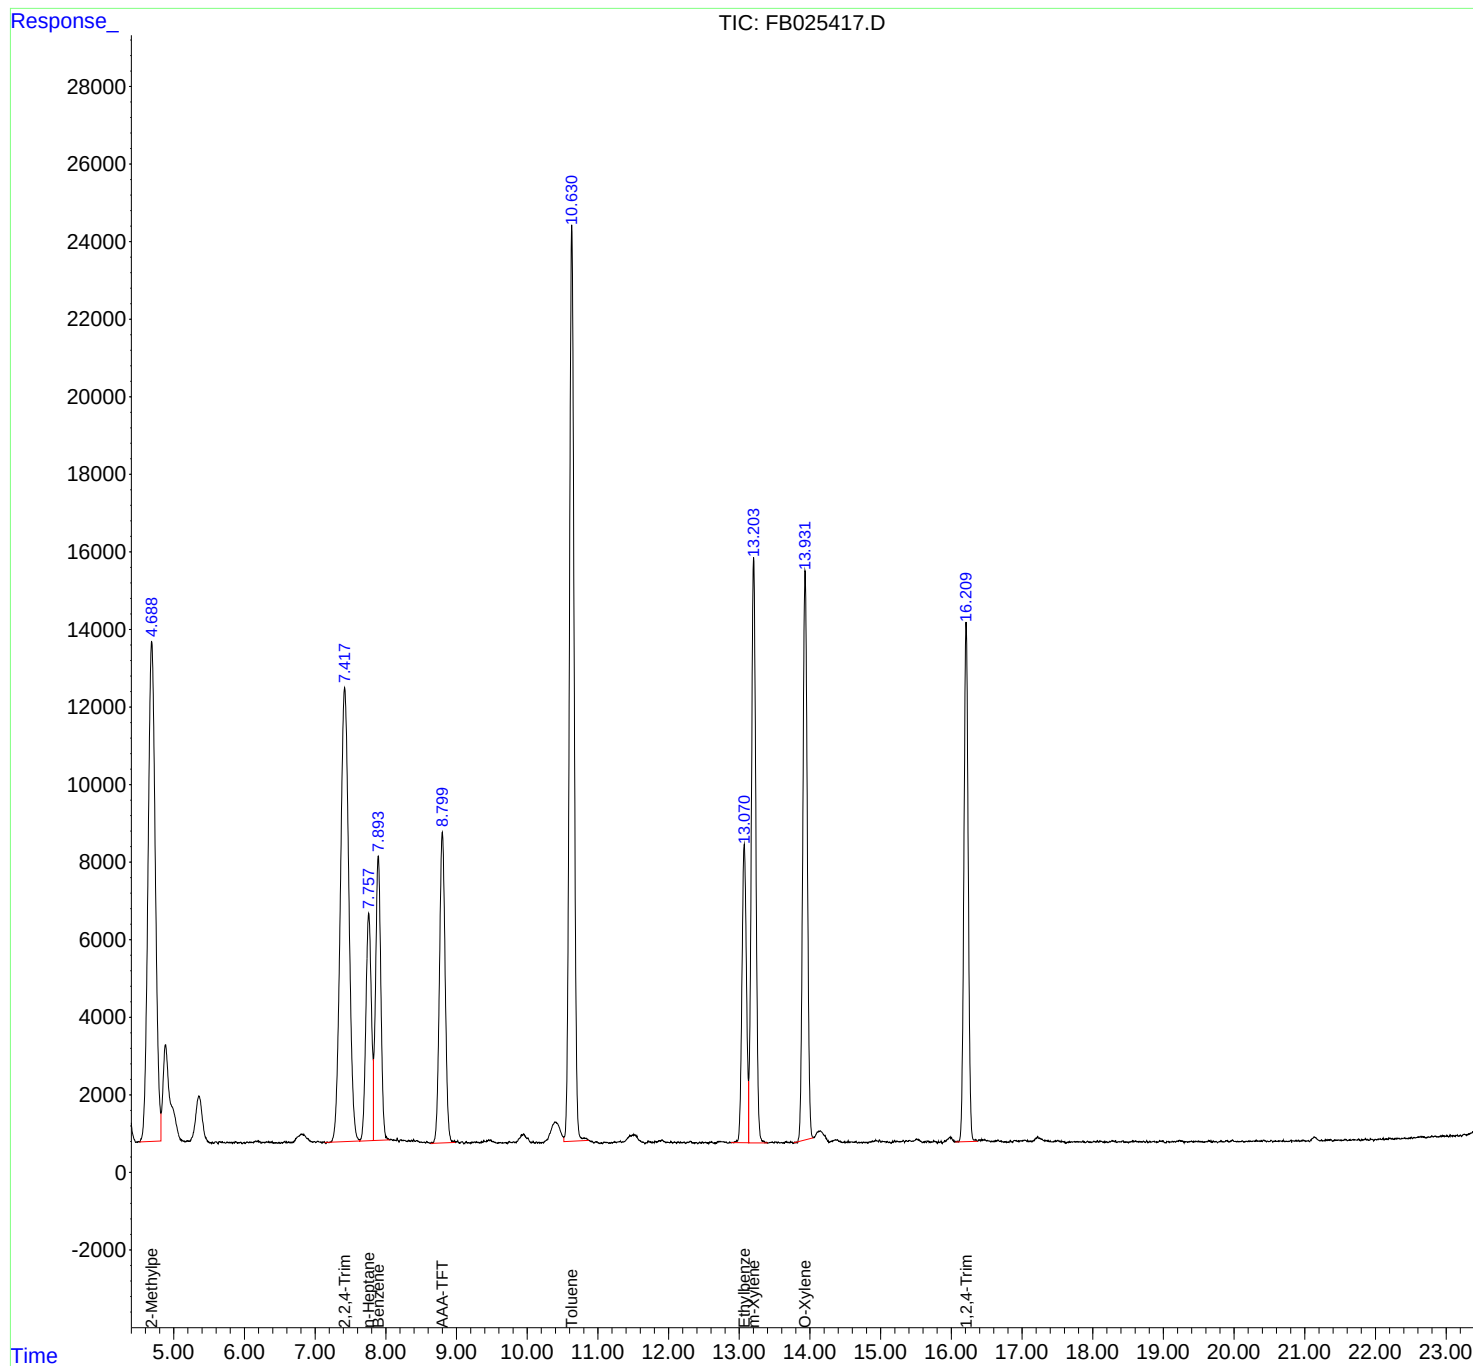


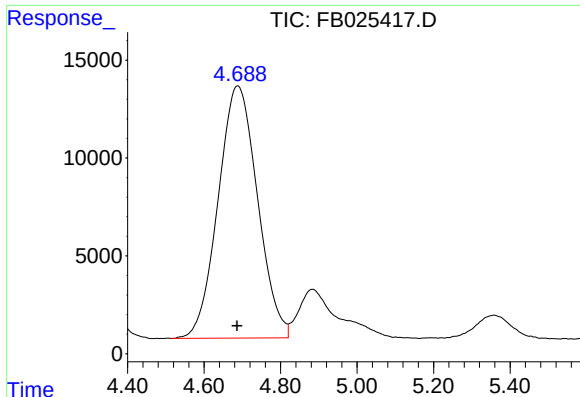

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.003 min
Response: 921552
Conc: 29.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S1

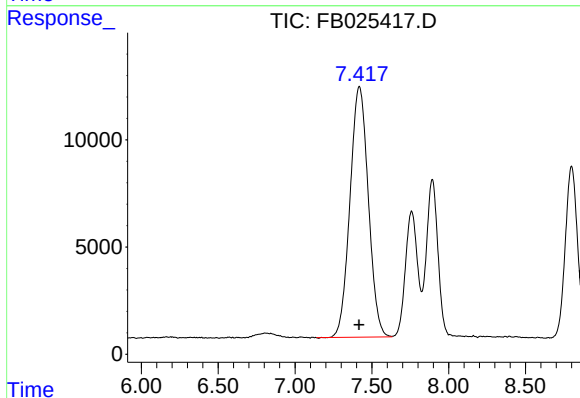


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 970509
Conc: 30.61 ng/ml

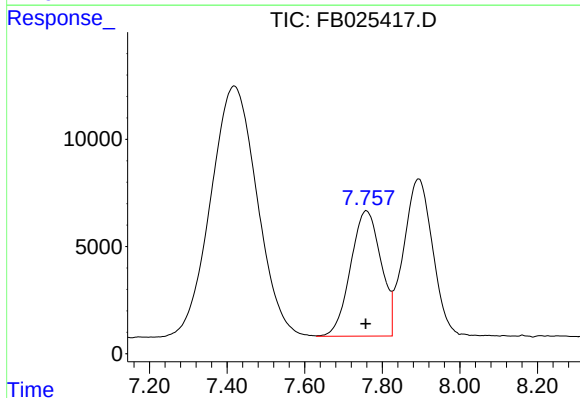


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.002 min
Response: 318565
Conc: 10.19 ng/ml

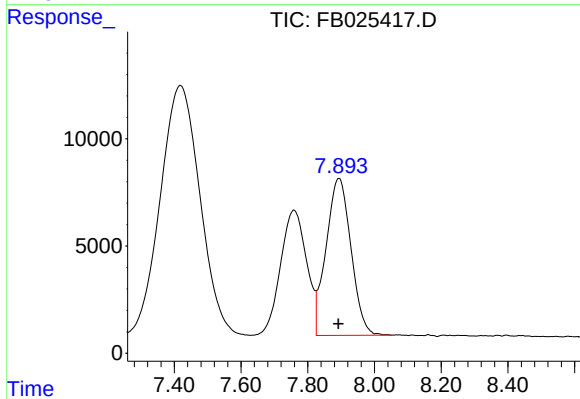

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 380700
Conc: 9.68 ng/ml

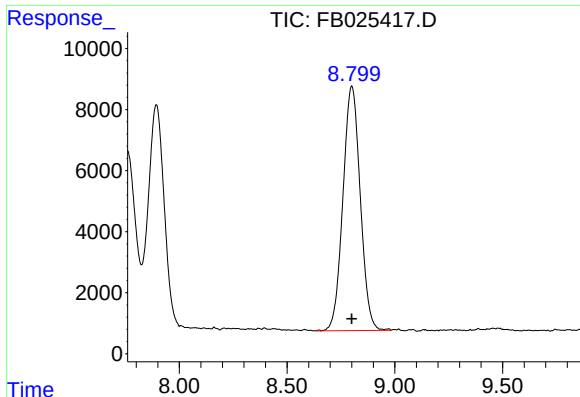

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 448212
Conc: 19.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S1

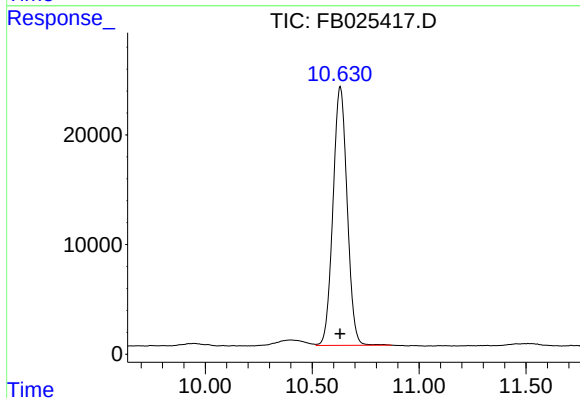


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1086827
Conc: 28.95 ng/ml

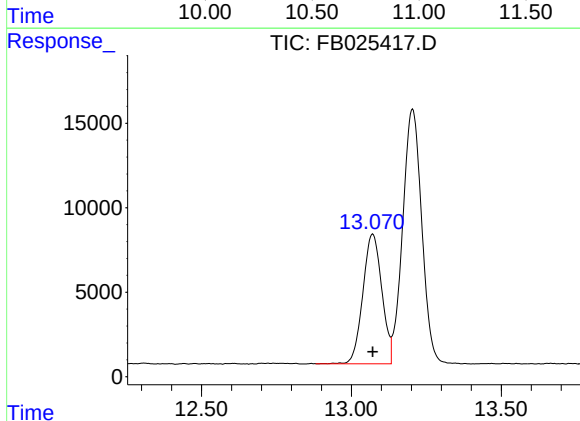


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 337123
Conc: 9.84 ng/ml

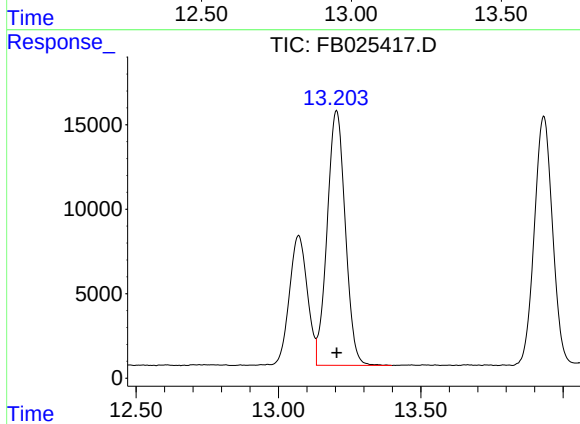

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 667622
Conc: 19.51 ng/ml

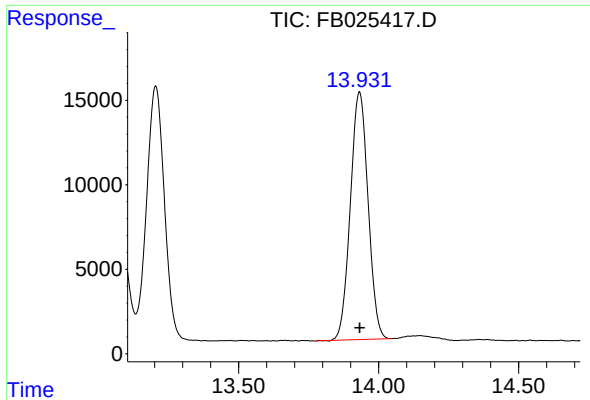

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 644274
Conc: 19.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S1

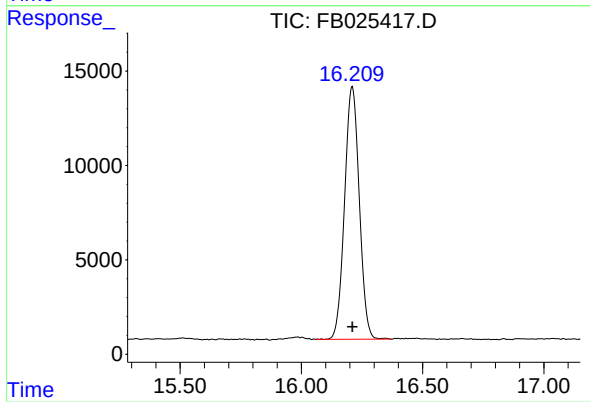

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 563875
Conc: 19.61 ng/ml