

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012721\
 Data File : FB025418.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2021 10:43
 Operator : DD/AJ
 Sample : BSF0127S2
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0127S2

Integration File: Calibration.e
 Quant Time: Jan 28 00:22:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	472347	20.997 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	910714	28.932 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	922254	29.090 ng/ml
3) t n-Heptane	7.758	303567	9.707 ng/ml
4) t Benzene	7.893	381468	9.703 ng/ml
6) t Toluene	10.631	1079267	28.750 ng/ml
7) t Ethylbenzene	13.072	322545	9.417 ng/ml
8) t m-Xylene	13.205	652777	19.080 ng/ml
9) t O-Xylene	13.932	632153	19.017 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	557117	19.373 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012721\
Data File : FB025418.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2021 10:43
Operator : DD/AJ
Sample : BSF0127S2
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampled :
BSF0127S2

Integration File: Calibration.e
Quant Time: Jan 28 00:22:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

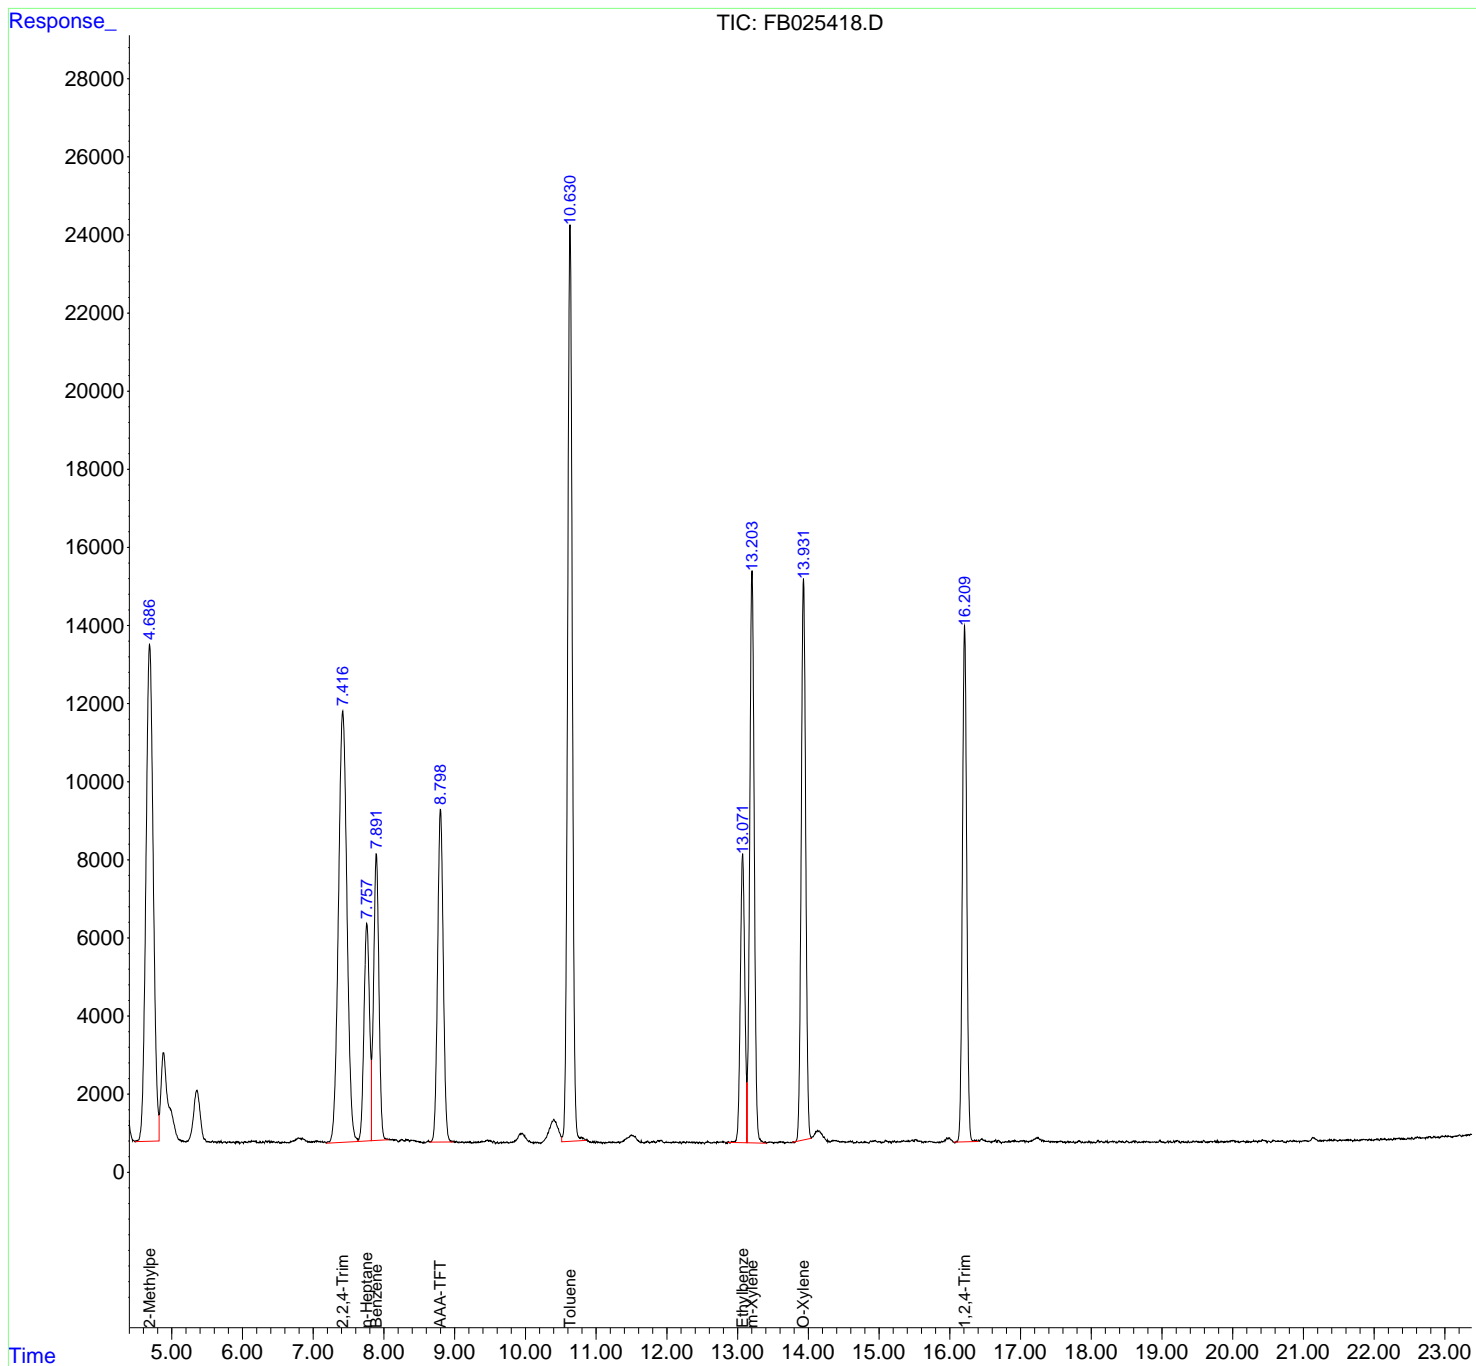


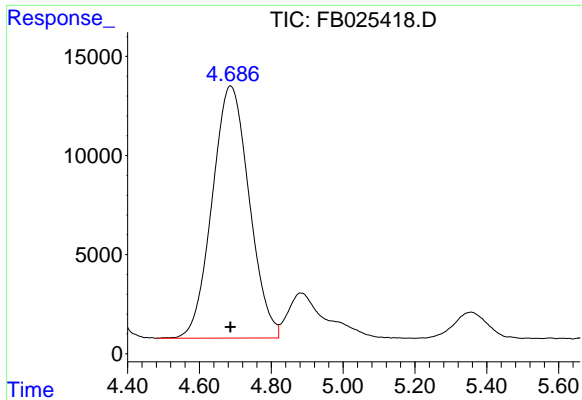

#1 2-Methylpentane


R.T.: 4.687 min
 Delta R.T.: 0.001 min
 Response: 910714
 Conc: 28.93 ng/ml

Instrument :
 FID_B
 ClientSampled :
 BSF0127S2

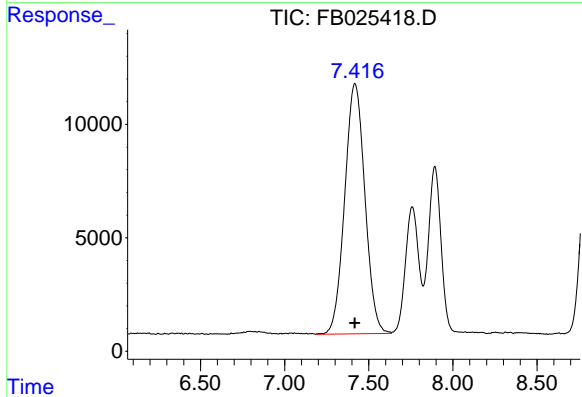


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
 Delta R.T.: 0.001 min
 Response: 922254
 Conc: 29.09 ng/ml

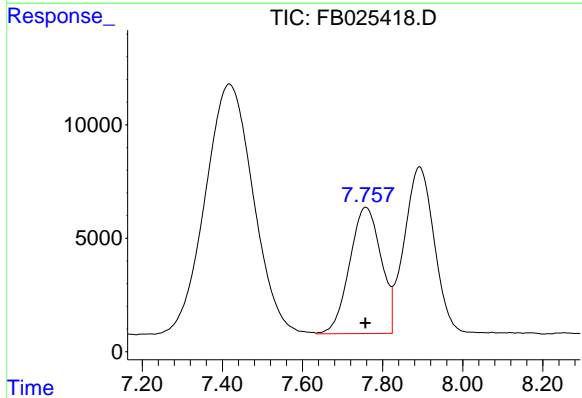


#3 n-Heptane

R.T.: 7.758 min
 Delta R.T.: 0.001 min
 Response: 303567
 Conc: 9.71 ng/ml

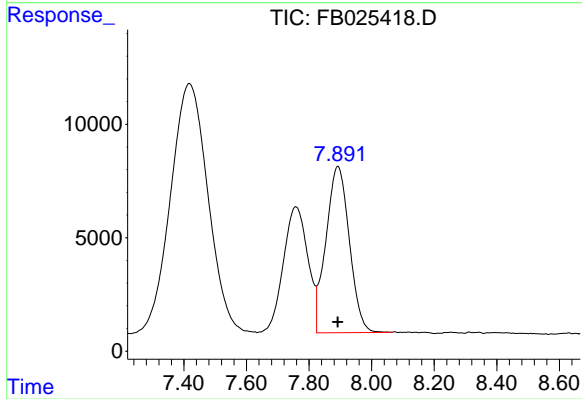


#4 Benzene

R.T.: 7.893 min
 Delta R.T.: 0.000 min
 Response: 381468
 Conc: 9.70 ng/ml

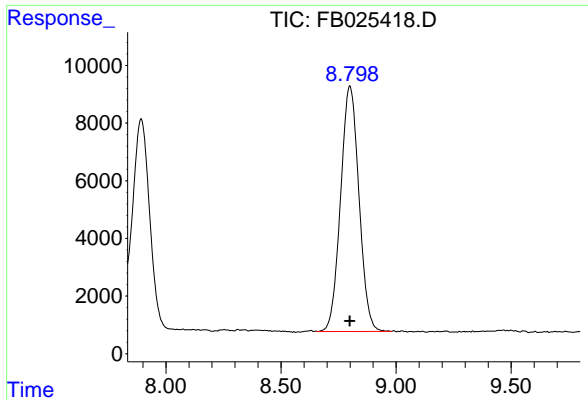


#5 AAA-TFT
 R.T.: 8.799 min
 Delta R.T.: 0.000 min
 Response: 472347
 Conc: 21.00 ng/ml


Instrument :
 FID_B
 ClientSampleId :
 BSF0127S2

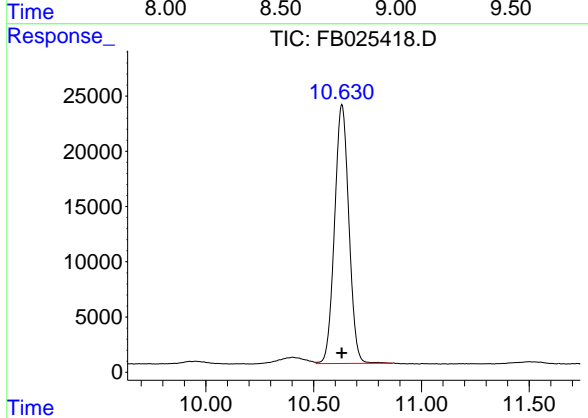


#6 Toluene
 R.T.: 10.631 min
 Delta R.T.: 0.000 min
 Response: 1079267
 Conc: 28.75 ng/ml

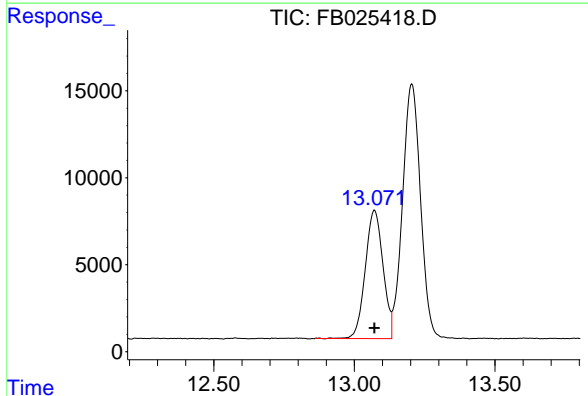

#7 Ethylbenzene
 R.T.: 13.072 min
 Delta R.T.: 0.000 min
 Response: 322545
 Conc: 9.42 ng/ml

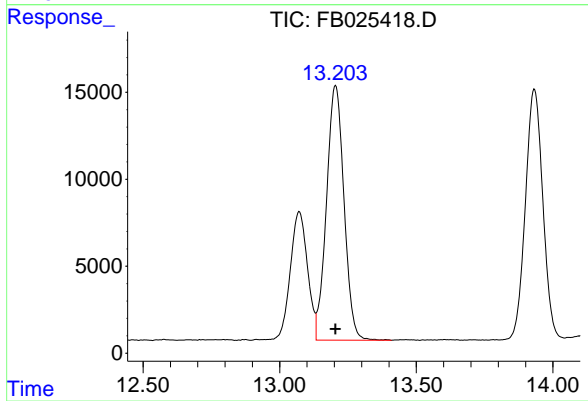


#8 m-Xylene
 R.T.: 13.205 min
 Delta R.T.: 0.000 min
 Response: 652777
 Conc: 19.08 ng/ml

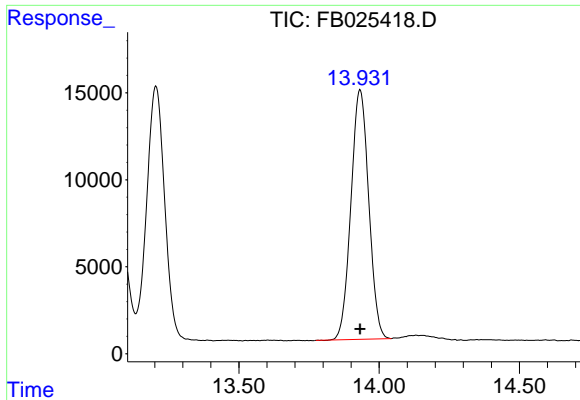

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 632153
Conc: 19.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0127S2

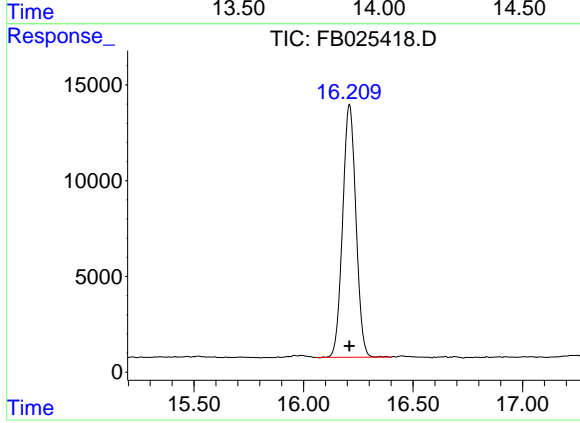

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 557117
Conc: 19.37 ng/ml