

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012723\
 Data File : FB029168.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2023 12:26
 Operator : AJ/MA
 Sample : 01318-01
 Misc : 7.68G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 27 16:58:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.789	216773	17.740 ng/ml
Target Compounds				
6) t	Toluene	10.618	255321	12.668 ng/ml
8) t	m-Xylene	13.180	14426	0.771 ng/ml
9) t	O-Xylene	13.913	8838	0.491 ng/ml
10) t	1,2,4-Trimethylbenzene	16.191	12908	0.724 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012723\
Data File : FB029168.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2023 12:26
Operator : AJ/MA
Sample : 01318-01
Misc : 7.68G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 27 16:58:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

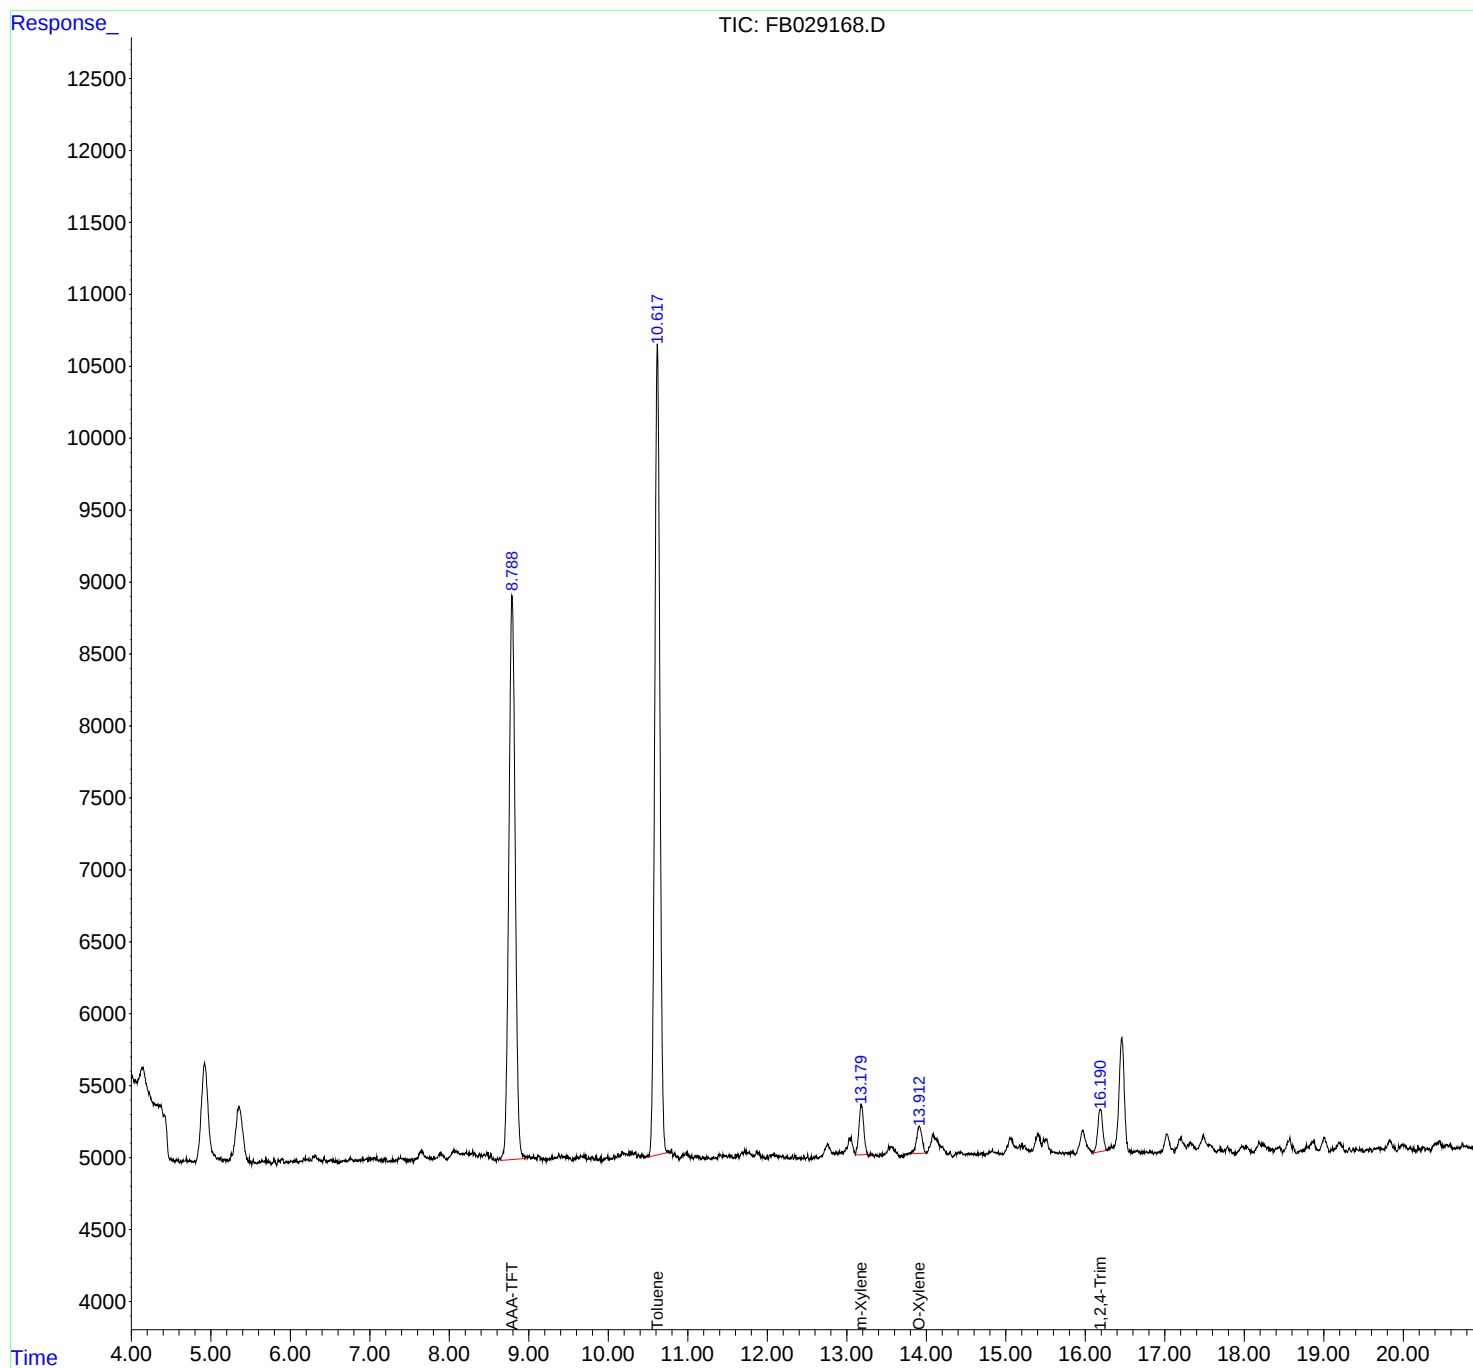

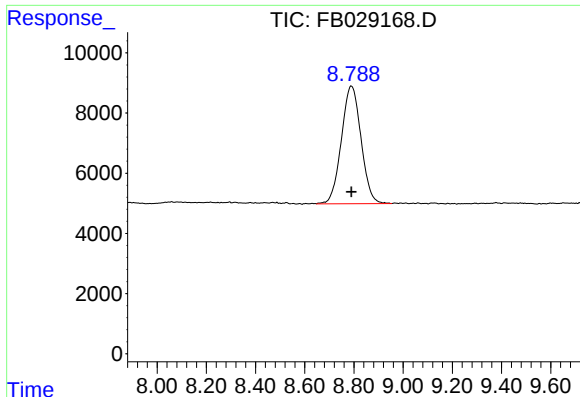


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 216773
Conc: 17.74 ng/ml

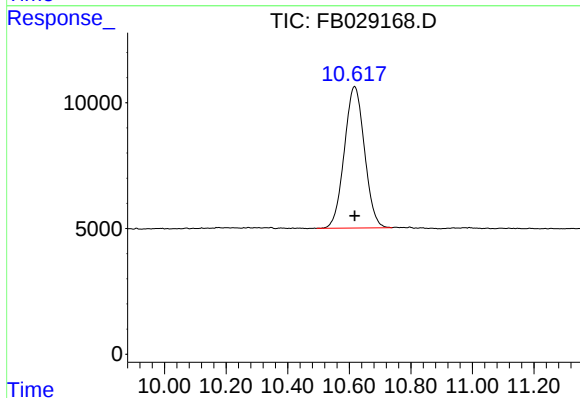


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 255321
Conc: 12.67 ng/ml

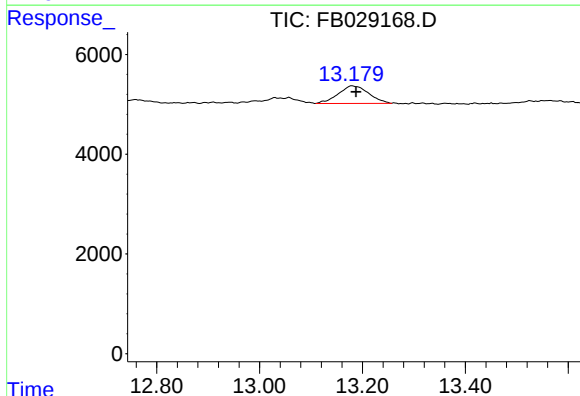


#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.007 min
Response: 14426
Conc: 0.77 ng/ml

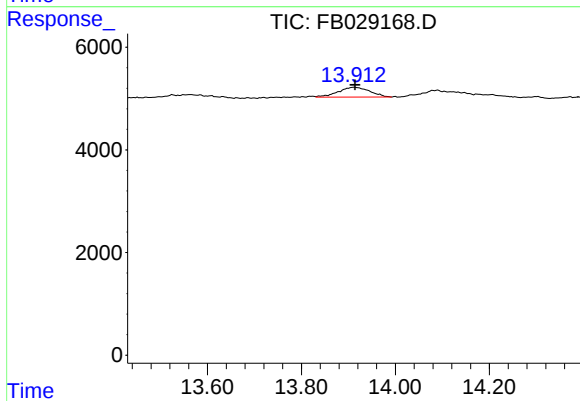

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.002 min
Response: 8838
Conc: 0.49 ng/ml

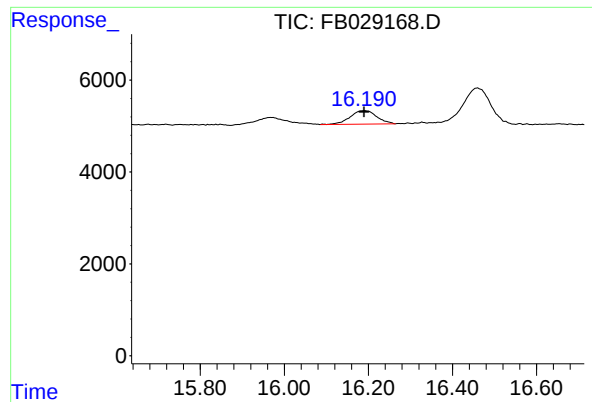

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.001 min
Response: 12908
Conc: 0.72 ng/ml