

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012723\
 Data File : FB029170.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2023 13:43
 Operator : AJ/MA
 Sample : BSF0127S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 27 16:58:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.789	247791	20.278 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.705	365994	24.999 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	429116	27.046 ng/ml
3) t	n-Heptane	7.749	132251	7.915 ng/ml
4) t	Benzene	7.885	181282	8.527 ng/ml
6) t	Toluene	10.617	540710	26.827 ng/ml
7) t	Ethylbenzene	13.054	171402	8.936 ng/ml
8) t	m-Xylene	13.186	340433	18.195 ng/ml
9) t	O-Xylene	13.914	331718	18.434 ng/ml
10) t	1,2,4-Trimethylbenzene	16.189	334477	18.762 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012723\
Data File : FB029170.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2023 13:43
Operator : AJ/MA
Sample : BSF0127S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 27 16:58:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

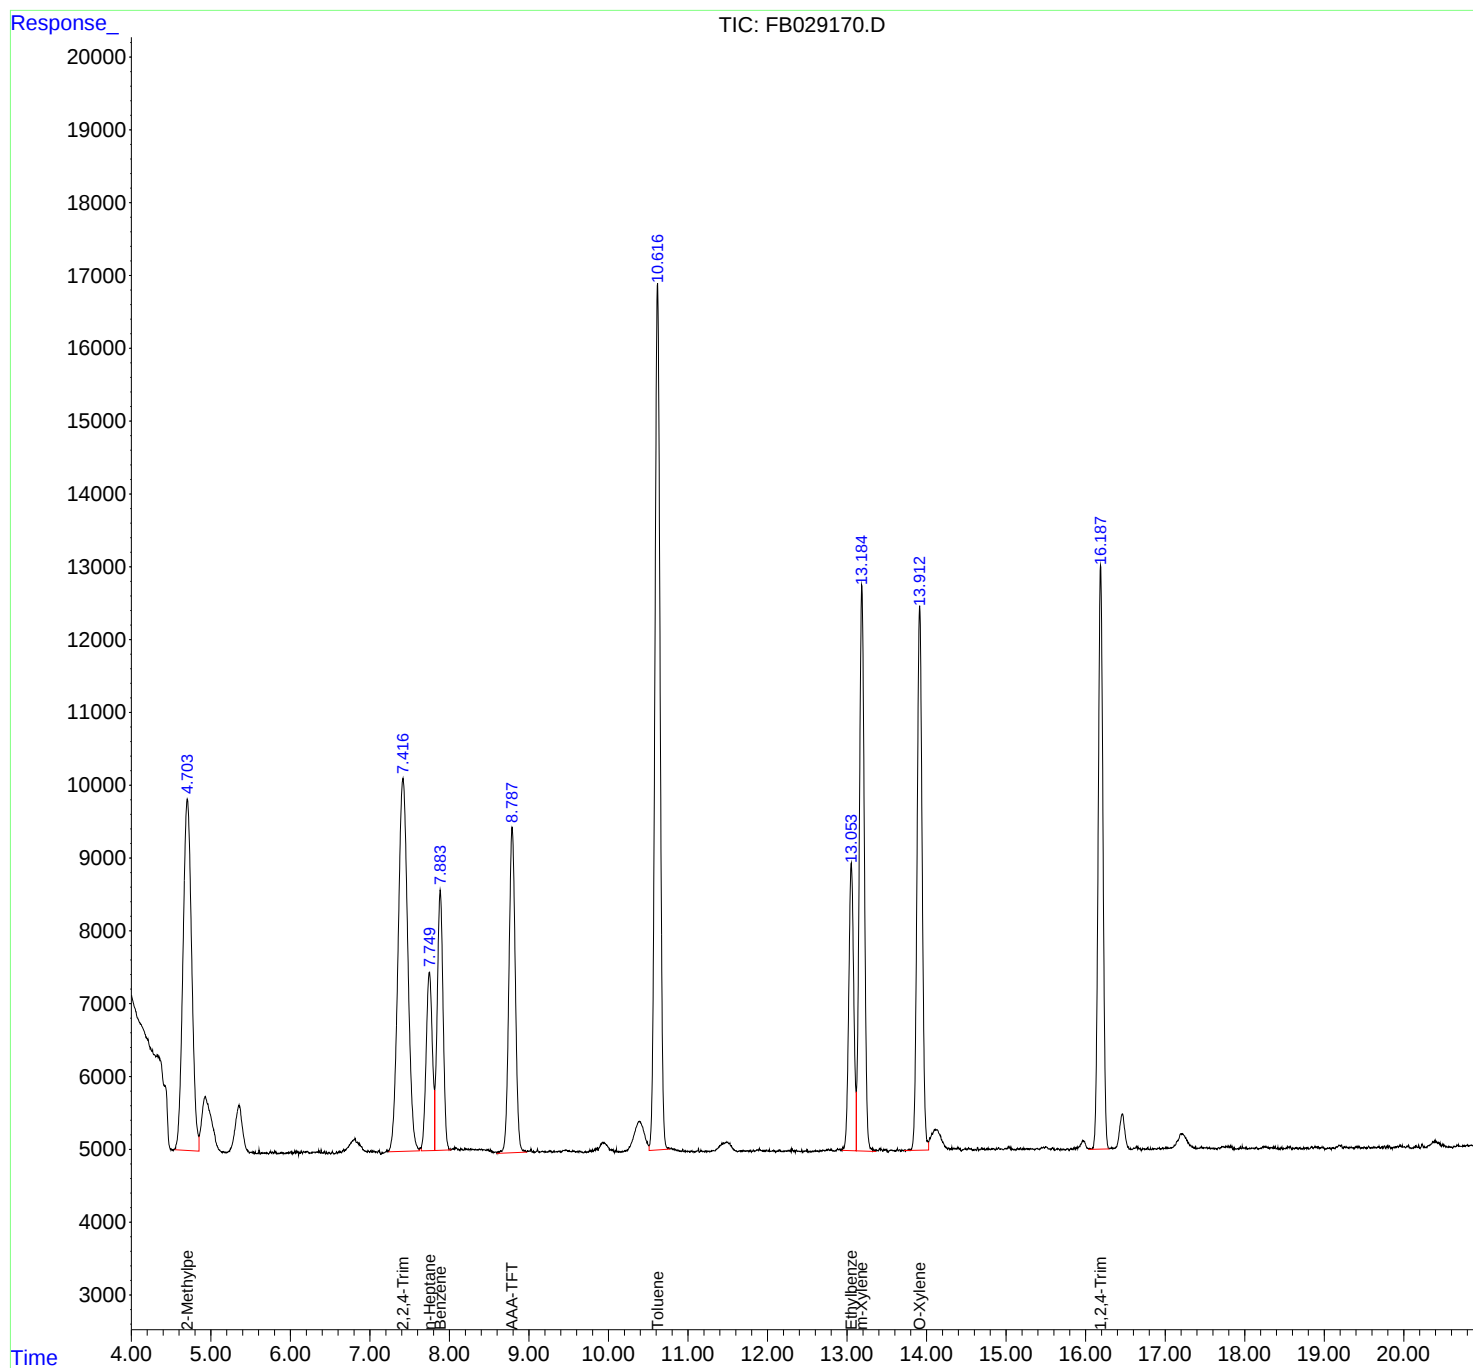

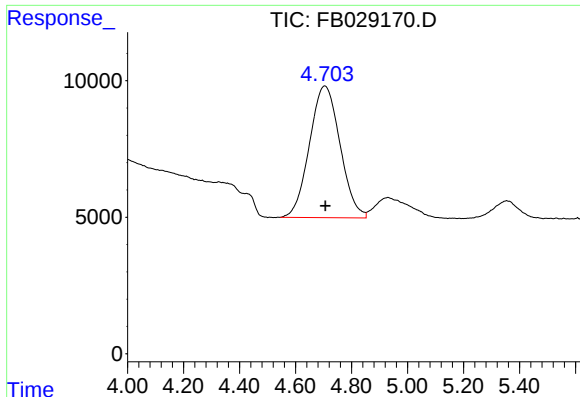


#1 2-Methylpentane

R.T.: 4.705 min
Delta R.T.: -0.002 min
Response: 365994
Conc: 25.00 ng/ml

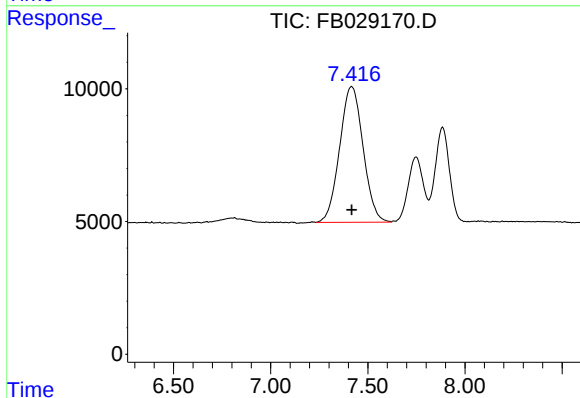


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 429116
Conc: 27.05 ng/ml

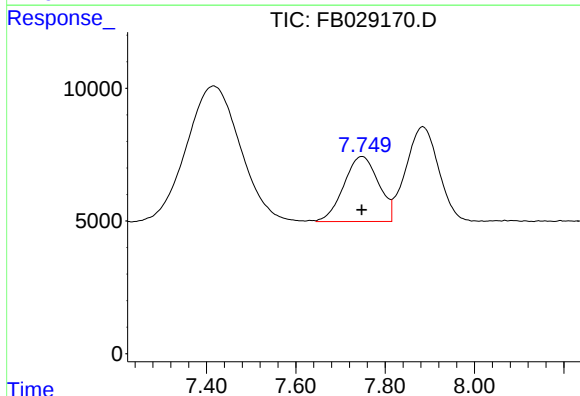


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.002 min
Response: 132251
Conc: 7.91 ng/ml

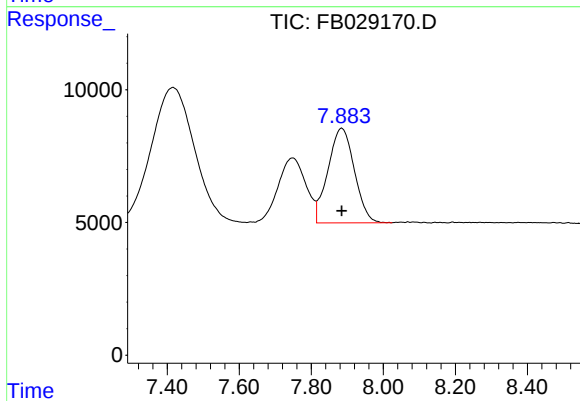


#4 Benzene

R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 181282
Conc: 8.53 ng/ml

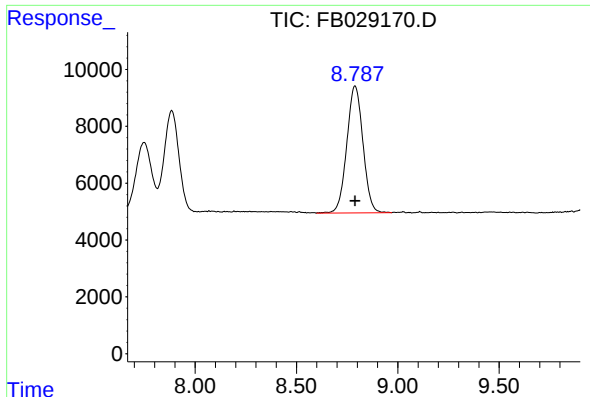


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 247791
Conc: 20.28 ng/ml

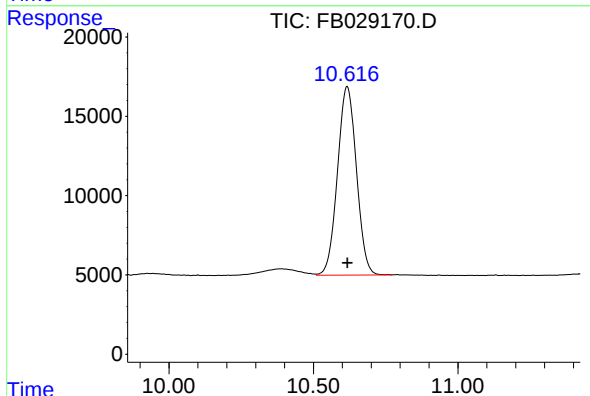


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 540710
Conc: 26.83 ng/ml

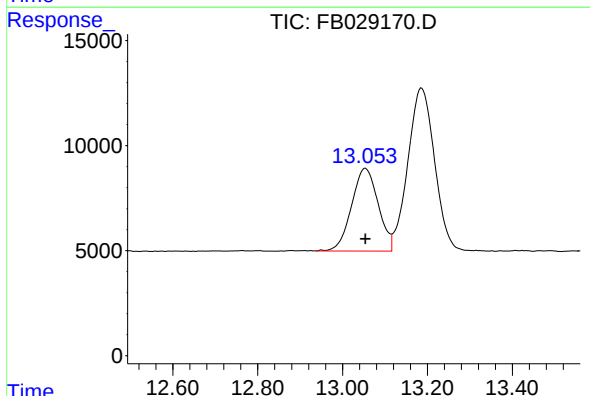


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 171402
Conc: 8.94 ng/ml

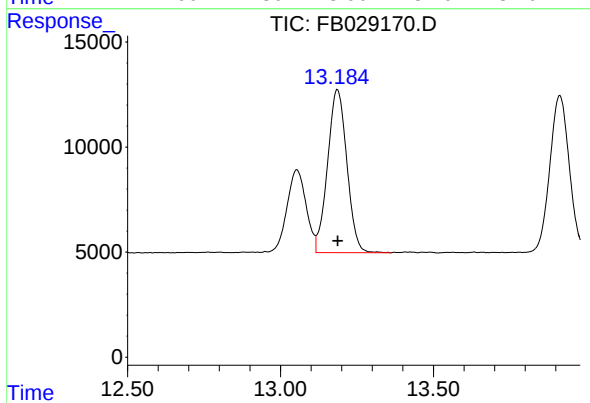


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 340433
Conc: 18.20 ng/ml

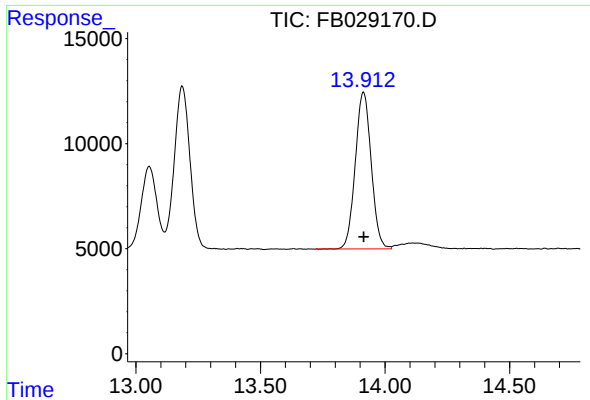

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.000 min
Response: 331718
Conc: 18.43 ng/ml

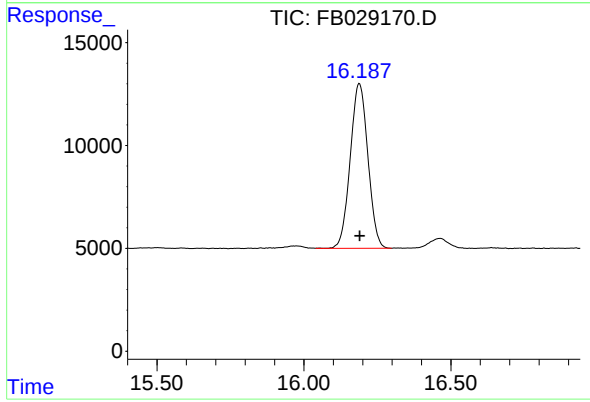

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.001 min
Response: 334477
Conc: 18.76 ng/ml