

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012725\
 Data File : FB031349.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jan 2025 11:46
 Operator : YP/AJ
 Sample : BSF0127S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 28 00:29:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	426543	17.882 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	1033925	31.193 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1212254	32.234 ng/ml
3) t n-Heptane	7.752	373108	10.336 ng/ml
4) t Benzene	7.890	460009	10.801 ng/ml
6) t Toluene	10.619	1259639	32.260 ng/ml
7) t Ethylbenzene	13.056	365769	10.563 ng/ml
8) t m-Xylene	13.190	791320	21.170 ng/ml
9) t O-Xylene	13.918	743059	20.865 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	586133	20.696 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012725\
Data File : FB031349.D
Signal(s) : FID2B.CH
Acq On : 27 Jan 2025 11:46
Operator : YP/AJ
Sample : BSF0127S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 28 00:29:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

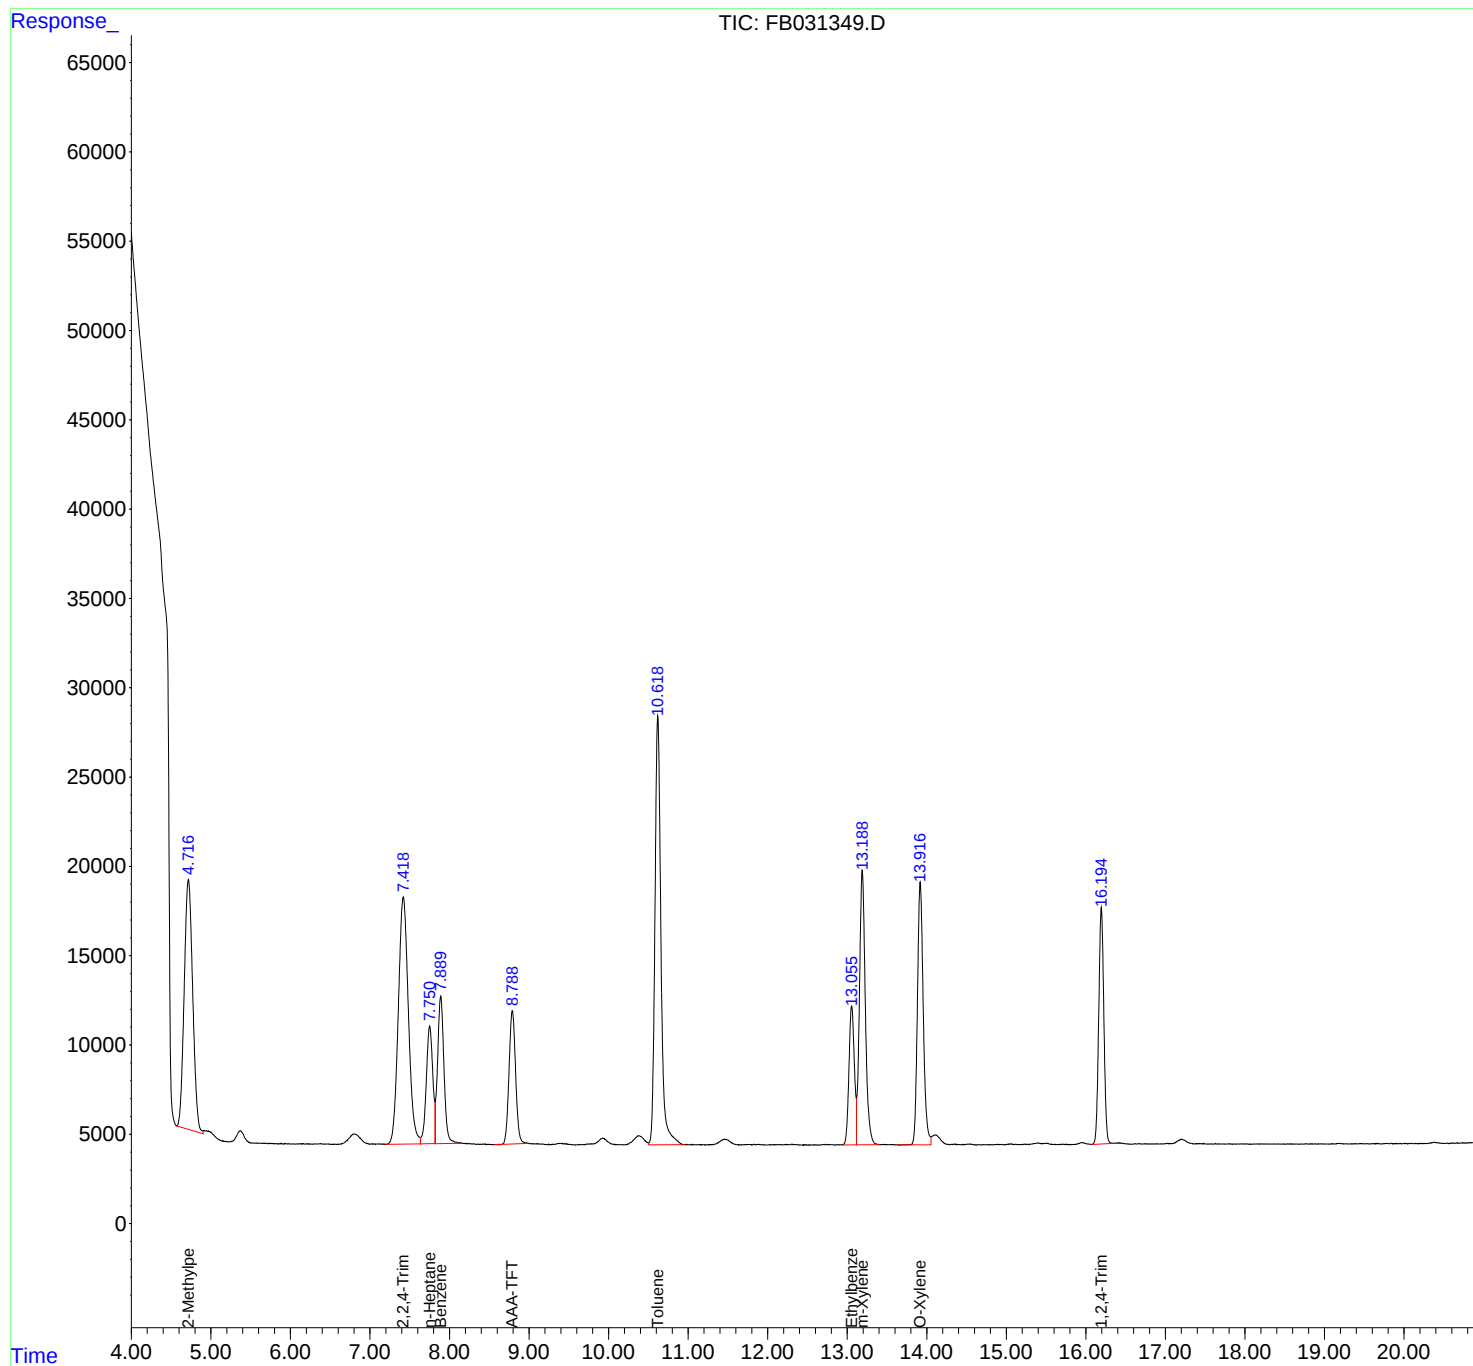


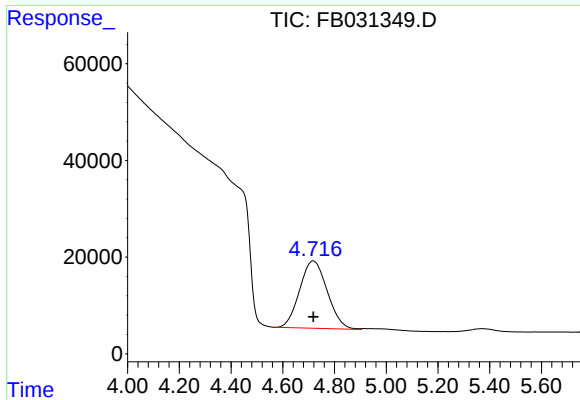

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 1033925
Conc: 31.19 ng/ml

Instrument :
FID_B
ClientSampleId :

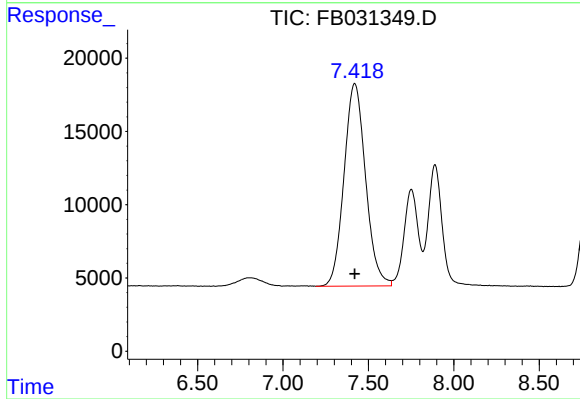


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1212254
Conc: 32.23 ng/ml

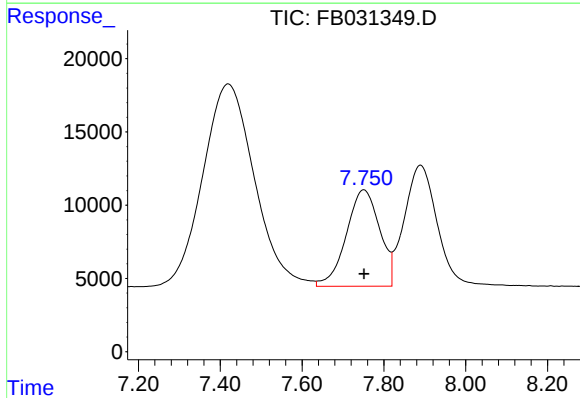


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 373108
Conc: 10.34 ng/ml

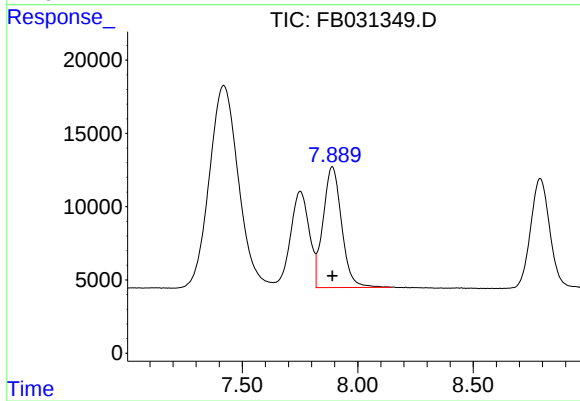

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 460009
Conc: 10.80 ng/ml

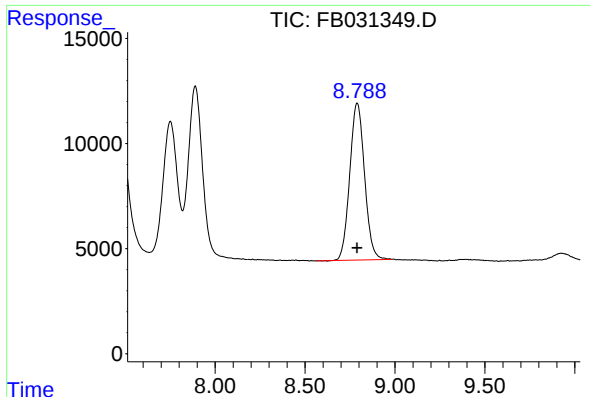

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 426543
Conc: 17.88 ng/ml

Instrument :
FID_B
ClientSampleId :

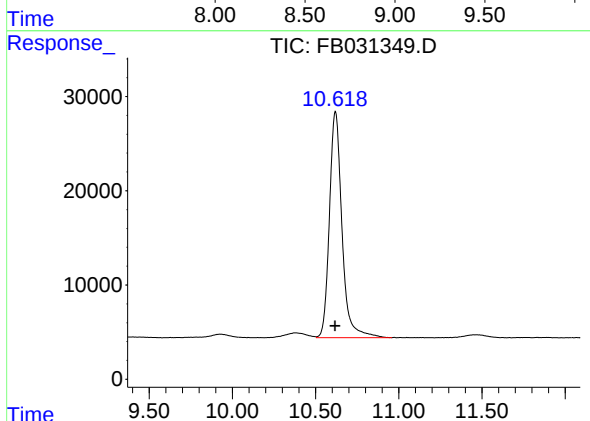


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.001 min
Response: 1259639
Conc: 32.26 ng/ml

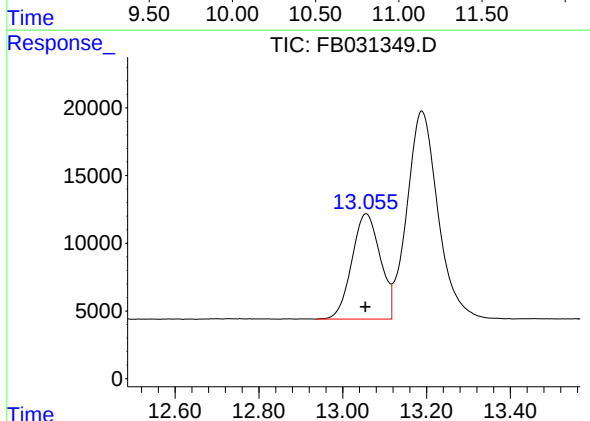


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 365769
Conc: 10.56 ng/ml

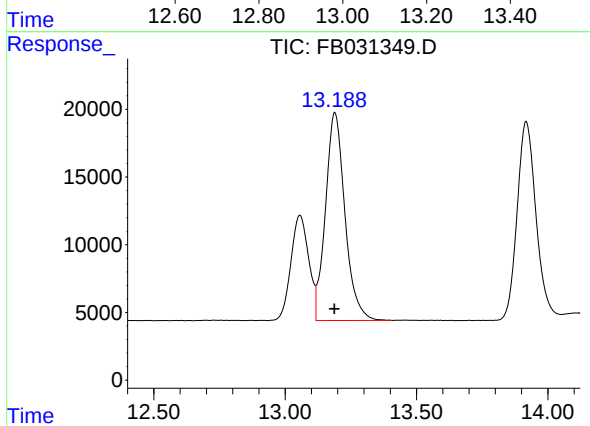

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 791320
Conc: 21.17 ng/ml

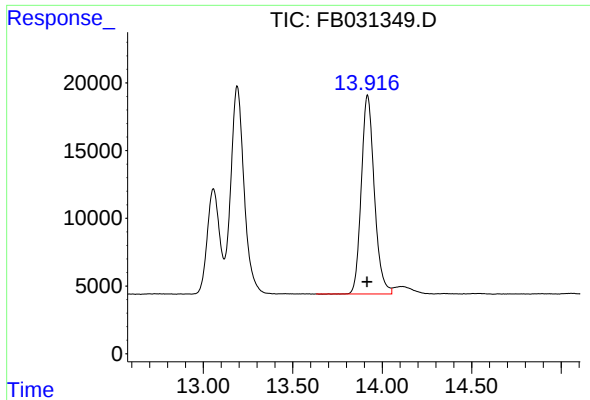

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 743059
Conc: 20.86 ng/ml

Instrument :
FID_B
ClientSampleId :

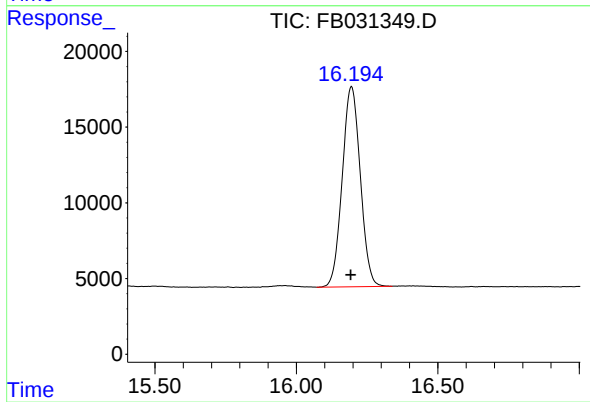

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 586133
Conc: 20.70 ng/ml