

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012919\
Data File : FB019572.D
Signal(s) : FID2B.CH
Acq On : 29 Jan 2019 14:20
Operator : MJ/SJ
Sample : BSF0129S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 29 15:23:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.050	196288	17.550 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.900	537265	29.322 ng/ml
2) t	2,2,4-Trimethylpentane	7.664	521891	29.877 ng/ml
3) t	n-Heptane	8.004	163116	9.798 ng/ml
4) t	Benzene	8.142	184341	9.573 ng/ml
6) t	Toluene	10.897	512273	29.433 ng/ml
7) t	Ethylbenzene	13.349	208749	9.641 ng/ml
8) t	m-Xylene	13.483	440113	19.486 ng/ml
9) t	O-Xylene	14.215	429664	19.430 ng/ml
10) t	1,2,4-Trimethylbenzene	16.501	441720	19.407 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB012919\
Data File : FB019572.D
Signal(s) : FID2B.CH
Acq On : 29 Jan 2019 14:20
Operator : MJ/SJ
Sample : BSF0129S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 29 15:23:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

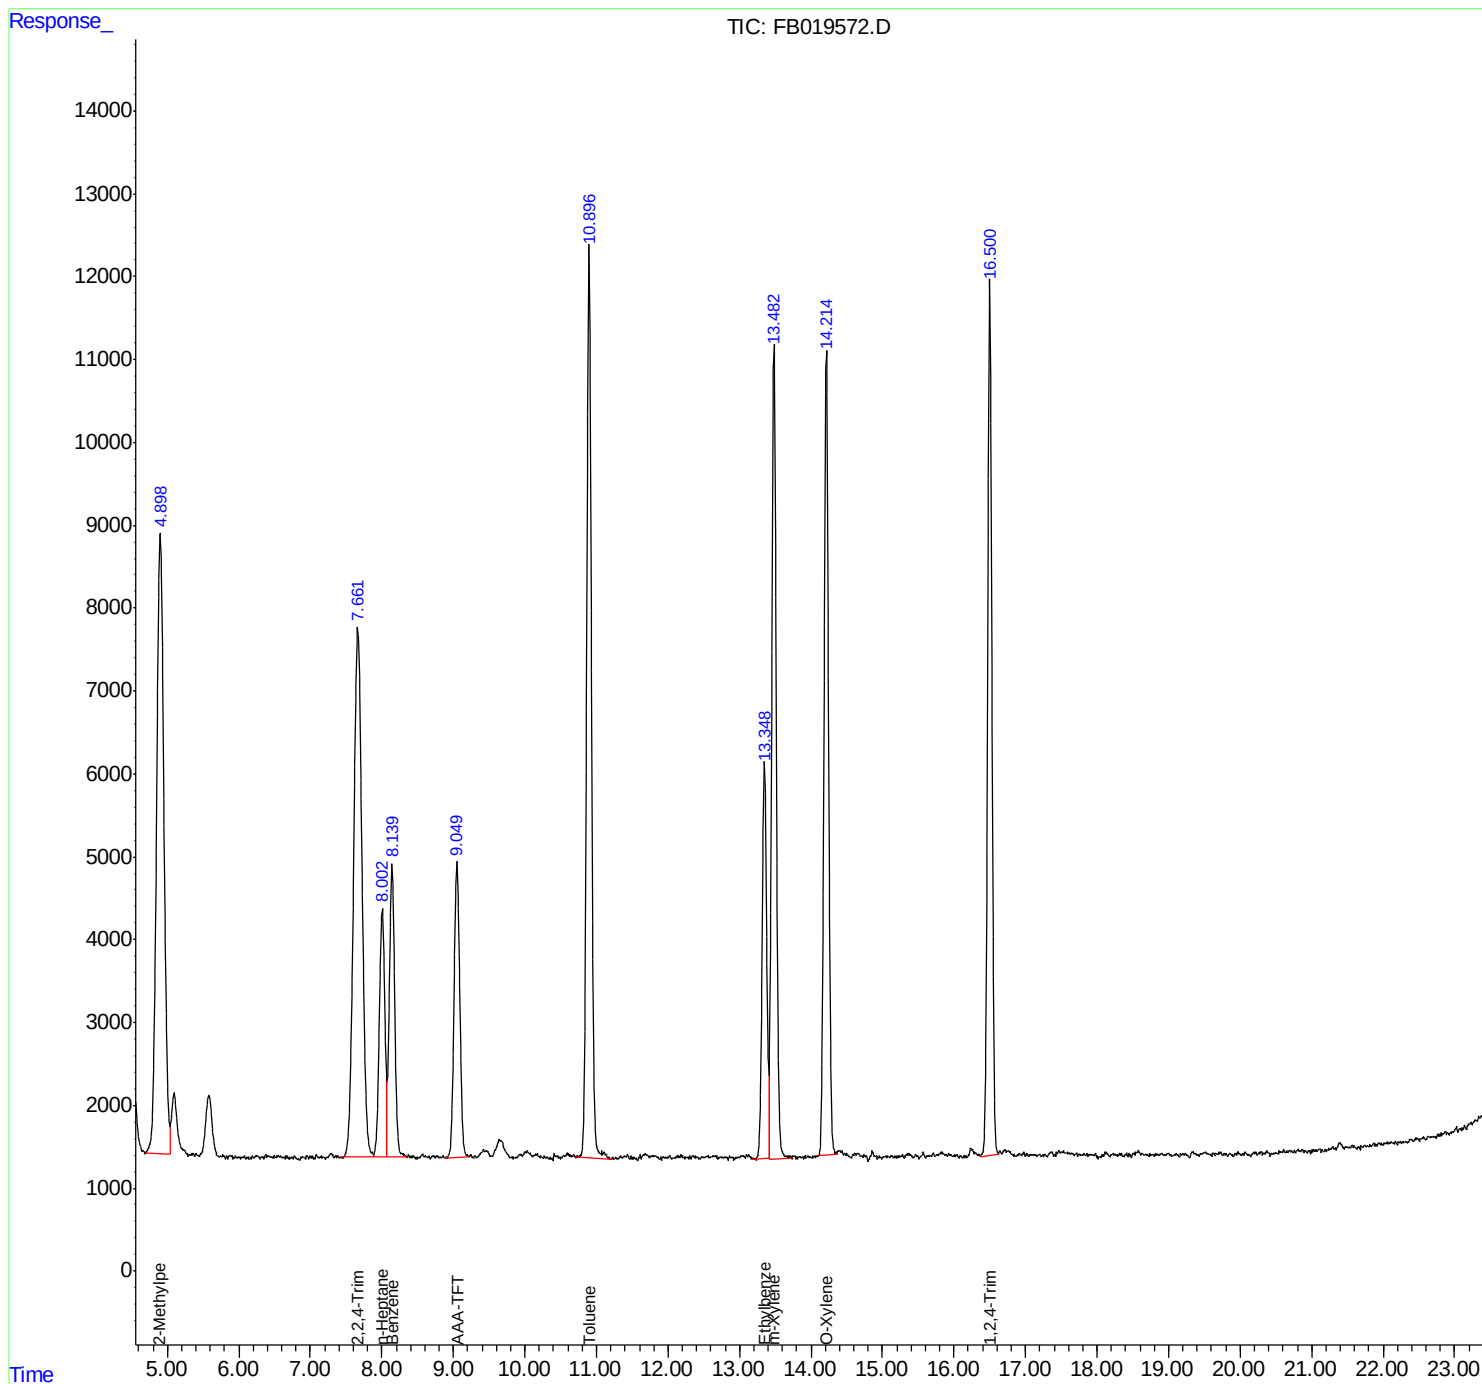

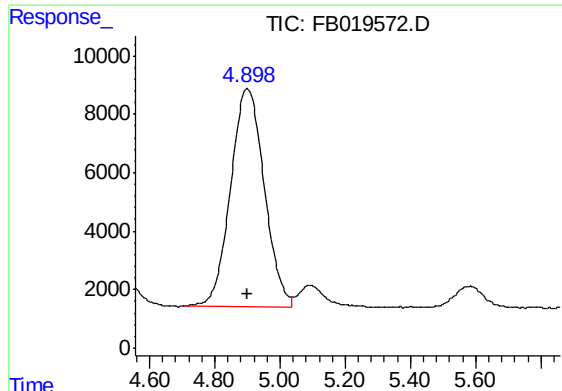


#1 2-Methylpentane

R.T.: 4.900 min
Delta R.T.: -0.002 min
Response: 537265
Conc: 29.32 ng/ml

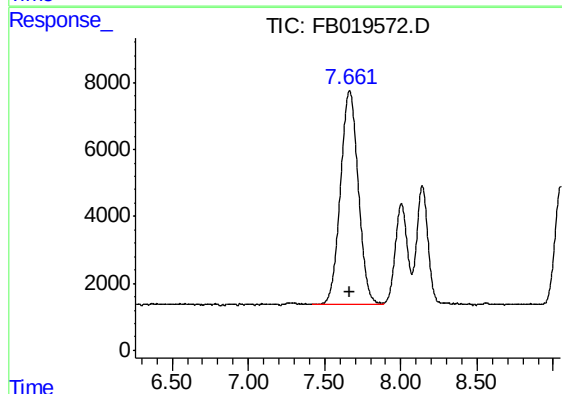


#2 2,2,4-Trimethylpentane

R.T.: 7.664 min
Delta R.T.: 0.000 min
Response: 521891
Conc: 29.88 ng/ml

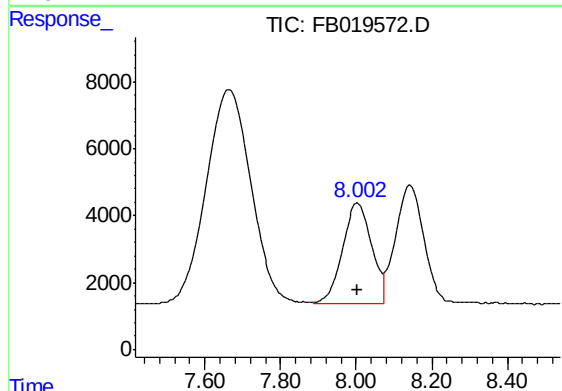


#3 n-Heptane

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 163116
Conc: 9.80 ng/ml

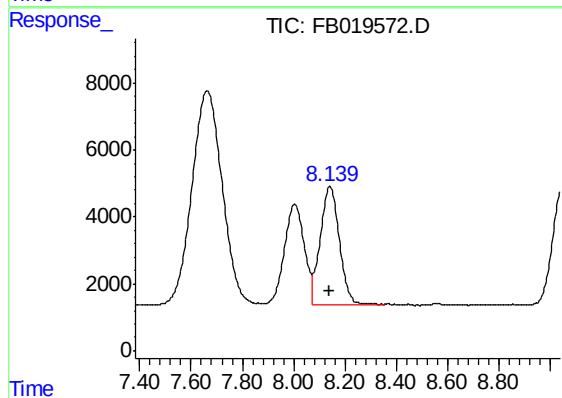


#4 Benzene

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 184341
Conc: 9.57 ng/ml

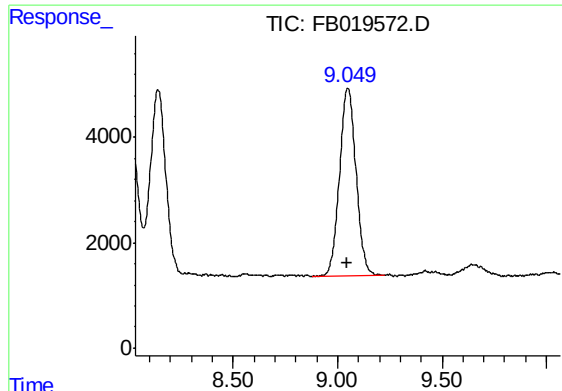


#5 AAA-TFT

R.T.: 9.050 min
Delta R.T.: 0.000 min
Response: 196288
Conc: 17.55 ng/ml

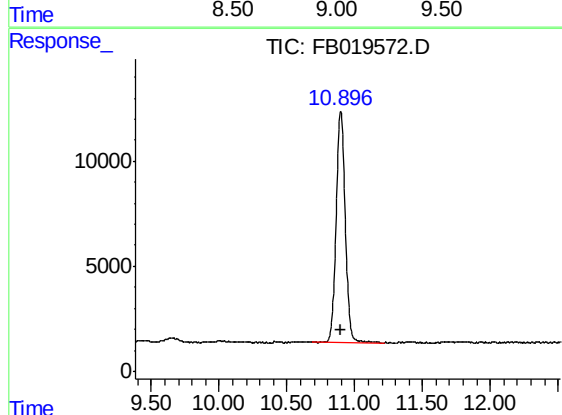


#6 Toluene

R.T.: 10.897 min
Delta R.T.: 0.000 min
Response: 512273
Conc: 29.43 ng/ml

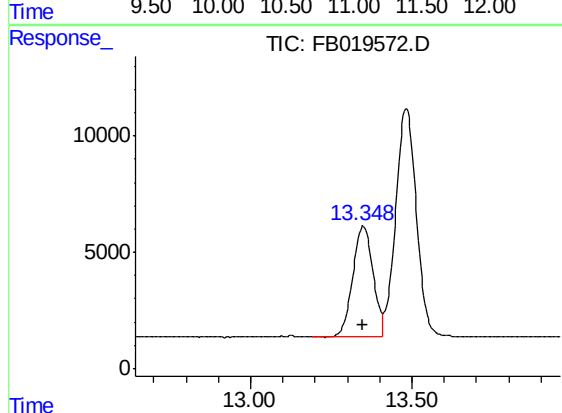


#7 Ethylbenzene

R.T.: 13.349 min
Delta R.T.: 0.000 min
Response: 208749
Conc: 9.64 ng/ml

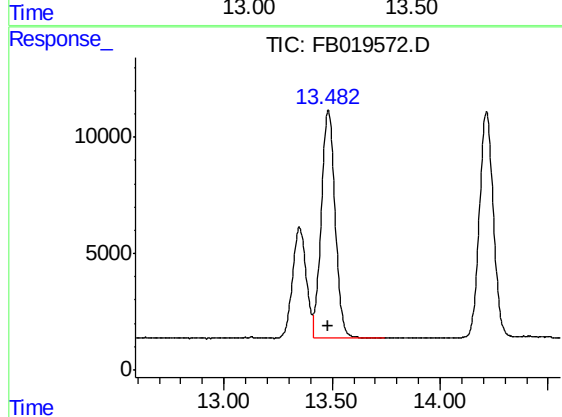


#8 m-Xylene

R.T.: 13.483 min
Delta R.T.: 0.000 min
Response: 440113
Conc: 19.49 ng/ml

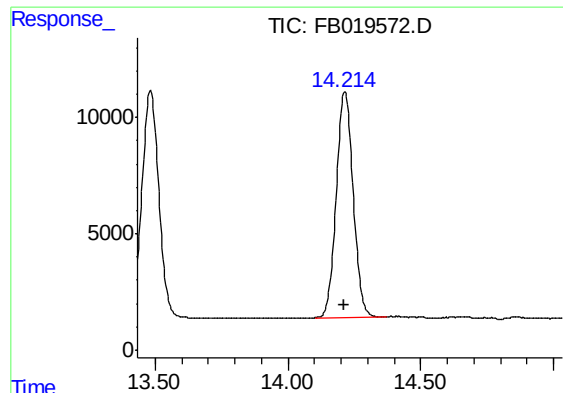

#9 O-Xylene

R.T.: 14.215 min
Delta R.T.: 0.000 min
Response: 429664
Conc: 19.43 ng/ml

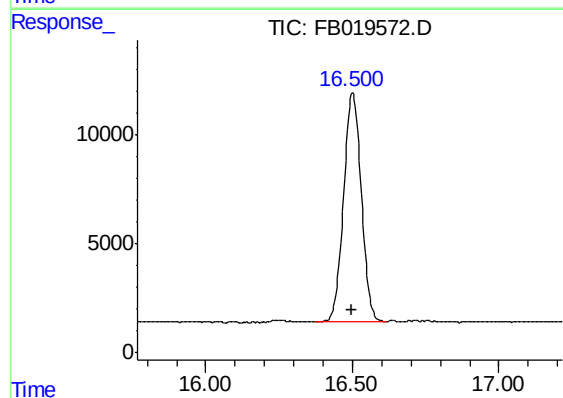

#10 1,2,4-Trimethylbenzene

R.T.: 16.501 min
Delta R.T.: 0.001 min
Response: 441720
Conc: 19.41 ng/ml