

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB012920\  
Data File : FB023562.D  
Signal(s) : FID2B.CH  
Acq On : 29 Jan 2020 13:10  
Operator : DD/AJ  
Sample : L1289-21  
Misc : 5.04g/5.00ml DI WATER  
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jan 30 00:42:52 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011620.M  
Quant Title :  
QLast Update : Thu Jan 16 11:42:55 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.796  | 534160   | 22.487 ng/ml |
| Target Compounds            |        |          |              |
| 1) t 2-Methylpentane        | 4.683  | 3806     | 0.120 ng/ml  |
| 6) t Toluene                | 10.621 | 2089     | 0.053 ng/ml  |
| 9) t O-Xylene               | 13.940 | 1039     | 0.030 ng/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB012920\  
Data File : FB023562.D  
Signal(s) : FID2B.CH  
Acq On : 29 Jan 2020 13:10  
Operator : DD/AJ  
Sample : L1289-21  
Misc : 5.04g/5.00ml DI WATER  
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jan 30 00:42:52 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011620.M  
Quant Title :  
QLast Update : Thu Jan 16 11:42:55 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

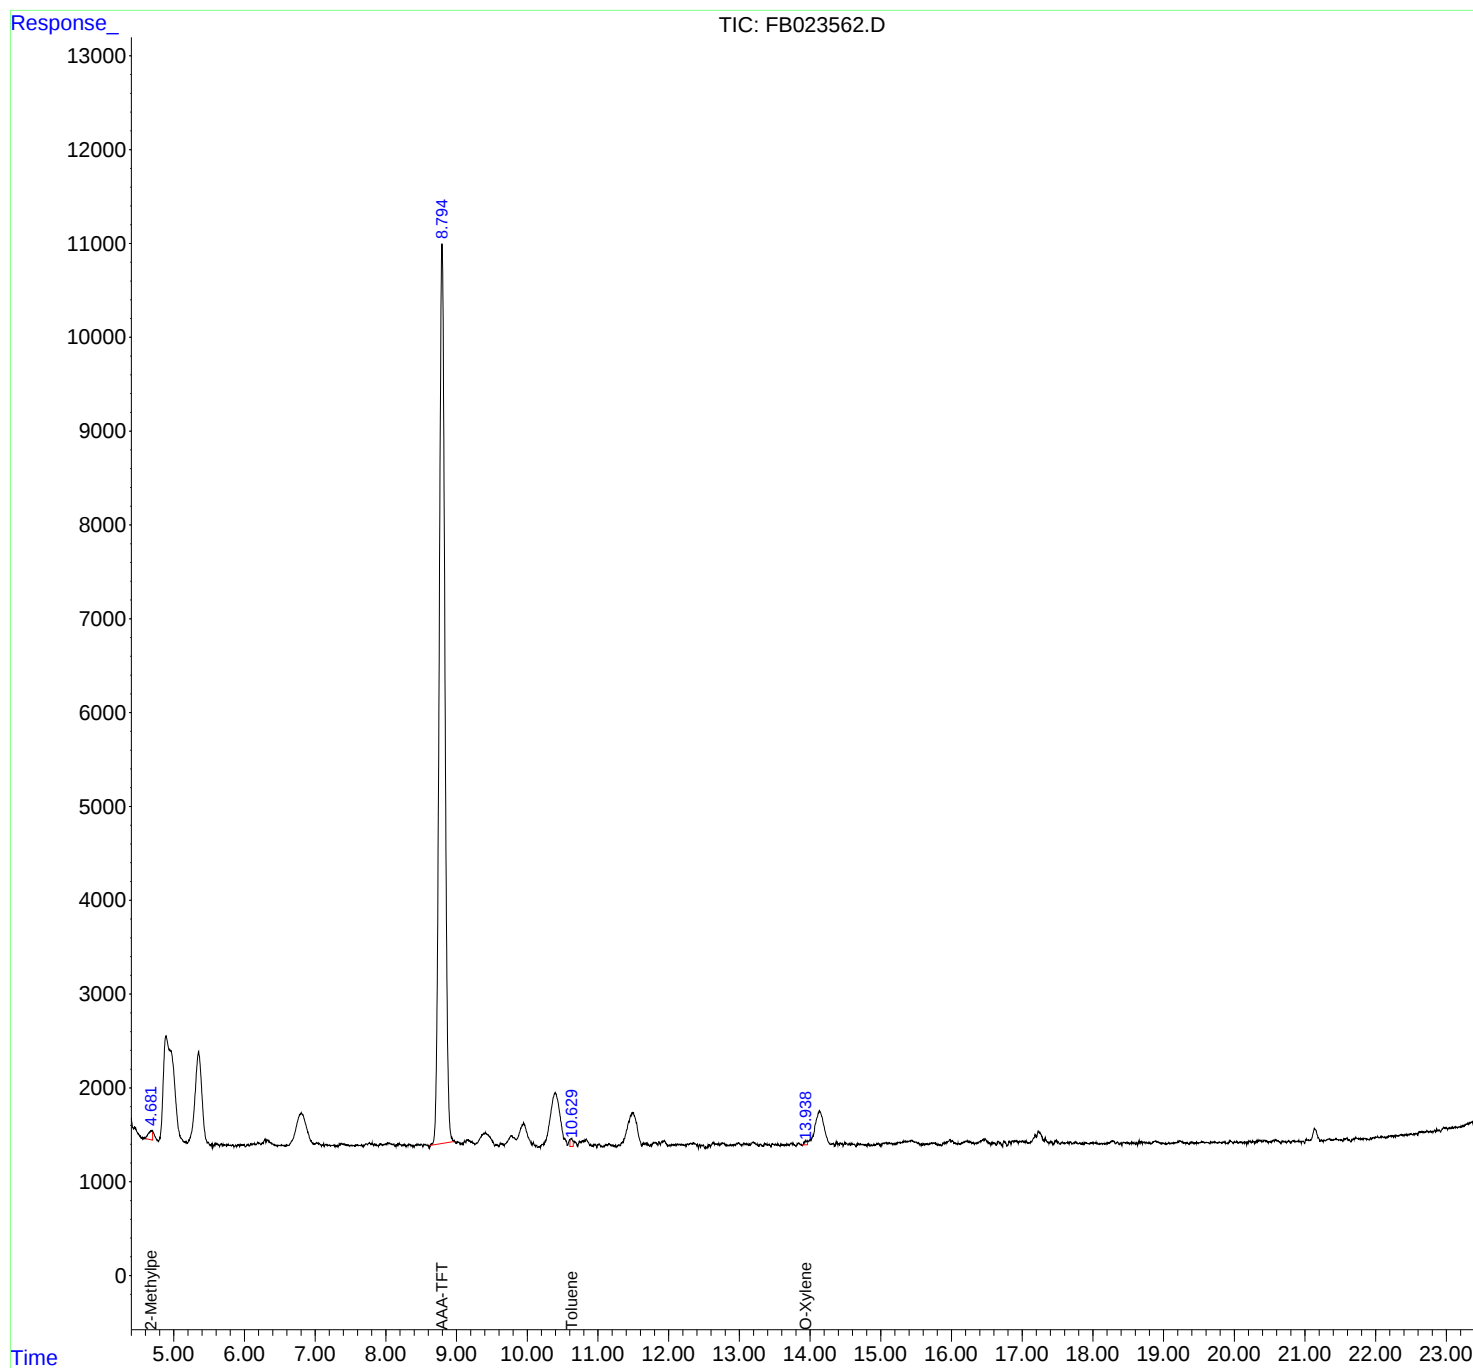

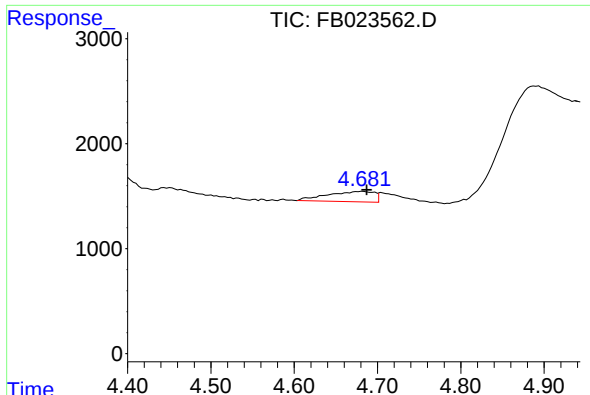


#1 2-Methylpentane

R.T.: 4.683 min  
Delta R.T.: -0.005 min  
Response: 3806  
Conc: 0.12 ng/ml

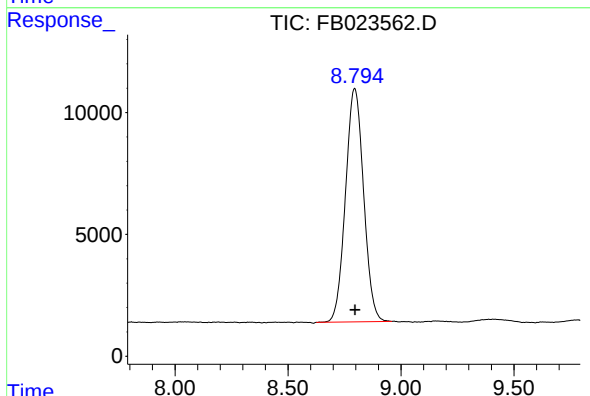


#5 AAA-TFT

R.T.: 8.796 min  
Delta R.T.: -0.001 min  
Response: 534160  
Conc: 22.49 ng/ml

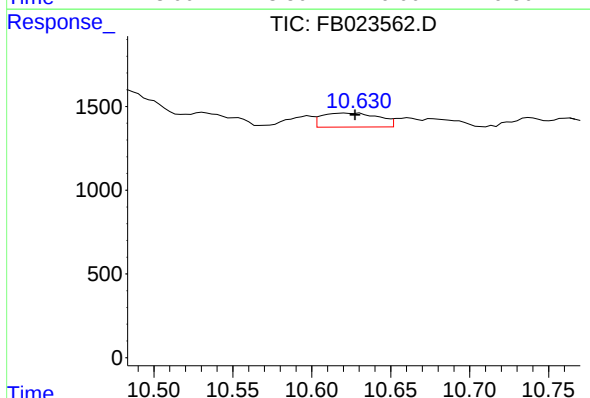

#6 Toluene

R.T.: 10.621 min  
Delta R.T.: -0.007 min  
Response: 2089  
Conc: 0.05 ng/ml

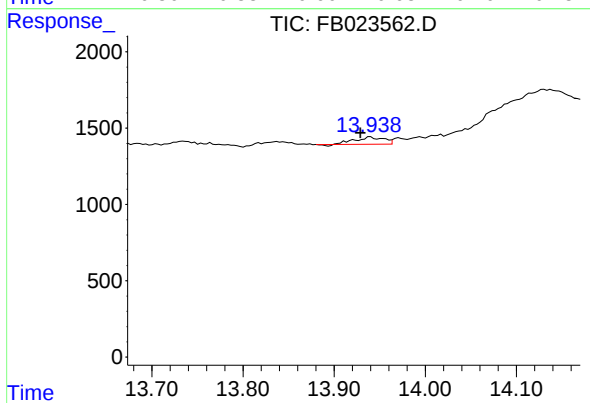

#9 O-Xylene

R.T.: 13.940 min  
Delta R.T.: 0.011 min  
Response: 1039  
Conc: 0.03 ng/ml