

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013019\
 Data File : FB019582.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2019 9:26
 Operator : MJ/SJ
 Sample : BSF0130S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 30 23:43:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.050	189909	16.246 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.900	537496	31.046 ng/ml
2) t	2,2,4-Trimethylpentane	7.664	518973	31.295 ng/ml
3) t	n-Heptane	8.004	162884	10.108 ng/ml
4) t	Benzene	8.141	181647	9.631 ng/ml
6) t	Toluene	10.896	509220	29.111 ng/ml
7) t	Ethylbenzene	13.349	210444	9.589 ng/ml
8) t	m-Xylene	13.481	444162	19.406 ng/ml
9) t	O-Xylene	14.213	436120	19.526 ng/ml
10) t	1,2,4-Trimethylbenzene	16.499	448154	19.342 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013019\
Data File : FB019582.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2019 9:26
Operator : MJ/SJ
Sample : BSF0130S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 30 23:43:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

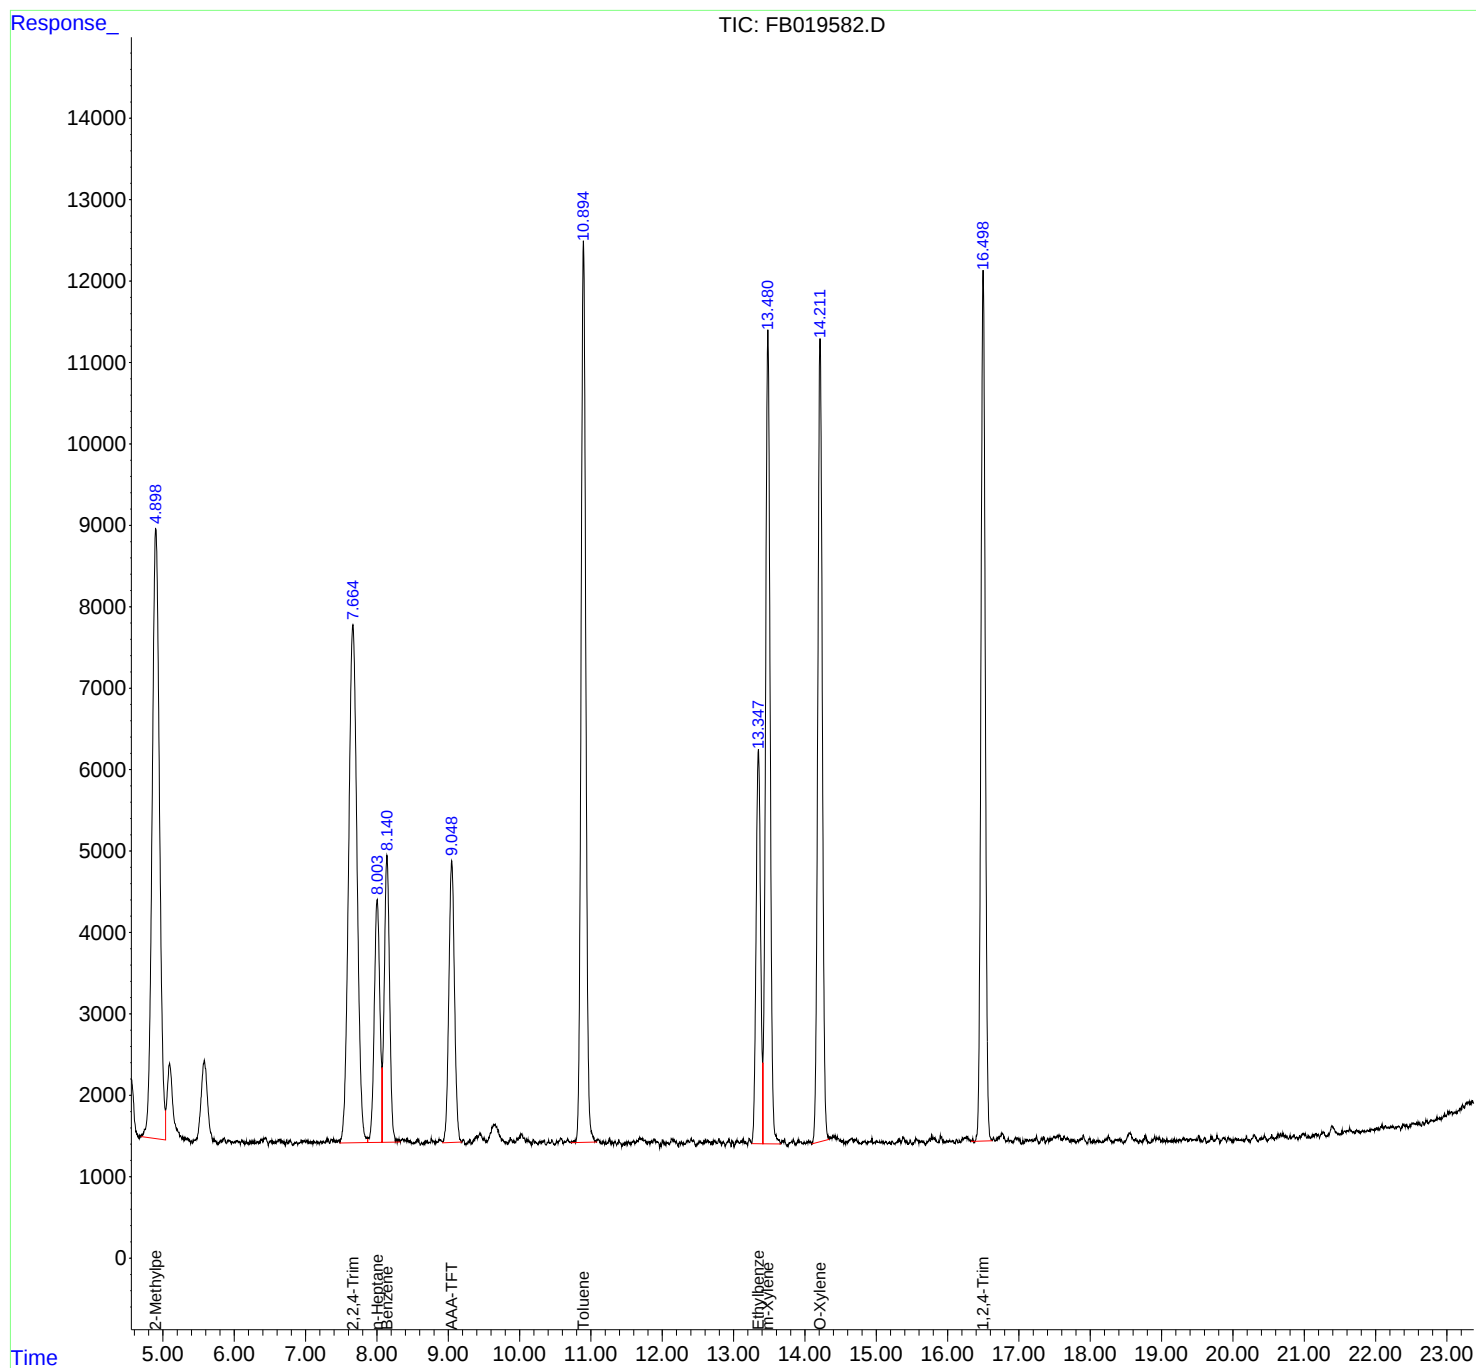

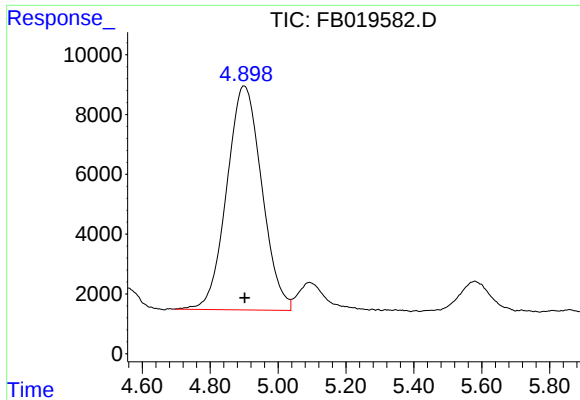


#1 2-Methylpentane

R.T.: 4.900 min
Delta R.T.: -0.002 min
Response: 537496
Conc: 31.05 ng/ml

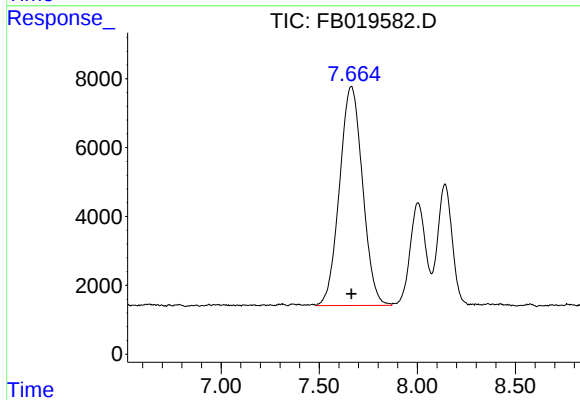


#2 2,2,4-Trimethylpentane

R.T.: 7.664 min
Delta R.T.: 0.000 min
Response: 518973
Conc: 31.29 ng/ml

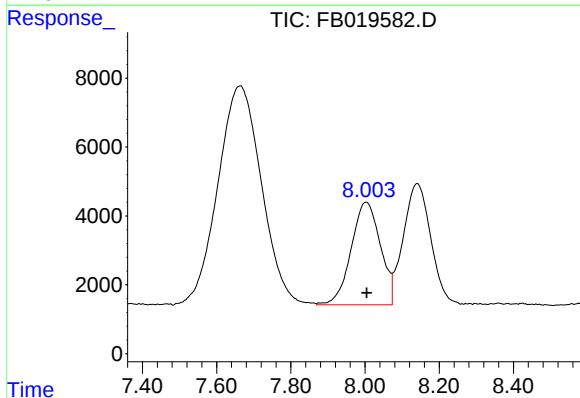


#3 n-Heptane

R.T.: 8.004 min
Delta R.T.: -0.001 min
Response: 162884
Conc: 10.11 ng/ml

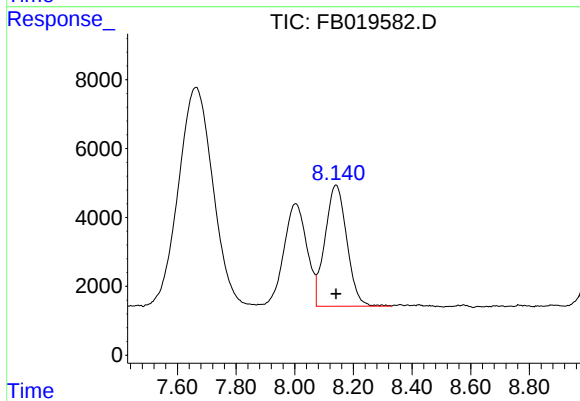


#4 Benzene

R.T.: 8.141 min
Delta R.T.: 0.000 min
Response: 181647
Conc: 9.63 ng/ml

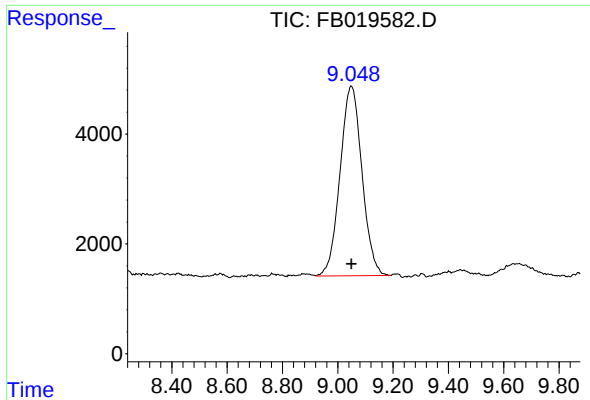


#5 AAA-TFT

R.T.: 9.050 min
Delta R.T.: 0.000 min
Response: 189909
Conc: 16.25 ng/ml

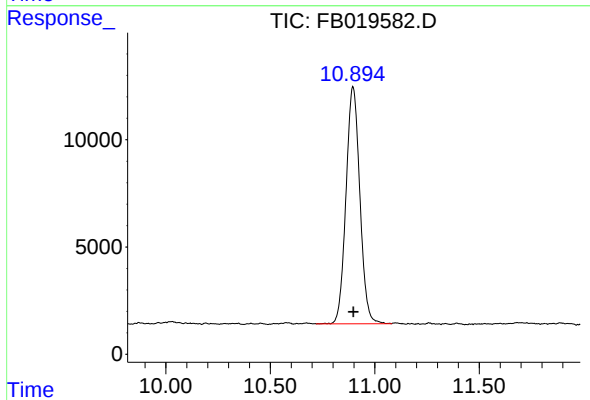


#6 Toluene

R.T.: 10.896 min
Delta R.T.: 0.000 min
Response: 509220
Conc: 29.11 ng/ml

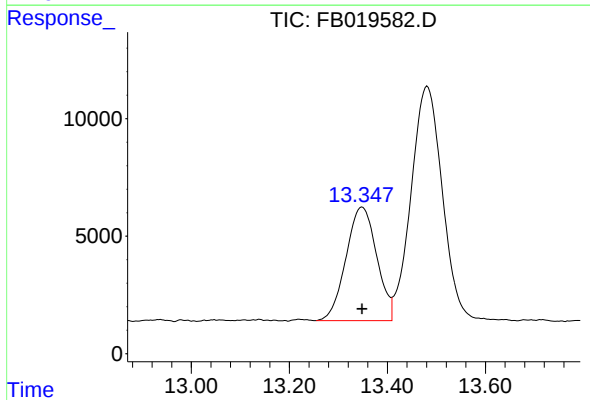


#7 Ethylbenzene

R.T.: 13.349 min
Delta R.T.: 0.000 min
Response: 210444
Conc: 9.59 ng/ml

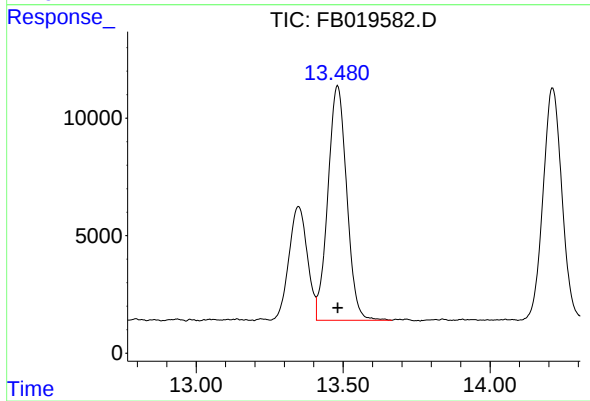

#8 m-Xylene

R.T.: 13.481 min
Delta R.T.: 0.000 min
Response: 444162
Conc: 19.41 ng/ml

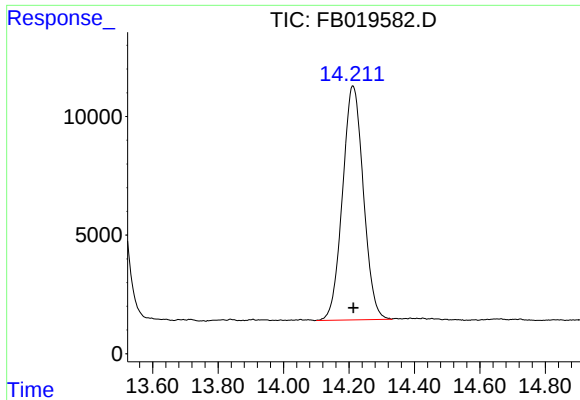


#9 O-Xylene

R.T.: 14.213 min

Delta R.T.: 0.000 min

Response: 436120

Conc: 19.53 ng/ml

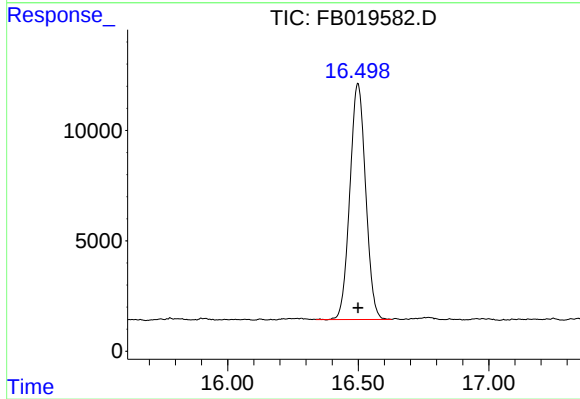

#10 1,2,4-Trimethylbenzene

R.T.: 16.499 min

Delta R.T.: 0.000 min

Response: 448154

Conc: 19.34 ng/ml